

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111922\
 Data File : VU051931.D
 Acq On : 19 Nov 2022 04:00
 Operator : JC/MD
 Sample : N5685-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW701

Quant Time: Nov 19 04:57:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 18 22:29:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	218220	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	225056	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	84449	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	107498	5.064	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	101.200%	
7) Chloroethane-d5	1.912	69	87603	5.313	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	106.200%	
11) 1,1-Dichloroethene-d2	2.568	65	38012	4.996	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	100.000%	
20) 2-Butanone-d5	4.617	46	192470	50.024	ug/L	-0.03
Spiked Amount	50.000	Range 40 - 130	Recovery	=	100.040%	
24) Chloroform-d	5.060	84	157239	5.042	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	100.800%	
26) 1,2-Dichloroethane-d4	5.700	65	85097	5.402	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	108.000%	
32) Benzene-d6	5.726	84	331057	4.955	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	99.000%	
36) 1,2-Dichloropropane-d6	6.687	67	107009	5.175	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	103.600%	
41) Toluene-d8	7.896	98	262589	4.344	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	86.800%	
43) trans-1,3-Dichloroprop...	8.176	79	34044	4.518	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	90.400%	
46) 2-Hexanone-d5	8.629	63	146724	45.948	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	91.900%	
56) 1,1,2,2-Tetrachloroeth...	10.755	84	90381	5.041	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	100.800%	
66) 1,2-Dichlorobenzene-d4	12.192	152	90288	5.584	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	111.600%	
Target Compounds						Qvalue
34) Trichloroethene	6.546	95	4518	0.247	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111922\
Data File : VU051931.D
Acq On : 19 Nov 2022 04:00
Operator : JC/MD
Sample : N5685-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW701


Quant Time: Nov 19 04:57:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 18 22:29:23 2022
Response via : Initial Calibration

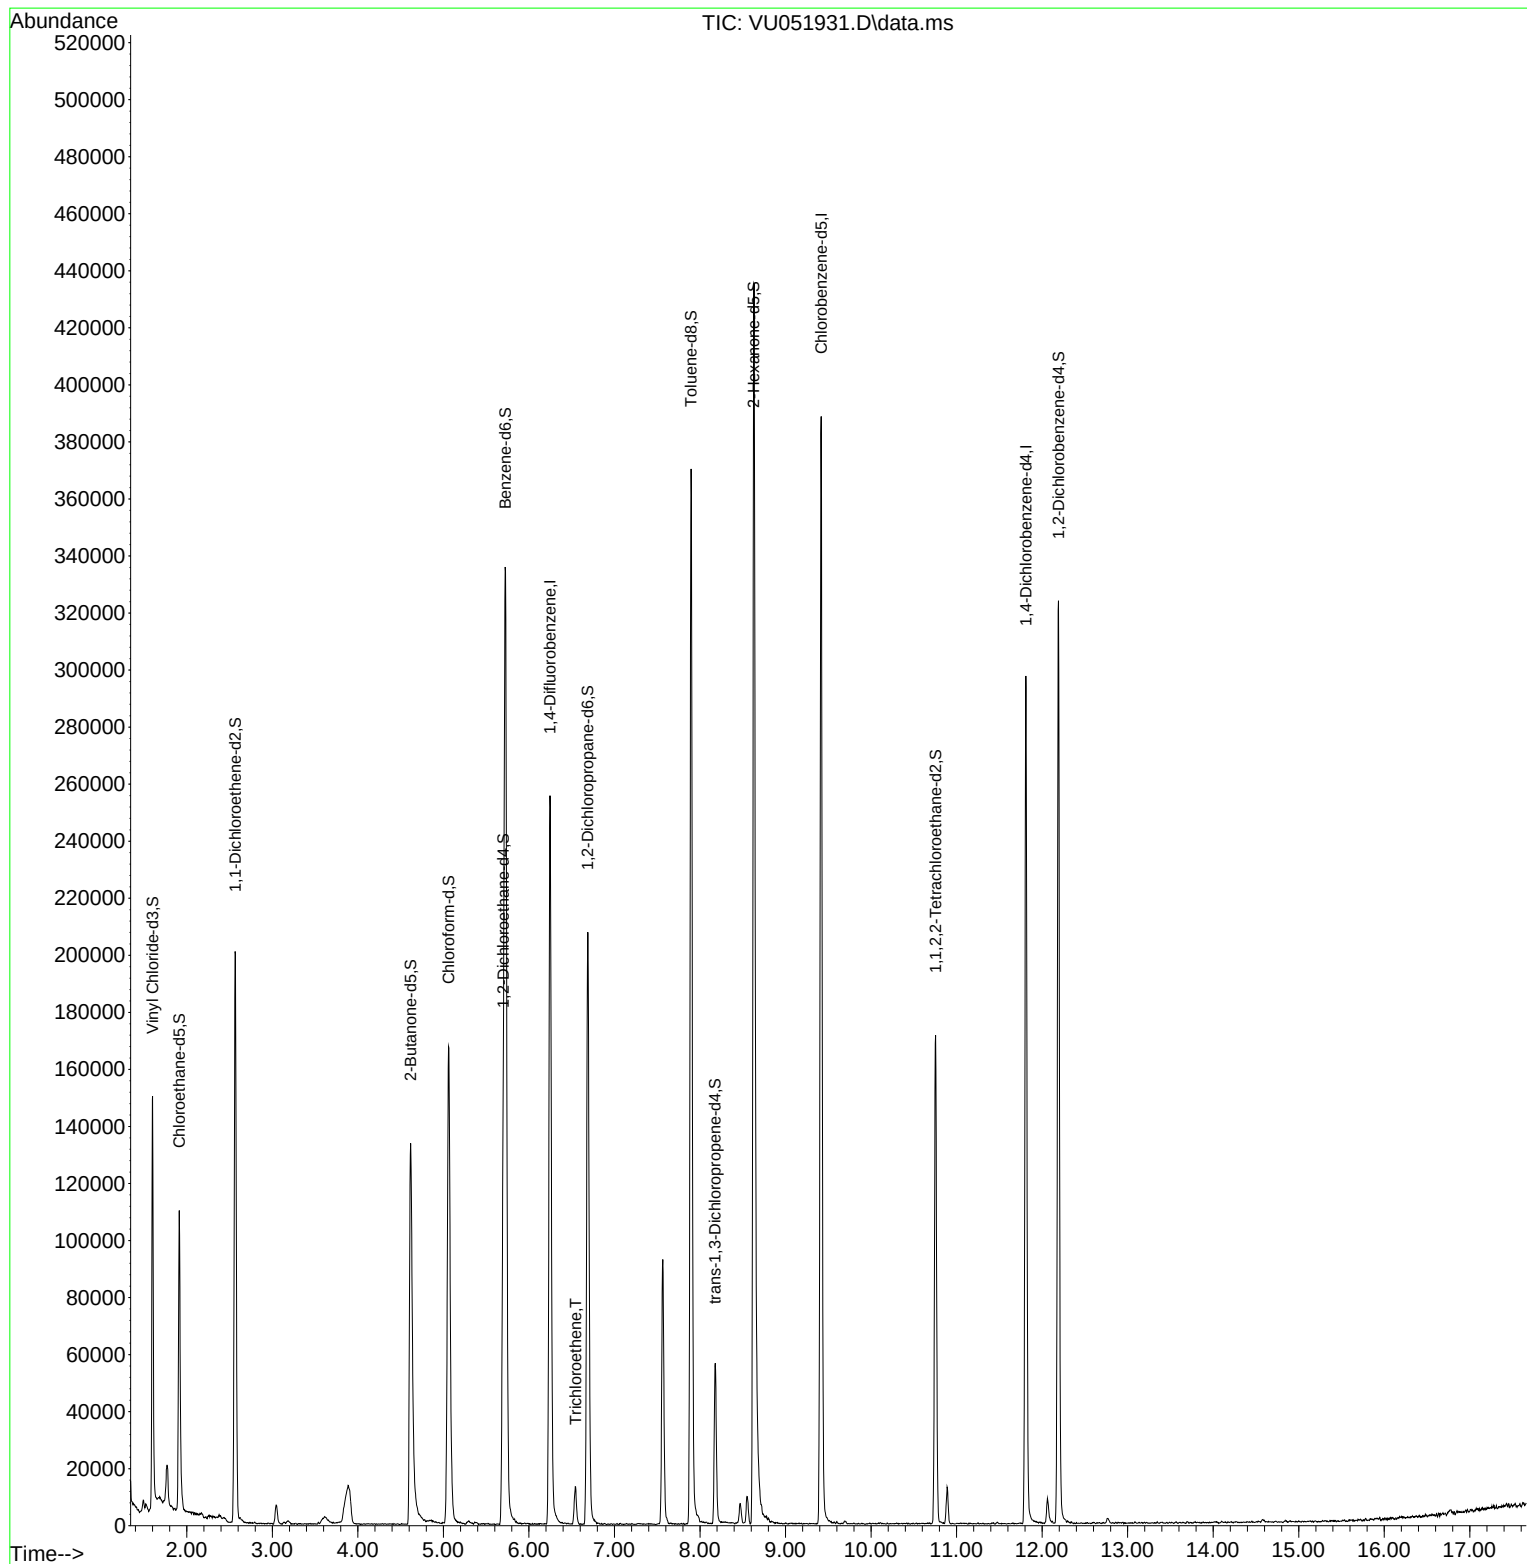

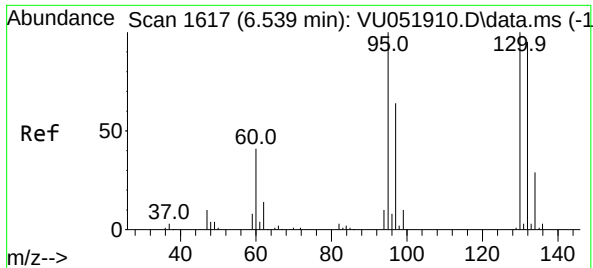

#34
 Trichloroethene
 Concen: 0.247 ug/L
 RT: 6.546 min Scan# 1
 Delta R.T. 0.006 min
 Lab File: VU051931.D
 Acq: 19 Nov 2022 04:00

Instrument :
 MSVOA_U
 ClientSampleId :
 EW701

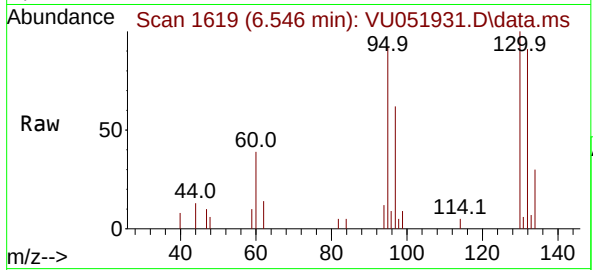

Tgt Ion:	95	Resp:	4518
Ion	Ratio	Lower	Upper
95	100		
97	66.9	43.7	81.1
132	98.6	64.3	119.3
130	108.3	67.3	124.9

