

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111922\
 Data File : VU051949.D
 Acq On : 19 Nov 2022 12:33
 Operator : JC/MD
 Sample : N5693-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBN87

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU051949.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	72	81	93	rBV	139299	170073	1.75%	0.914%
2	1.909	169	177	201	rVB	100644	149366	1.53%	0.803%
3	2.420	324	336	352	rVB2	62202	105790	1.09%	0.569%
4	2.565	368	381	390	rBV	196434	320481	3.29%	1.722%
5	2.620	390	398	424	rVB	271332	461506	4.74%	2.480%
6	3.044	516	530	555	rBV	124103	245761	2.52%	1.321%
7	4.616	1008	1019	1023	rBV2	142143	243425	2.50%	1.308%
8	4.665	1024	1034	1072	rVB	496176	1175683	12.07%	6.319%
9	5.063	1142	1158	1191	rVB	171443	422858	4.34%	2.273%
10	5.722	1343	1363	1383	rBV2	338220	880316	9.04%	4.731%
11	6.246	1513	1526	1544	rBV	261248	496013	5.09%	2.666%
12	6.539	1599	1617	1651	rBV	5274127	9737454	100.00%	52.335%
13	6.687	1652	1663	1687	rVB	217359	434695	4.46%	2.336%
14	7.565	1924	1936	1955	rBV2	94854	170880	1.75%	0.918%
15	7.896	2023	2039	2068	rBV	384980	682644	7.01%	3.669%
16	8.179	2112	2127	2145	rBV2	57013	98294	1.01%	0.528%
17	8.629	2255	2267	2299	rBV2	444721	871142	8.95%	4.682%
18	9.414	2498	2511	2534	rBV	389677	647287	6.65%	3.479%
19	10.754	2914	2928	2945	rBV	173357	282709	2.90%	1.519%
20	11.809	3245	3256	3277	rBV	291273	480994	4.94%	2.585%
21	12.192	3362	3375	3399	rBV	315111	528593	5.43%	2.841%




Sum of corrected areas: 18605964

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111922\
Data File : VU051949.D
Acq On : 19 Nov 2022 12:33
Operator : JC/MD
Sample : N5693-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBN87

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

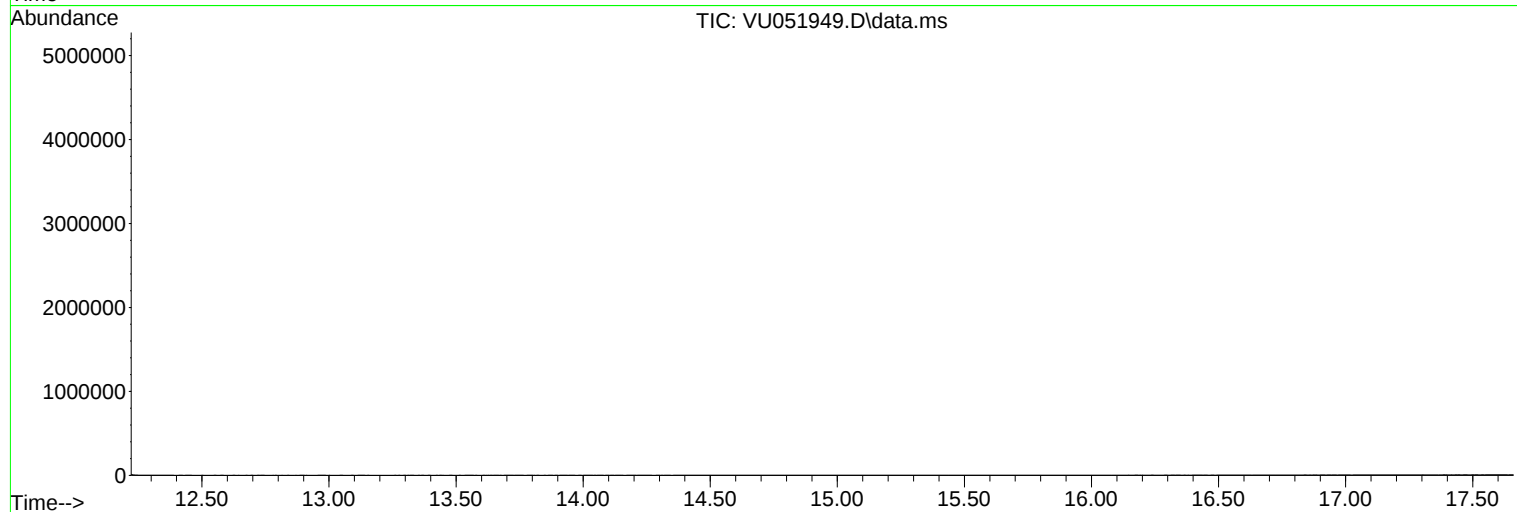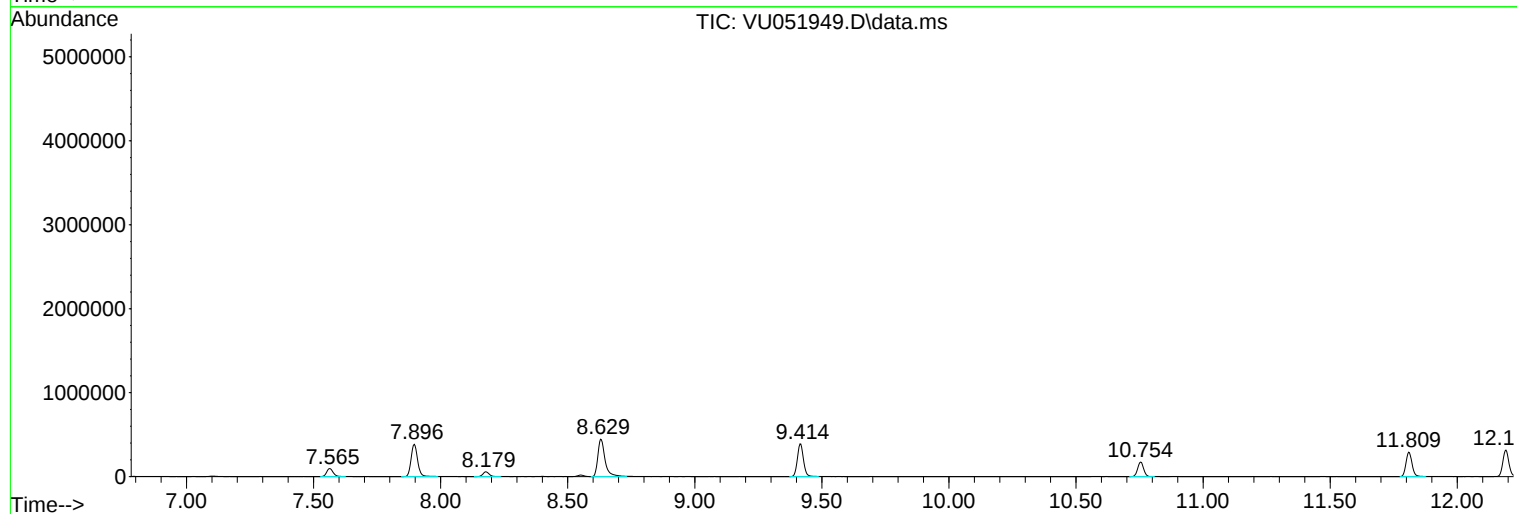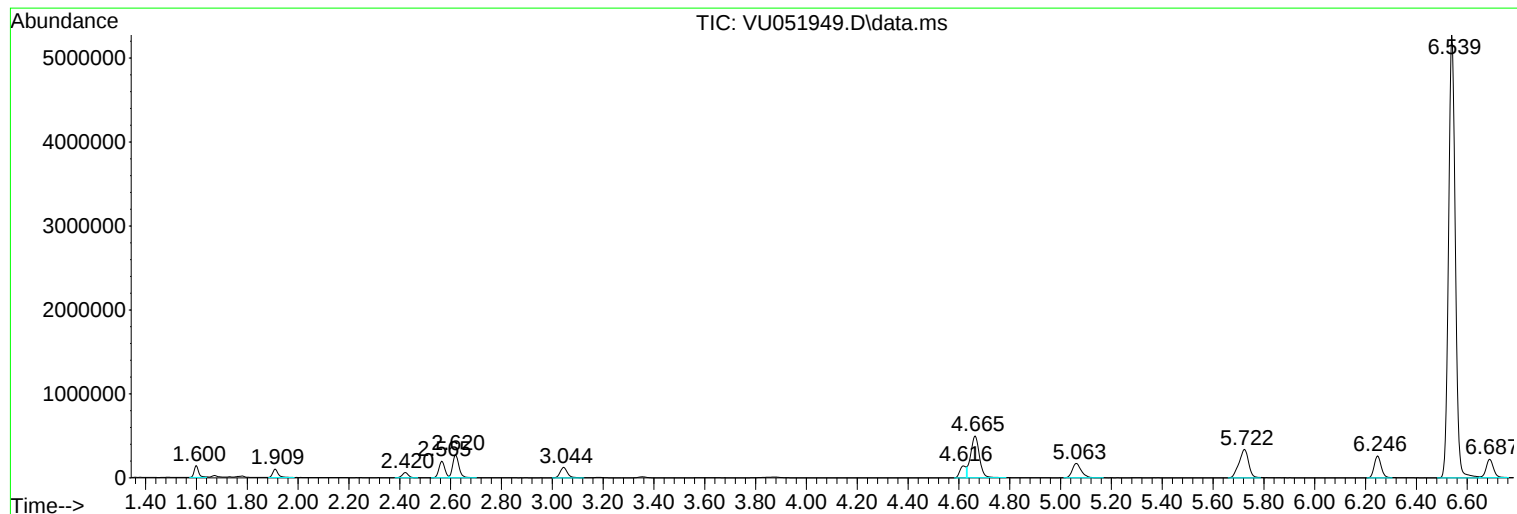

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111922\
Data File : VU051949.D
Acq On : 19 Nov 2022 12:33
Operator : JC/MD
Sample : N5693-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBN87









Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethane, 2,2-dichloro-1,1,1-... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.420	1.07 ug/L	105790	1,4-Difluorobenzene	6.246

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethane, 2,2-dichloro-1,1,1-trifl...	152	C2HCl2F3	000306-83-2	95
2			Ethane, 2,2-dichloro-1,1,1-trifl...	152	C2HCl2F3	000306-83-2	91
3			Ethane, 2,2-dichloro-1,1,1-trifl...	152	C2HCl2F3	000306-83-2	90
4			Ethane, 1,1-dichloro-2,2-difluoro-	134	C2H2Cl2F2	000471-43-2	74
5			Ethane, 1,2,2-trichloro-1,1-difl...	168	C2HCl3F2	000354-21-2	64

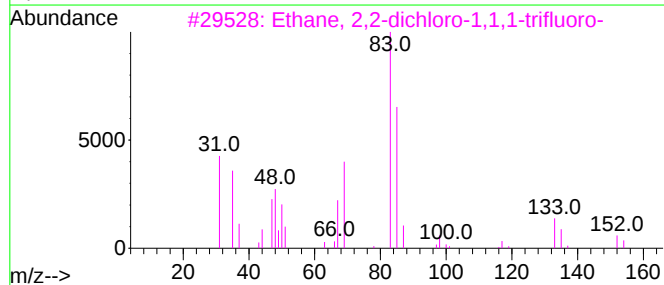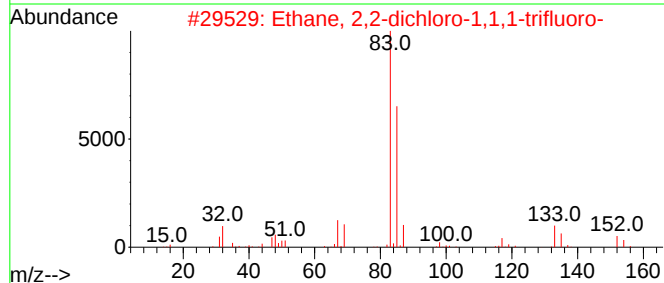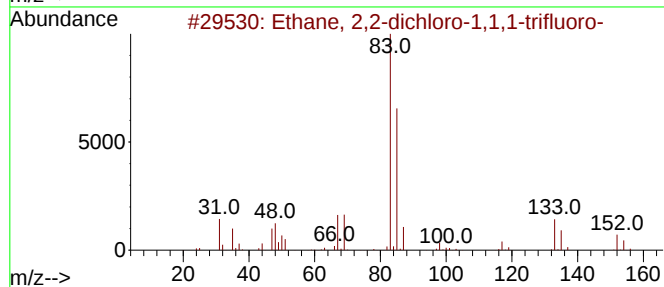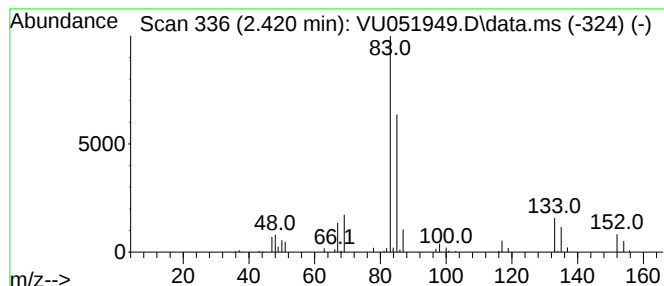

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111922\
Data File : VU051949.D
Acq On : 19 Nov 2022 12:33
Operator : JC/MD
Sample : N5693-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBN87

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethane, 2,2-dic...	2.420	1.1	ug/L	105790	1	6.246	496013	5.0