


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU112019\
 Data File : VU035781.D
 Acq On : 20 Nov 2019 10:59
 Operator : JC/SP
 Sample : BFB31
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB31

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
 Title : VOC Analysis
 Last Update : Thu Nov 21 04:09:14 2019

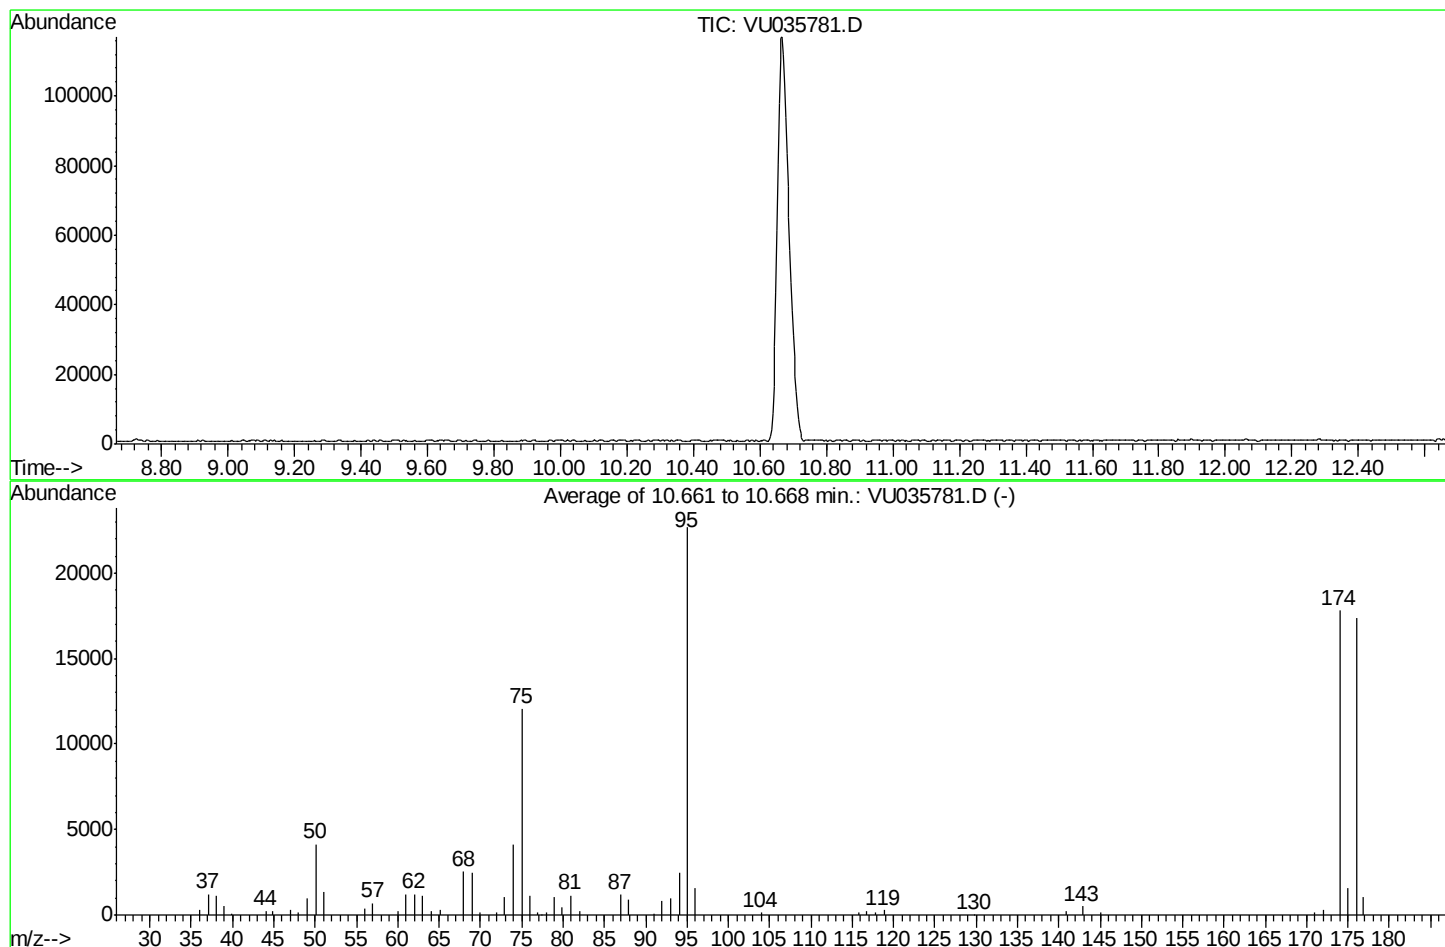

AutoFind: Scans 2899, 2900, 2901; Background Corrected with Scan 2888

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	4154	PASS
75	95	30	80	53.2	12077	PASS
95	95	100	100	100.0	22680	PASS
96	95	5	9	7.0	1583	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.6	17818	PASS
175	174	5	9	9.0	1602	PASS
176	174	95	101	97.4	17354	PASS
177	176	5	9	6.2	1071	PASS

m/z	Abundance
35.90	201.0
37.00	1146.0
38.00	1135.0
39.00	425.0
40.00	282.0
44.00	851.0
44.90	235.0
47.00	363.0
47.90	142.0
49.00	918.0
50.10	3999.0
51.00	1391.0
55.90	418.0
57.00	588.0
60.00	286.0
60.90	990.0
62.00	1034.0
63.00	1165.0
64.00	225.0
65.10	236.0
68.00	2377.0
69.00	2372.0
70.00	111.0
72.00	140.0
72.90	1046.0
74.00	3926.0
75.00	12021.0
76.00	1146.0
76.90	143.0
78.10	153.0
78.90	982.0
79.90	355.0
80.90	1157.0
82.00	217.0
86.90	1384.0
87.90	816.0
91.90	804.0
93.10	908.0
94.10	2355.0
95.00	21920.0
96.00	1530.0
104.00	145.0
115.90	112.0
116.80	258.0
117.80	126.0
118.90	232.0
140.90	284.0
142.90	524.0
145.00	150.0
170.90	167.0
172.00	342.0
174.00	16832.0
175.00	1493.0
176.00	16800.0
176.90	943.0

Instrument :
MSVOA_U
ClientSampleId :
BFB31

m/z	Abundance
36.00	266.0
37.00	1256.0
38.00	1122.0
39.00	509.0
40.00	297.0
44.00	835.0
44.90	189.0
47.00	335.0
47.90	121.0
49.00	978.0
50.10	4184.0
51.00	1408.0
56.00	411.0
57.00	706.0
60.10	266.0
61.00	1195.0
62.00	1236.0
63.00	1165.0
64.00	242.0
65.10	256.0
68.00	2588.0
69.00	2537.0
70.00	135.0
72.00	159.0
72.90	1060.0
74.00	4211.0
75.00	12329.0
76.00	1205.0
76.90	188.0
78.10	168.0
78.90	1058.0
79.90	447.0
80.90	1181.0
82.00	229.0
86.90	1221.0
87.90	898.0
91.00	138.0
92.00	872.0
93.00	954.0
94.00	2463.0
95.00	23216.0
96.00	1621.0
104.00	144.0
115.80	138.0
116.80	245.0
117.80	138.0
118.90	270.0
140.90	232.0
142.90	517.0
145.00	146.0
170.90	195.0
172.00	329.0
174.00	18032.0
175.00	1667.0
176.00	17608.0
176.90	1107.0

Instrument :
MSVOA_U
ClientSampleId :
BFB31

m/z	Abundance
36.00	329.0
37.10	1255.0
38.00	1011.0
39.00	614.0
40.00	303.0
44.00	861.0
44.90	207.0
47.00	314.0
47.90	126.0
49.00	1047.0
50.10	4280.0
51.00	1345.0
56.00	404.0
57.00	735.0
60.10	239.0
61.00	1326.0
62.00	1418.0
63.00	1050.0
64.10	223.0
65.10	311.0
68.00	2577.0
69.00	2451.0
70.00	174.0
72.00	150.0
72.90	1102.0
74.00	4261.0
75.00	11882.0
76.00	1139.0
76.90	197.0
77.40	100.0
78.00	161.0
78.90	1142.0
79.90	457.0
80.90	1090.0
82.00	172.0
87.00	976.0
88.00	955.0
91.00	161.0
92.00	836.0
93.00	1057.0
94.00	2609.0
95.00	22904.0
96.00	1599.0
104.00	114.0
115.80	123.0
116.70	231.0
117.80	161.0
118.80	314.0
129.80	106.0
140.90	217.0
142.90	473.0
145.00	108.0
170.90	159.0
171.90	318.0
174.00	18592.0
175.00	1647.0
176.00	17656.0
176.90	1165.0

Instrument :
MSVOA_U
ClientSampleId :
BFB31

Scan 2888 (10.626 min): VU035781.D
BFB31

m/z	Abundance
39.90	252.0
44.00	594.0

Instrument :
MSVOA_U
ClientSampleId :
BFB31