


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU112020\
 Data File : VU041357.D
 Acq On : 20 Nov 2020 08:42
 Operator : SY/MD
 Sample : BFB16
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB16

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR111620WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat Nov 21 02:42:19 2020

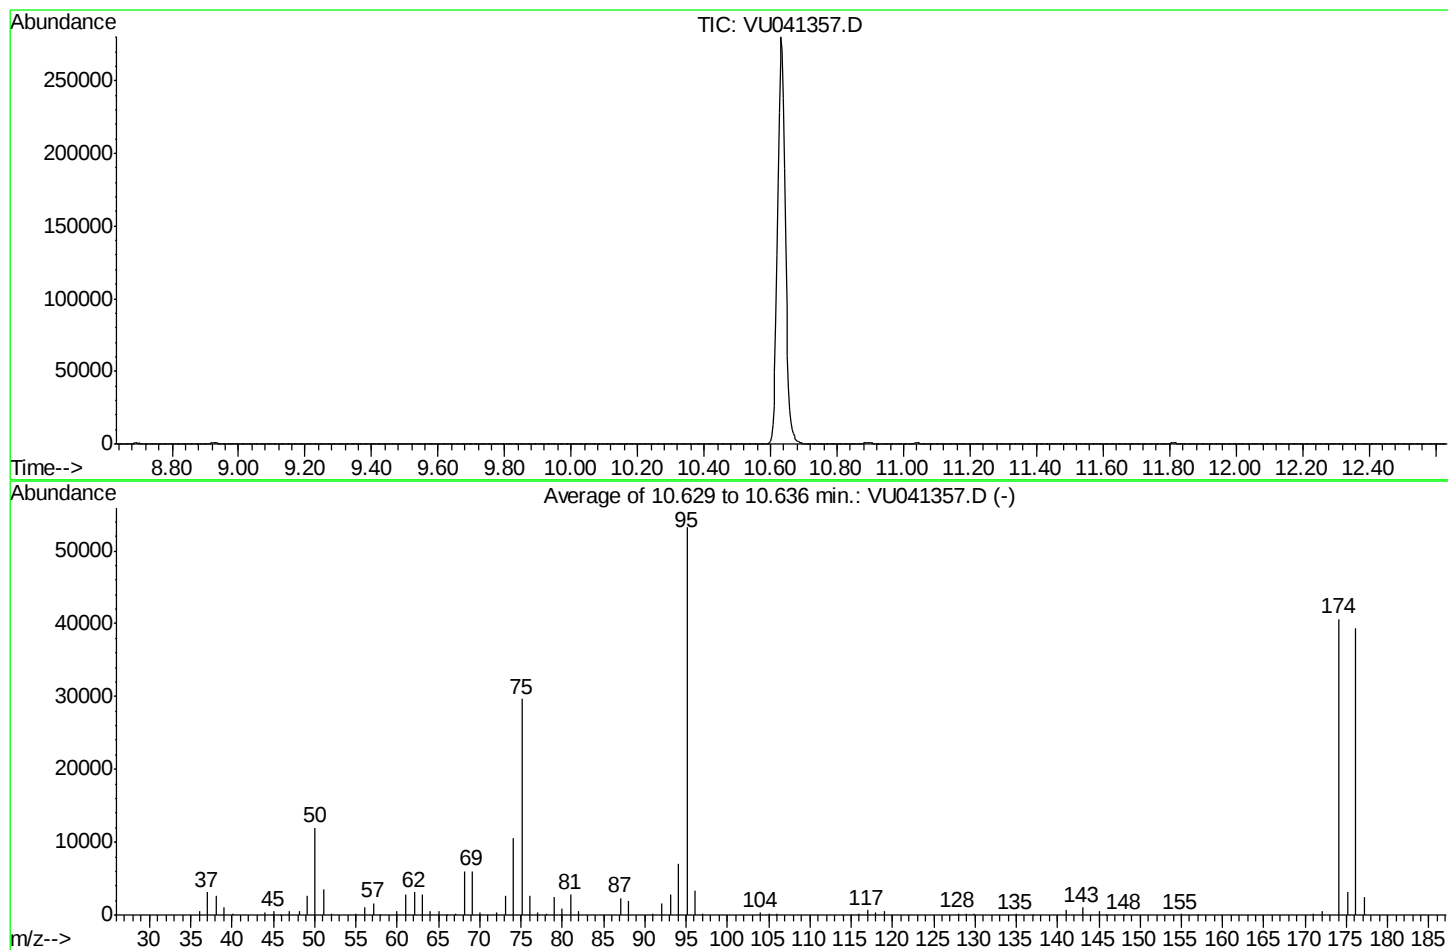

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.5	11968	PASS
75	95	30	80	55.7	29650	PASS
95	95	100	100	100.0	53226	PASS
96	95	5	9	6.2	3313	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.4	40650	PASS
175	174	5	9	7.9	3207	PASS
176	174	95	101	96.9	39392	PASS
177	176	5	9	6.1	2404	PASS

m/z	Abundance
36.00	584.0
37.00	2957.0
38.00	2684.0
39.00	1041.0
40.00	110.0
44.00	487.0
45.10	568.0
45.90	104.0
47.00	580.0
48.10	430.0
49.00	2576.0
50.10	11722.0
51.10	3476.0
52.00	196.0
55.00	143.0
56.00	980.0
57.10	1619.0
57.90	116.0
60.00	491.0
61.10	2723.0
62.10	3018.0
63.10	2711.0
64.10	563.0
65.00	525.0
66.00	106.0
67.10	165.0
68.10	5926.0
69.10	6045.0
70.10	397.0
72.00	386.0
73.10	2580.0
74.10	10361.0
75.10	29048.0
76.10	2753.0
77.10	385.0
78.10	246.0
79.00	2552.0
80.00	754.0
81.00	2841.0
82.00	583.0
87.10	2490.0
88.00	2034.0
91.00	230.0
92.10	1588.0
93.10	2789.0
94.10	6724.0
95.10	51848.0
96.10	3364.0
97.00	145.0
104.00	296.0
105.10	102.0
106.00	211.0
115.00	117.0
116.00	150.0
117.00	619.0
117.90	271.0
119.00	490.0
128.00	162.0
129.00	119.0
130.00	143.0
135.00	104.0
137.00	116.0
141.00	786.0
143.00	1024.0
145.00	425.0
145.90	130.0
148.10	123.0
155.00	119.0
171.00	190.0
172.00	454.0
174.10	38400.0
175.10	3171.0
176.10	37640.0
177.10	2304.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16

m/z	Abundance
36.00	628.0
37.00	3263.0
38.00	2651.0
39.00	1137.0
40.10	118.0
44.00	498.0
45.10	514.0
47.00	620.0
48.10	495.0
49.00	2678.0
50.10	12440.0
51.10	3531.0
52.00	181.0
54.90	164.0
56.00	1043.0
57.10	1678.0
60.00	539.0
61.10	2895.0
62.10	3215.0
63.10	2811.0
64.00	579.0
65.00	585.0
67.10	210.0
68.10	6168.0
69.10	6223.0
70.10	437.0
72.00	404.0
73.10	2771.0
74.10	10926.0
75.10	30408.0
76.10	2718.0
77.10	443.0
78.10	249.0
79.00	2568.0
80.00	815.0
81.00	2881.0
81.90	639.0
87.10	2423.0
88.00	2085.0
91.00	248.0
92.10	1723.0
93.10	2945.0
94.10	7353.0
95.10	54912.0
96.10	3373.0
97.00	142.0
104.00	325.0
105.10	114.0
106.00	262.0
115.00	115.0
116.00	146.0
117.00	674.0
118.00	269.0
118.90	484.0
128.00	181.0
128.90	123.0
129.90	172.0
135.00	130.0
137.00	106.0
141.00	769.0
143.00	1038.0
145.00	466.0
145.90	148.0
148.00	105.0
155.00	144.0
157.10	123.0
171.00	148.0
172.10	510.0
174.10	41832.0
175.10	3352.0
176.10	40616.0
177.10	2467.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16

m/z	Abundance
36.00	568.0
37.00	3192.0
38.10	2506.0
39.00	1178.0
40.00	113.0
44.00	469.0
45.00	428.0
47.00	609.0
48.10	428.0
49.10	2495.0
50.10	11744.0
51.10	3399.0
52.00	145.0
54.90	183.0
56.00	944.0
57.10	1629.0
60.00	544.0
61.10	2870.0
62.10	3157.0
63.10	2716.0
64.00	530.0
65.10	577.0
67.10	222.0
68.10	5884.0
69.10	5917.0
70.10	420.0
72.00	391.0
73.10	2750.0
74.10	10547.0
75.10	29496.0
76.10	2458.0
77.00	418.0
78.00	237.0
79.00	2418.0
80.00	842.0
81.00	2692.0
81.90	613.0
87.00	2145.0
88.10	1943.0
90.90	230.0
92.10	1687.0
93.10	2761.0
94.10	7145.0
95.10	52920.0
96.10	3203.0
97.00	111.0
104.00	328.0
105.10	104.0
106.00	298.0
116.00	165.0
116.90	583.0
118.00	274.0
119.00	456.0
128.00	201.0
128.90	138.0
129.90	186.0
134.90	124.0
141.00	679.0
143.00	974.0
145.00	452.0
154.90	153.0
157.00	139.0
170.90	109.0
172.10	540.0
174.10	41720.0
175.10	3098.0
176.10	39920.0
177.10	2441.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16

m/z	Abundance
44.00	146.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16