

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112023\
 Data File : VU056519.D
 Acq On : 20 Nov 2023 10:29
 Operator : MD/SY
 Sample : VU1120WBL01
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK081

Quant Time: Nov 21 00:39:19 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 21 00:36:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	281957	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	262471	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.810	152	119517	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	121814	5.776	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	115.600%
7) Chloroethane-d5	1.911	69	79880	4.940	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.800%
11) 1,1-Dichloroethene-d2	2.563	65	50725	5.450	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	109.000%
20) 2-Butanone-d5	4.621	46	200039	47.569	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.140%
24) Chloroform-d	5.058	84	205153	5.029	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.600%
26) 1,2-Dichloroethane-d4	5.698	65	96746	5.133	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.600%
32) Benzene-d6	5.724	84	415493	5.313	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.200%
36) 1,2-Dichloropropane-d6	6.685	67	125820	5.338	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	106.800%
41) Toluene-d8	7.894	98	367243	5.318	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.400%
43) trans-1,3-Dichloroprop...	8.177	79	47846	5.293	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	105.800%
46) 2-Hexanone-d5	8.631	63	168605	47.465	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.920%
56) 1,1,2,2-Tetrachloroeth...	10.753	84	83134	4.936	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.800%
66) 1,2-Dichlorobenzene-d4	12.190	152	120264	5.447	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.000%
Target Compounds						Qvalue
16) Methylene chloride	3.042	84	20326	0.890	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112023\
Data File : VU056519.D
Acq On : 20 Nov 2023 10:29
Operator : MD/SY
Sample : VU1120WBL01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK081


Quant Time: Nov 21 00:39:19 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 21 00:36:07 2023
Response via : Initial Calibration

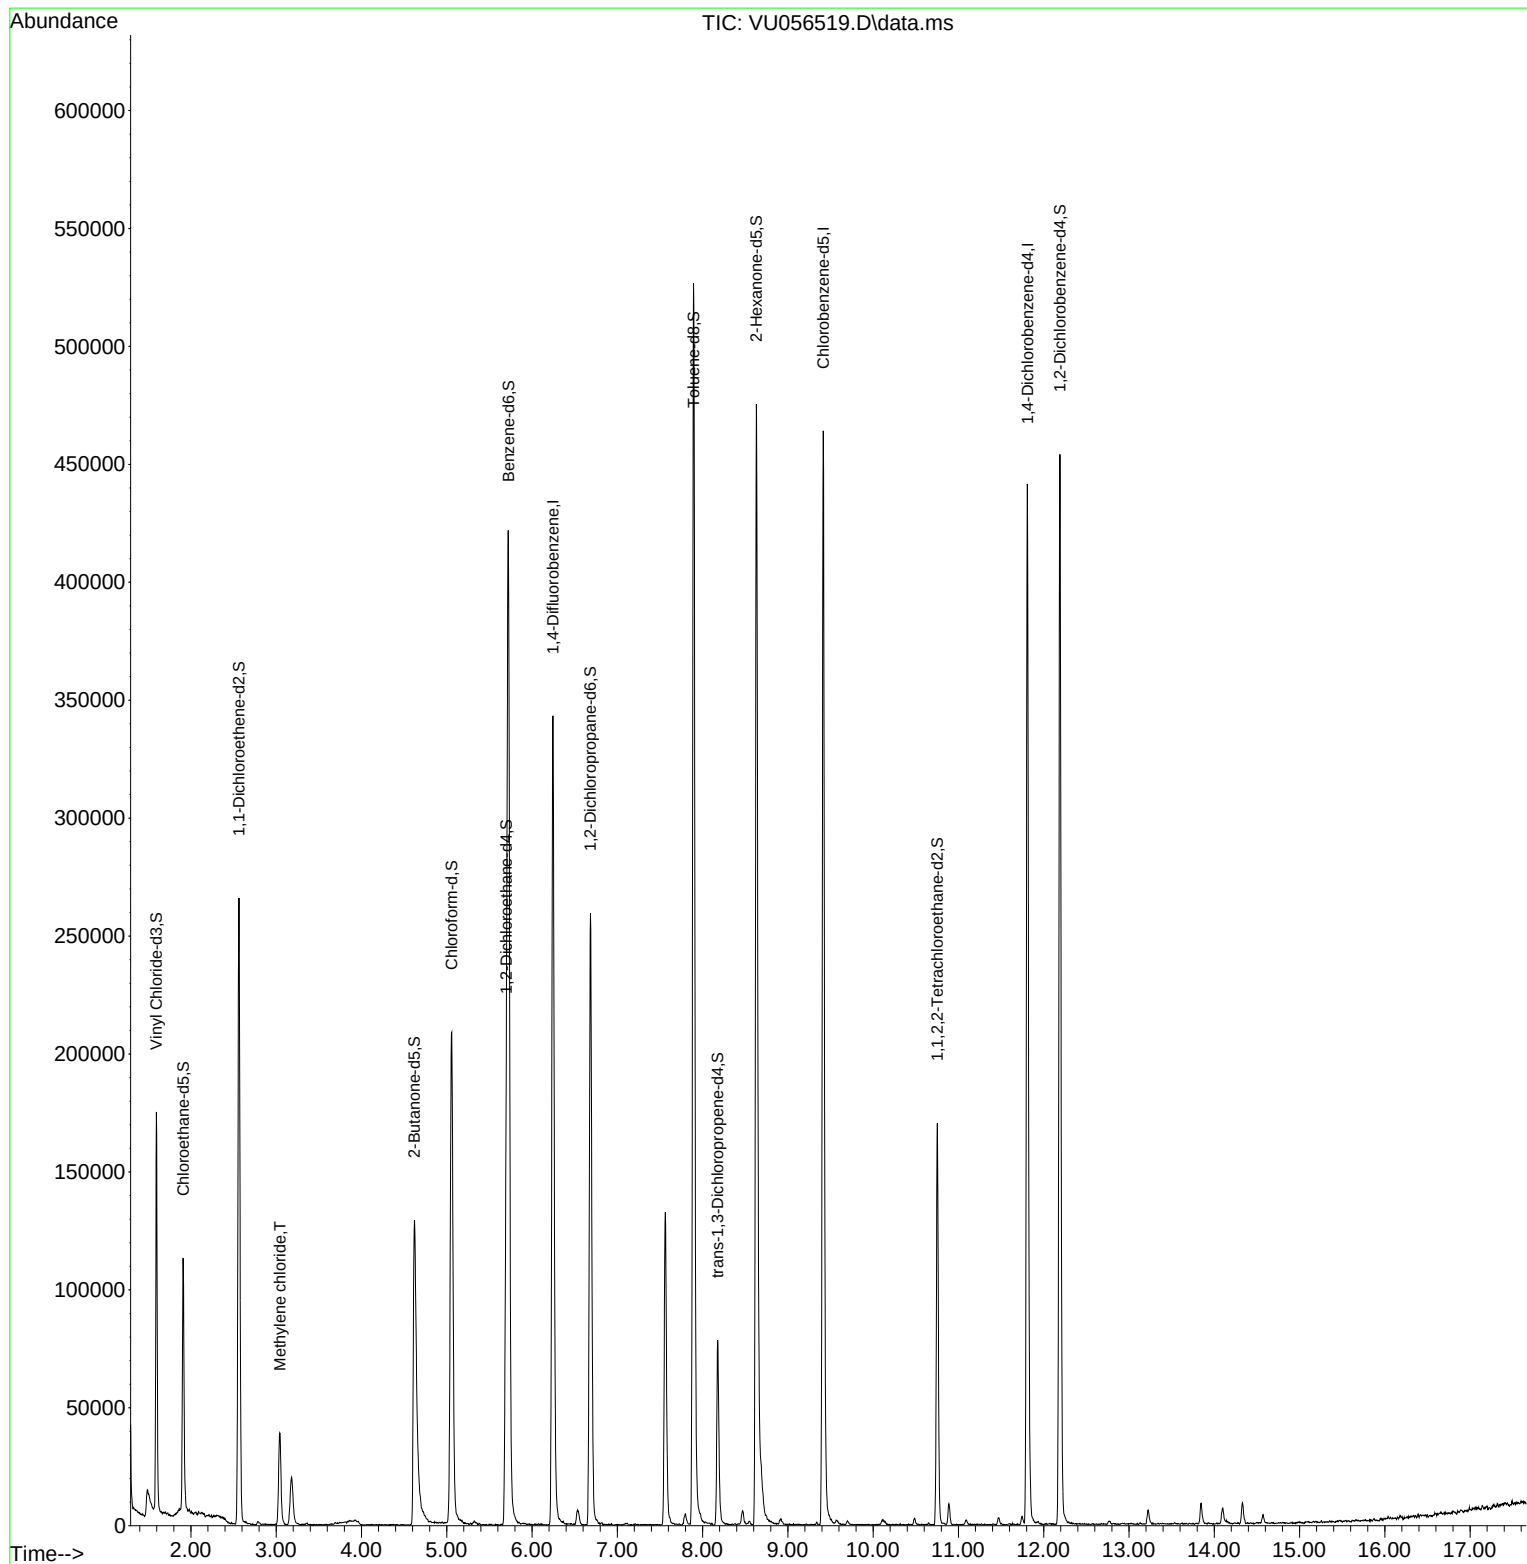

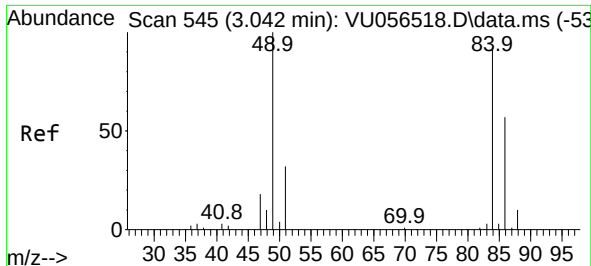

#16
Methylene chloride
Concen: 0.890 ug/L
RT: 3.042 min Scan# 54
Delta R.T. 0.000 min
Lab File: VU056519.D
Acq: 20 Nov 2023 10:29

Instrument :
MSVOA_U
ClientSampleId :
VBLK081

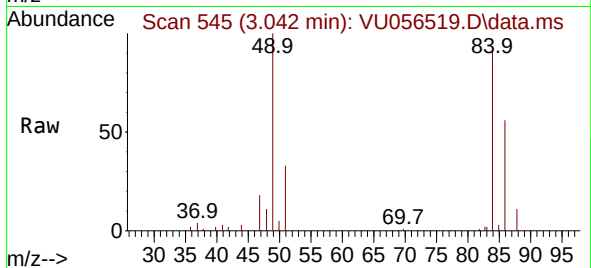

Tgt Ion: 84 Resp: 20326
Ion Ratio Lower Upper
84 100
86 61.3 44.7 83.1
49 110.4 81.8 152.0

