

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112025\
 Data File : VU063750.D
 Acq On : 20 Nov 2025 09:51
 Operator : MD/SY
 Sample : VU1120WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK169

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111925WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU063750.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.583	83	91	103	rBV	124242	138165	14.15%	2.002%
2	1.895	179	188	206	rVB	107087	141488	14.49%	2.050%
3	2.541	377	389	408	rBV	200250	332691	34.08%	4.821%
4	4.596	1019	1028	1058	rBV	83036	242335	24.82%	3.511%
5	5.030	1148	1163	1189	rBV	177805	418546	42.87%	6.065%
6	5.695	1351	1370	1410	rBV2	345762	976254	100.00%	14.146%
7	6.222	1520	1534	1569	rBV	174605	372516	38.16%	5.398%
8	6.660	1657	1670	1698	rBV	213522	450285	46.12%	6.524%
9	7.541	1931	1944	1969	rBV2	94630	181264	18.57%	2.626%
10	7.872	2034	2047	2086	rBV	453025	866682	88.78%	12.558%
11	8.155	2125	2135	2158	rBV	49256	94027	9.63%	1.362%
12	8.615	2267	2278	2328	rBV2	238291	656296	67.23%	9.510%
13	9.393	2507	2520	2563	rBV	269578	497362	50.95%	7.207%
14	10.730	2923	2936	2955	rBV	144985	243050	24.90%	3.522%
15	11.788	3254	3265	3287	rBV	329040	574545	58.85%	8.325%
16	12.168	3368	3383	3410	rBV	392604	670059	68.64%	9.709%
17	13.820	3888	3897	3913	rBV4	10001	16873	1.73%	0.244%
18	14.071	3964	3975	3986	rBV2	7873	14076	1.44%	0.204%
19	14.306	4038	4048	4062	rVB4	8228	14946	1.53%	0.217%




Sum of corrected areas: 6901460

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112025\
Data File : VU063750.D
Acq On : 20 Nov 2025 09:51
Operator : MD/SY
Sample : VU1120WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK169

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111925WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

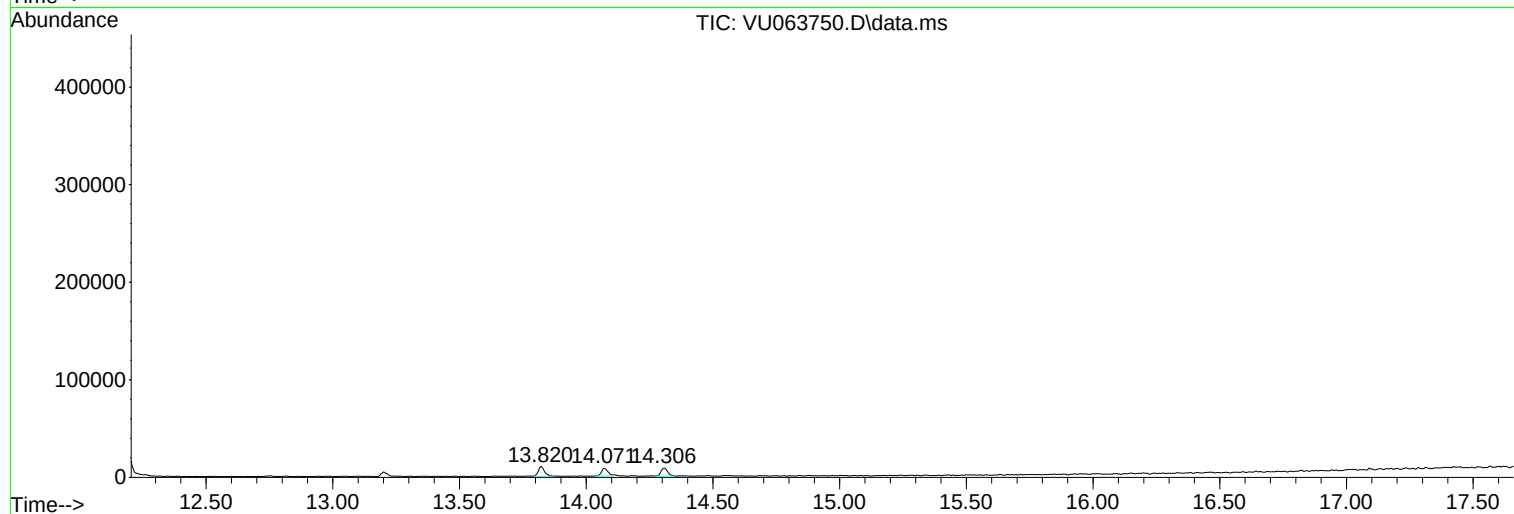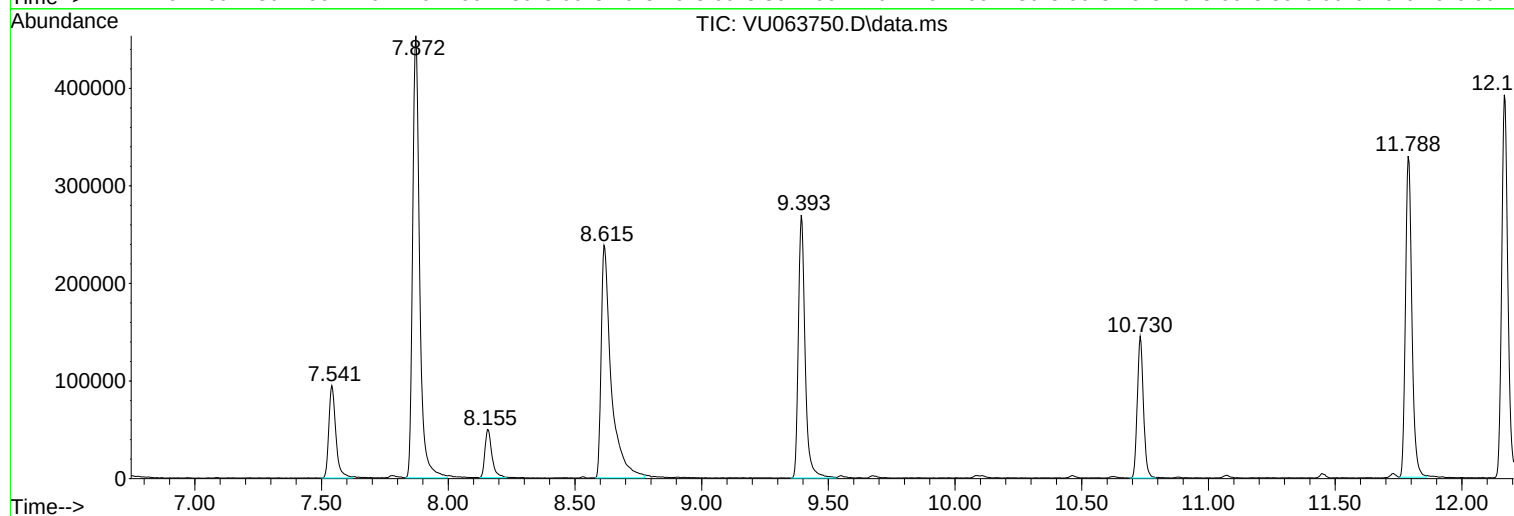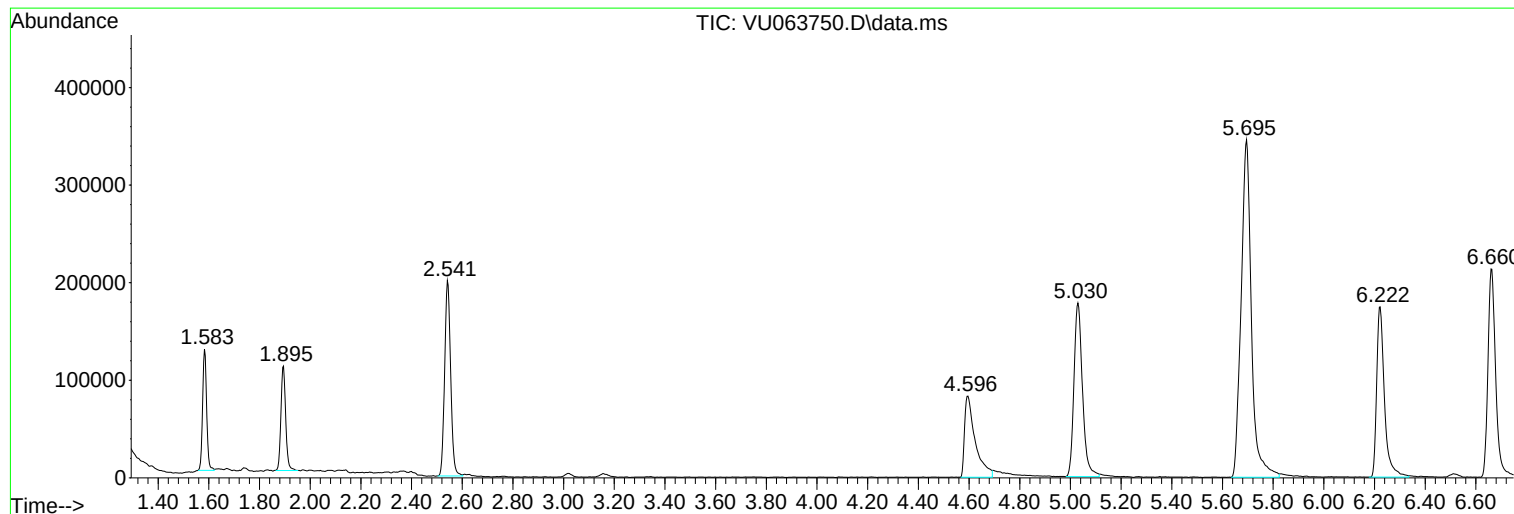

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112025\
Data File : VU063750.D
Acq On : 20 Nov 2025 09:51
Operator : MD/SY
Sample : VU1120WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK169

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111925WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112025\
Data File : VU063750.D
Acq On : 20 Nov 2025 09:51
Operator : MD/SY
Sample : VU1120WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK169

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111925WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc