


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112025\
Data File : VU063748.D
Acq On : 20 Nov 2025 08:04
Operator : MD/SY
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB087

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111925WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Nov 21 04:14:42 2025

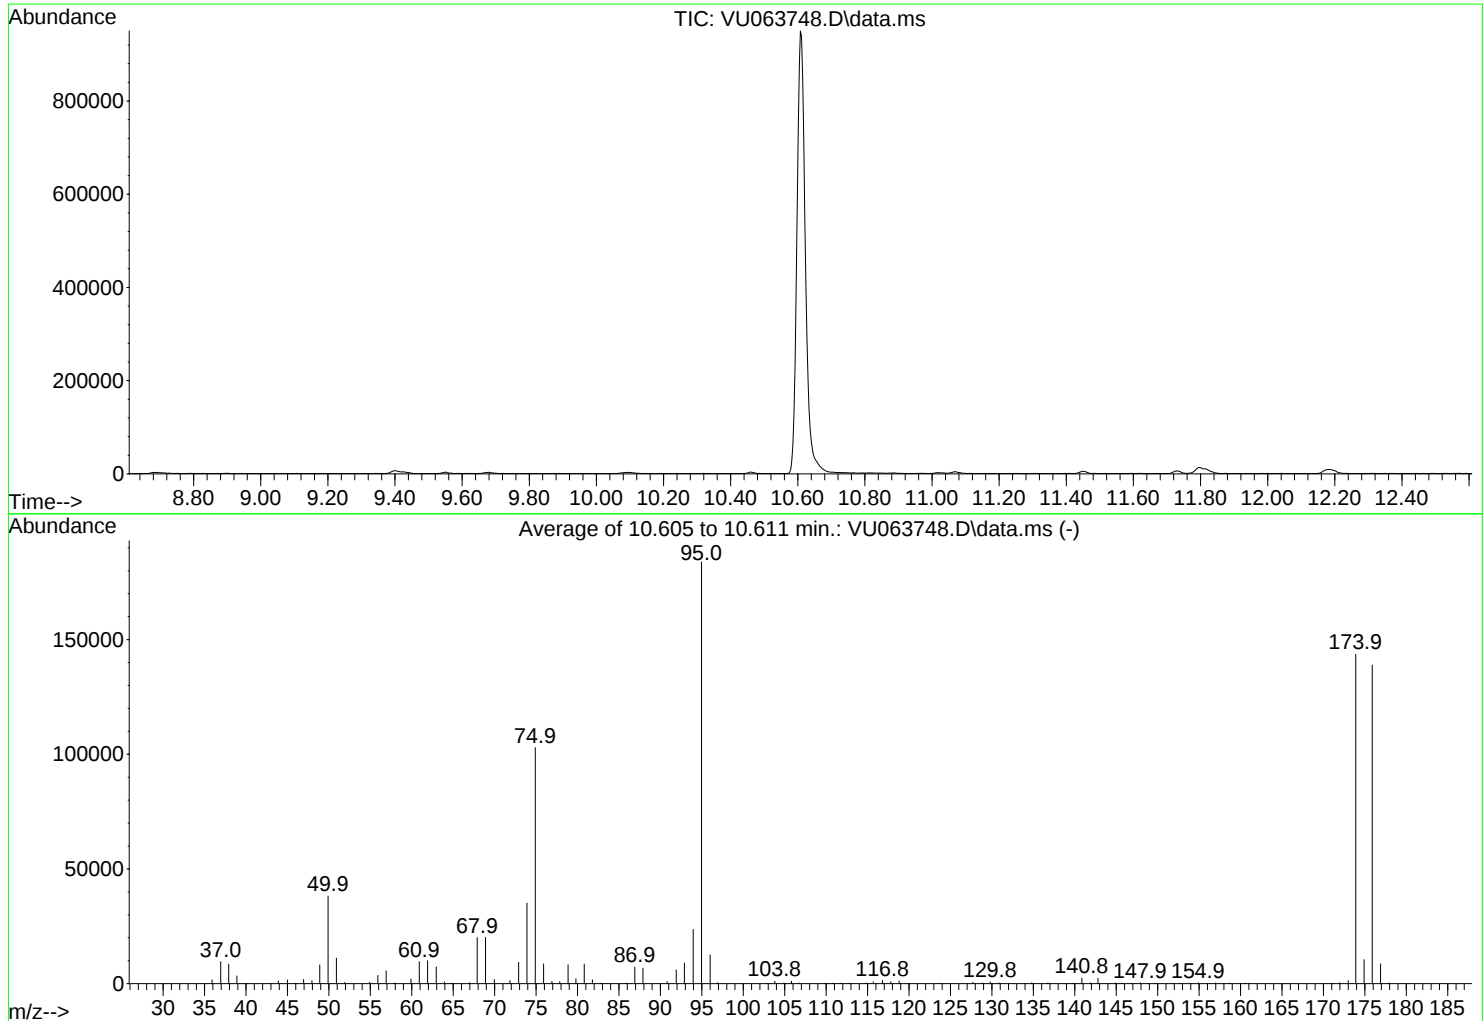

AutoFind: Scans 2897, 2898, 2899; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	38152	PASS
75	95	30	80	56.0	102909	PASS
95	95	100	100	100.0	183893	PASS
96	95	5	9	6.8	12592	PASS
173	174	0.00	2	0.9	1338	PASS
174	95	50	120	78.1	143595	PASS
175	174	5	9	7.3	10445	PASS
176	174	95	101	96.7	138861	PASS
177	176	5	9	6.2	8661	PASS