


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU112118\
Data File : VU028303.D
Acq On : 21 Nov 2018 08:25
Operator : MD/SY
Sample : BFB58
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB58

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR111718WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Nov 23 00:40:40 2018

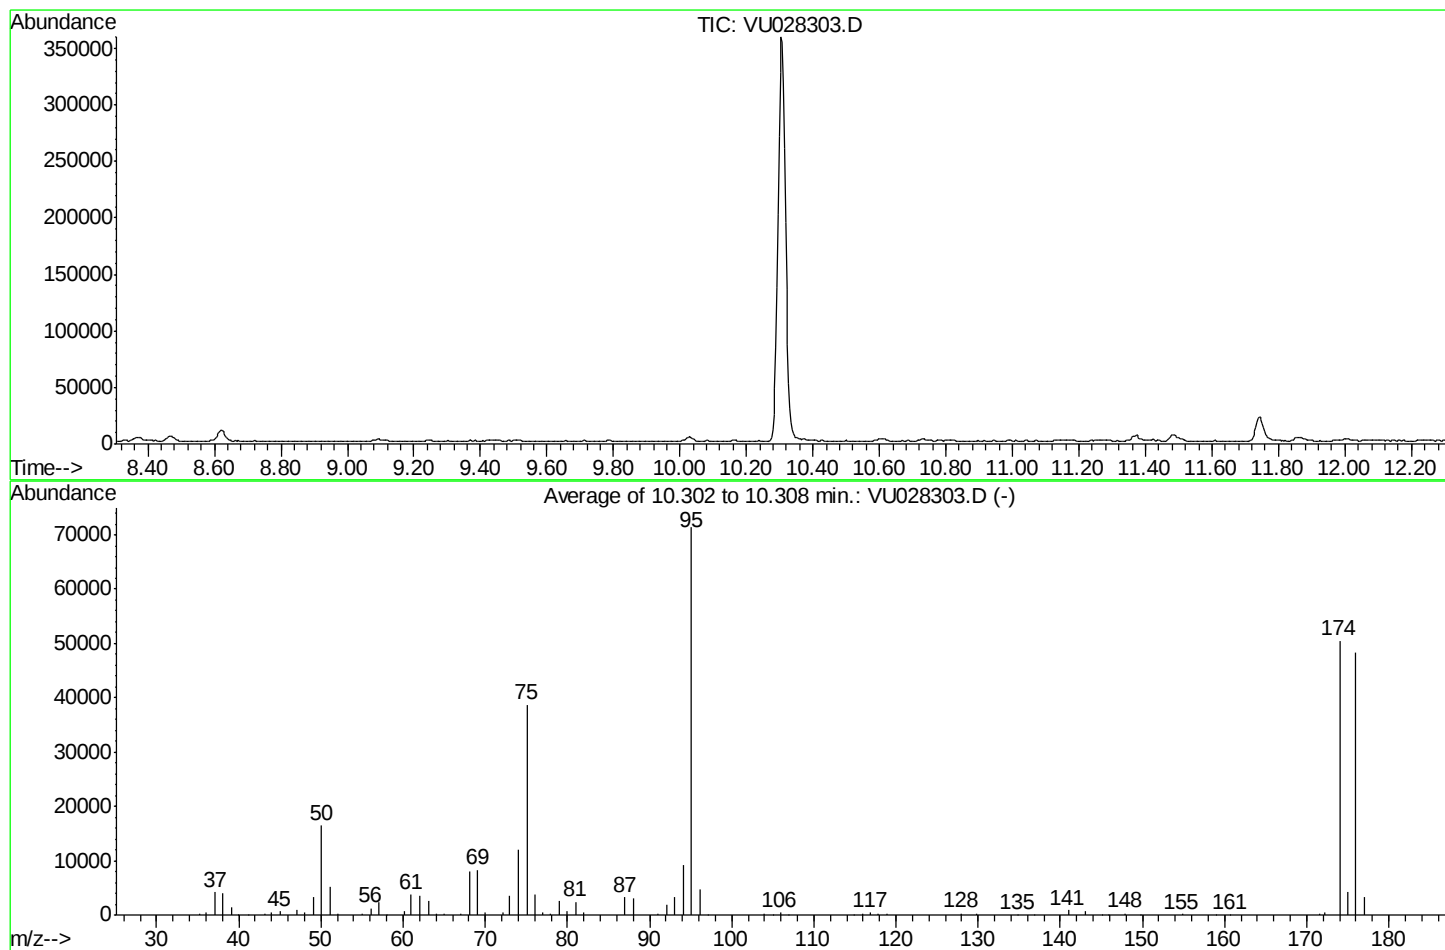

AutoFind: Scans 2839, 2840, 2841; Background Corrected with Scan 2826

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.0	16398	PASS
75	95	30	80	54.3	38733	PASS
95	95	100	100	100.0	71392	PASS
96	95	5	9	6.5	4613	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	70.7	50469	PASS
175	174	5	9	8.5	4282	PASS
176	174	95	101	95.6	48272	PASS
177	176	5	9	6.6	3201	PASS

m/z	Abundance
35.20	182.0
36.00	1235.0
37.10	4282.0
38.10	4438.0
39.10	1667.0
40.00	378.0
41.10	114.0
43.10	213.0
44.00	1367.0
45.00	742.0
47.10	1083.0
48.00	541.0
49.00	3384.0
50.10	16968.0
51.10	5388.0
52.00	223.0
55.10	239.0
56.10	1268.0
57.10	2347.0
60.10	803.0
61.00	3907.0
62.10	3776.0
63.00	2734.0
64.10	337.0
65.10	169.0
67.00	187.0
68.10	8465.0
69.10	8479.0
70.10	619.0
72.10	524.0
73.00	3802.0
74.10	12213.0
75.10	39792.0
76.10	3791.0
77.00	481.0
77.90	377.0
79.00	2720.0
80.00	631.0
81.00	2594.0
81.90	467.0
87.00	3368.0
88.00	3054.0
90.90	378.0
92.10	2039.0
93.00	3389.0
94.10	9652.0
95.10	74064.0
96.10	4760.0
97.20	100.0
103.90	339.0
105.10	115.0
105.90	383.0
106.90	125.0
114.80	111.0
116.00	232.0
117.00	459.0
117.80	279.0
118.90	339.0
128.00	373.0
129.90	183.0
134.90	129.0
136.80	124.0
140.90	944.0
143.00	718.0
145.10	112.0
145.80	145.0
147.90	303.0
149.80	106.0
154.90	180.0
158.90	125.0
171.50	166.0
172.20	459.0
174.00	52256.0
175.00	4379.0
176.00	49800.0
177.00	3314.0
207.00	231.0

Instrument :
MSVOA_U
ClientSampleId :
BFB58

m/z	Abundance
35.10	185.0
36.00	1165.0
37.10	4002.0
38.10	4178.0
39.10	1525.0
40.00	316.0
41.10	144.0
43.10	235.0
44.00	1412.0
45.00	641.0
47.10	1038.0
48.00	428.0
49.10	3269.0
50.10	15913.0
51.10	4747.0
52.00	151.0
55.10	335.0
56.10	1217.0
57.10	2157.0
60.10	820.0
61.00	3531.0
62.10	3379.0
63.10	2650.0
64.10	342.0
65.00	150.0
66.90	168.0
68.10	7319.0
69.10	7930.0
70.10	657.0
72.10	490.0
73.00	3284.0
74.10	11538.0
75.10	37200.0
76.00	3597.0
77.00	579.0
77.90	334.0
79.00	2611.0
79.90	599.0
81.00	2290.0
81.90	434.0
87.00	3237.0
88.00	2717.0
91.00	335.0
92.10	1733.0
93.00	3068.0
94.10	8649.0
95.10	67728.0
96.10	4324.0
97.10	104.0
104.00	250.0
105.10	146.0
105.90	341.0
106.80	113.0
114.80	123.0
116.00	188.0
116.90	366.0
117.80	216.0
118.90	263.0
128.00	259.0
129.90	191.0
134.90	142.0
140.90	900.0
143.00	672.0
147.90	311.0
154.90	203.0
158.90	114.0
171.50	148.0
172.20	423.0
174.00	45736.0
175.00	4095.0
176.00	45432.0
177.00	2865.0
207.00	246.0

Instrument :
MSVOA_U
ClientSampleId :
BFB58

Scan 2826 (10.260 min): VU028303.D
BFB58

m/z	Abundance
35.90	591.0
38.00	184.0
39.10	141.0
39.90	266.0
44.00	902.0
63.80	127.0
207.10	288.0

Instrument :
MSVOA_U
ClientSampleId :
BFB58

m/z	Abundance
35.20	198.0
36.10	1137.0
37.10	4265.0
38.10	4192.0
39.00	1609.0
40.00	361.0
43.00	138.0
44.00	1388.0
45.00	696.0
47.10	981.0
48.00	684.0
49.10	3316.0
50.10	16313.0
51.10	5434.0
52.00	298.0
55.00	198.0
56.10	1282.0
57.10	2498.0
58.00	108.0
60.10	657.0
61.00	3836.0
62.10	3709.0
63.00	2672.0
64.10	312.0
65.10	166.0
67.00	189.0
68.00	8532.0
69.10	8499.0
70.00	512.0
72.10	491.0
73.00	3832.0
74.10	12164.0
75.10	39208.0
76.10	3632.0
77.00	400.0
77.90	330.0
79.00	2615.0
80.00	614.0
81.00	2556.0
82.00	443.0
87.00	3192.0
88.00	3239.0
90.90	301.0
92.00	2058.0
93.10	3357.0
94.10	9338.0
95.10	72384.0
96.10	4755.0
103.90	445.0
105.90	379.0
107.00	104.0
115.90	279.0
117.00	469.0
117.80	298.0
118.90	353.0
128.00	383.0
129.80	182.0
134.80	103.0
136.80	162.0
141.00	859.0
143.00	710.0
145.00	104.0
145.80	142.0
147.90	220.0
154.90	158.0
158.90	118.0
160.70	119.0
171.50	122.0
172.10	386.0
174.00	53416.0
175.00	4374.0
176.00	49584.0
177.00	3425.0
207.00	183.0

Instrument :
MSVOA_U
ClientSampleId :
BFB58