


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU112119\
Data File : VU035791.D
Acq On : 21 Nov 2019 08:39
Operator : JC/SP
Sample : BFB03
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB03

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR112119WMA.M
Title : TRACE VOA SOM01.0
Last Update : Sat Nov 23 00:14:30 2019

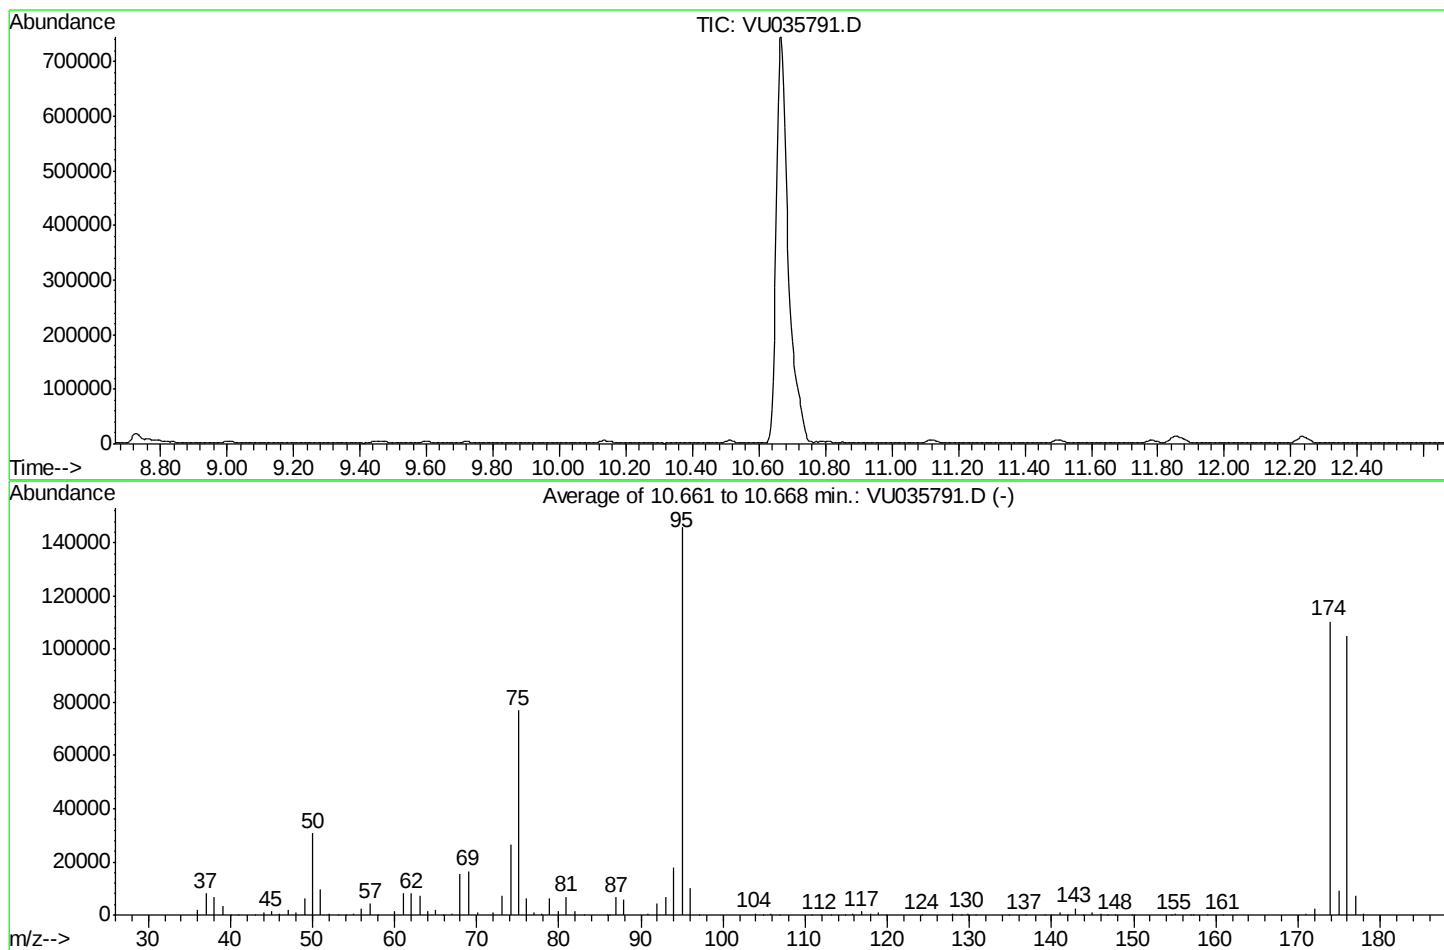

AutoFind: Scans 2899, 2900, 2901; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	30653	PASS
75	95	30	80	52.7	76840	PASS
95	95	100	100	100.0	145856	PASS
96	95	5	9	6.8	9931	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.6	110290	PASS
175	174	5	9	8.2	9047	PASS
176	174	95	101	95.4	105200	PASS
177	176	5	9	6.9	7280	PASS

m/z	Abundance
36.00	1690.0
37.00	7712.0
38.00	6818.0
39.00	3378.0
39.90	689.0
41.00	115.0
42.90	251.0
44.00	2231.0
45.00	1308.0
46.00	376.0
47.10	1858.0
48.00	1071.0
49.10	6320.0
50.10	30344.0
51.00	9734.0
52.10	596.0
53.10	193.0
54.00	152.0
55.00	490.0
56.00	2752.0
57.00	4142.0
58.00	103.0
60.00	1312.0
61.00	7959.0
62.10	8046.0
63.10	6718.0
64.00	1465.0
65.00	2026.0
66.00	148.0
67.10	573.0
68.00	15232.0
69.00	15951.0
70.10	1202.0
72.00	865.0
73.00	6709.0
74.10	25464.0
75.10	73368.0
76.10	6262.0
76.90	1032.0
77.90	765.0
78.90	6049.0
79.90	1497.0
80.90	6644.0
81.90	1696.0
83.00	131.0
86.10	237.0
87.00	6299.0
88.00	5582.0
90.90	657.0
92.00	3997.0
93.00	6252.0
94.00	17200.0
95.00	140864.0
96.00	9821.0
97.00	205.0
103.90	558.0
104.80	201.0
105.80	726.0
106.90	195.0
110.80	109.0
111.80	168.0
113.10	160.0
114.80	103.0
115.80	760.0
116.90	1305.0
117.90	604.0
119.00	979.0
119.80	143.0
124.20	115.0
127.90	363.0
129.00	248.0
129.80	667.0
130.80	184.0
134.90	187.0
136.80	213.0
140.00	135.0
141.00	1220.0
141.90	211.0
142.90	2188.0
143.90	133.0
144.90	1120.0
146.00	342.0
146.80	103.0
147.80	144.0
149.80	118.0
154.60	193.0
155.10	229.0
156.90	171.0
160.90	187.0
170.90	433.0
172.00	2244.0
173.90	104752.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

175.00	8696.0
175.90	99872.0
177.00	6764.0
178.00	250.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

m/z	Abundance
36.00	1891.0
37.00	8306.0
38.00	6914.0
39.00	3399.0
40.00	609.0
42.90	206.0
44.00	2261.0
45.00	1391.0
46.00	439.0
47.10	1855.0
48.00	1192.0
49.10	6578.0
50.00	30976.0
51.00	10080.0
52.10	581.0
53.00	184.0
54.00	200.0
55.00	548.0
56.00	2713.0
57.00	4278.0
58.00	244.0
60.00	1501.0
61.00	8211.0
62.00	8329.0
63.10	7174.0
64.00	1541.0
65.00	2178.0
65.90	133.0
67.00	564.0
68.00	16015.0
69.00	17032.0
70.00	1129.0
72.00	836.0
73.00	7235.0
74.10	27112.0
75.00	78144.0
76.10	6499.0
76.90	1135.0
77.90	641.0
78.90	6501.0
79.90	1591.0
80.90	7093.0
81.90	1661.0
83.00	172.0
86.10	215.0
87.00	6838.0
87.90	6199.0
90.90	681.0
92.00	4384.0
93.00	6659.0
94.00	18160.0
95.00	148416.0
96.00	10171.0
97.00	214.0
103.90	688.0
104.80	175.0
105.80	650.0
106.90	243.0
110.80	128.0
111.80	147.0
113.10	177.0
114.80	148.0
115.90	760.0
116.90	1363.0
117.90	553.0
119.00	1122.0
119.80	151.0
124.20	118.0
127.90	387.0
129.00	195.0
129.80	613.0
130.80	204.0
134.90	158.0
136.80	180.0
140.00	139.0
141.00	1221.0
141.90	214.0
142.90	2498.0
143.90	202.0
144.90	1189.0
146.00	311.0
146.80	135.0
147.80	141.0
149.80	135.0
155.10	319.0
156.80	140.0
159.00	132.0
160.90	159.0
171.00	425.0
172.00	2228.0
173.90	112464.0
175.00	9235.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

175.90	107184.0
177.00	7556.0
178.00	261.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

m/z	Abundance
36.00	1874.0
37.00	8428.0
38.00	6995.0
39.10	3292.0
40.00	528.0
42.90	138.0
44.00	2187.0
45.00	1359.0
46.00	440.0
47.10	1828.0
48.00	1160.0
49.10	6566.0
50.00	30640.0
51.00	9838.0
52.10	514.0
53.00	194.0
54.00	199.0
55.00	574.0
56.00	2499.0
57.10	4420.0
58.00	345.0
60.00	1681.0
61.00	8179.0
62.00	8134.0
63.00	7326.0
64.00	1559.0
65.00	1990.0
65.90	155.0
67.00	455.0
68.00	15700.0
69.00	16624.0
70.00	1085.0
72.00	735.0
73.00	7349.0
74.10	26920.0
75.00	79008.0
76.00	6596.0
77.00	1142.0
78.00	517.0
78.90	6359.0
79.90	1748.0
80.90	7041.0
81.90	1560.0
83.00	190.0
85.80	315.0
87.00	6894.0
88.00	6248.0
90.90	589.0
92.00	4614.0
93.00	6679.0
94.00	18296.0
95.00	148288.0
96.00	9802.0
97.00	233.0
103.90	763.0
104.80	170.0
105.80	626.0
106.90	294.0
110.90	170.0
111.90	125.0
113.00	167.0
114.80	195.0
115.90	593.0
116.90	1379.0
117.90	471.0
118.90	1127.0
127.90	494.0
129.00	154.0
129.80	479.0
130.80	198.0
134.80	201.0
136.70	192.0
139.10	101.0
139.90	112.0
141.00	1185.0
141.90	184.0
142.90	2774.0
143.90	248.0
144.90	1165.0
146.00	273.0
146.80	120.0
147.80	171.0
150.00	143.0
155.00	311.0
156.80	115.0
157.20	149.0
159.00	136.0
171.10	443.0
172.00	2106.0
173.90	113656.0
175.00	9212.0
176.00	108544.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

177.00	7522.0
177.90	322.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

Scan 2884 (10.613 min): VU035791.D
BFB03

m/z	Abundance
40.00	527.0
43.10	175.0
44.00	1164.0
44.80	107.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03