

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
 Data File : VU052018.D
 Acq On : 22 Nov 2022 01:00
 Operator : JC/MD
 Sample : N5737-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Nov 22 02:08:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Nov 22 01:03:12 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	435644	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	425086	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	164048	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	171819	45.513	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	91.020%		
7) Chloroethane-d5	1.906	69	147184	49.229	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	98.460%		
11) 1,1-Dichloroethene-d2	2.565	63	200214	35.779	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	71.560%		
21) 2-Butanone-d5	4.617	46	230012	101.390	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	101.390%		
24) Chloroform-d	5.060	84	299696	48.453	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.900%		
26) 1,2-Dichloroethane-d4	5.700	65	187046	50.279	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	100.560%		
32) Benzene-d6	5.726	84	629435	49.677	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.360%		
36) 1,2-Dichloropropane-d6	6.687	67	207849	51.062	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	102.120%		
41) Toluene-d8	7.896	98	519738	45.911	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	91.820%		
43) trans-1,3-Dichloroprop...	8.176	79	76366	44.071	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	88.140%		
47) 2-Hexanone-d5	8.629	63	152763	96.206	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	96.210%		
56) 1,1,2,2-Tetrachloroeth...	10.751	84	314862	48.894	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	97.780%		
66) 1,2-Dichlorobenzene-d4	12.189	152	182664	53.845	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	107.680%		
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.572	101	1982	0.750	ug/L #	20
12) 1,1-Dichloroethene	2.565	96	1679	0.666	ug/L #	1
13) Acetone	2.623	43	6344	3.061	ug/L	94
33) Benzene	5.774	78	10711	0.851	ug/L	100
39) cis-1,3-Dichloropropene	7.562	75	4296	0.903	ug/L #	69
44) trans-1,3-Dichloropropene	8.176	75	3200	0.719	ug/L #	80
51) Chlorobenzene	9.443	112	16421	1.918	ug/L	97
65) 1,4-Dichlorobenzene	11.835	146	4691	0.949	ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
Data File : VU052018.D
Acq On : 22 Nov 2022 01:00
Operator : JC/MD
Sample : N5737-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Nov 22 02:08:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 22 01:03:12 2022
Response via : Initial Calibration

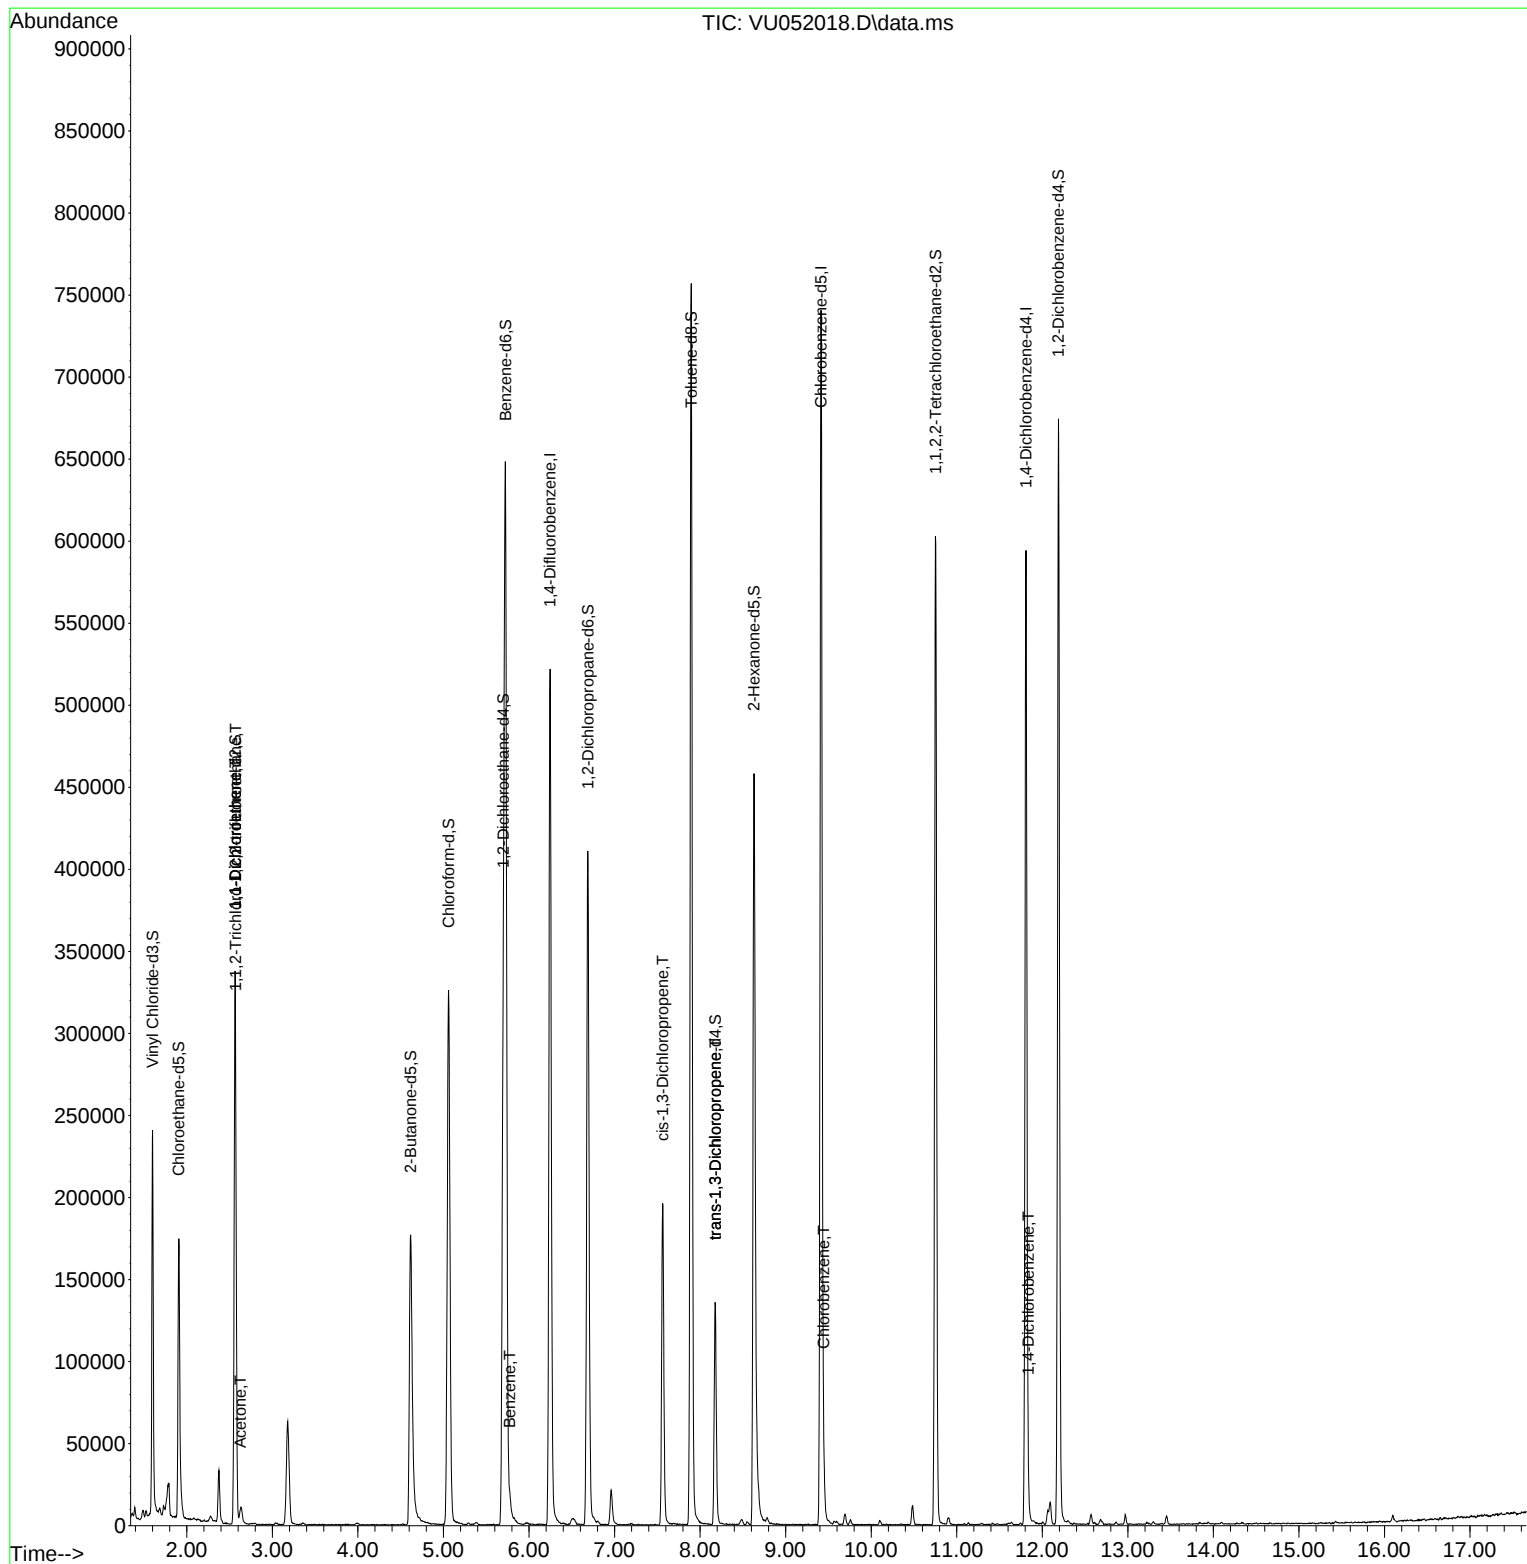

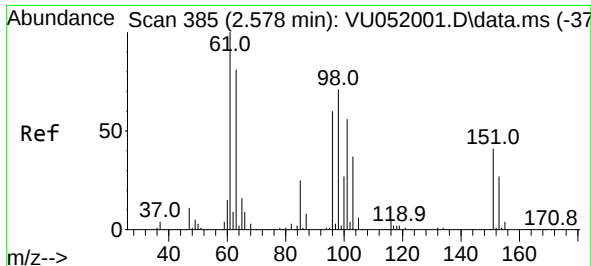

#10

1,1,2-Trichloro-1,2,2-trifluoroethane

Concen: 0.750 ug/L

RT: 2.572 min Scan# 385

Delta R.T. -0.006 min

Lab File: VU052018.D

Acq: 22 Nov 2022 01:00

Instrument :

MSVOA_U

ClientSampleId :





Tgt Ion:101 Resp: 1982

Ion Ratio Lower Upper

101 100

85 0.0 33.6 50.4#

151 0.0 58.9 88.3#

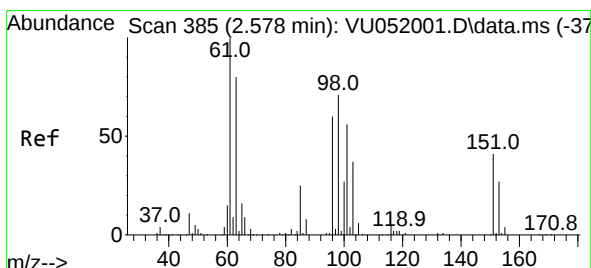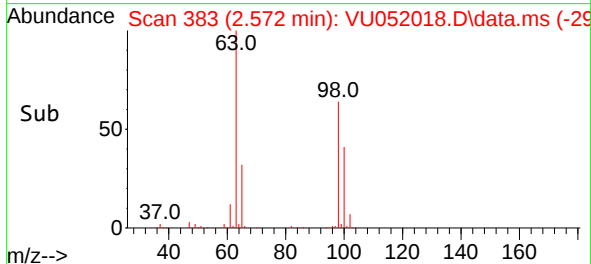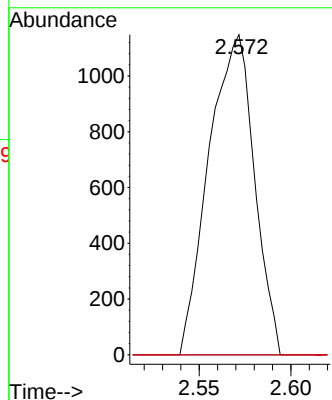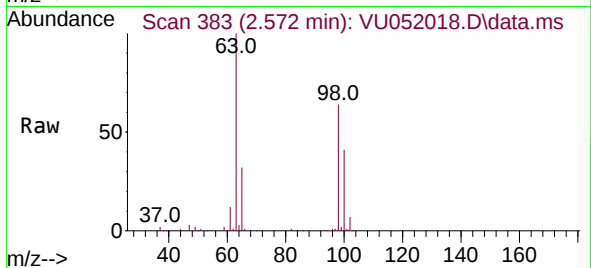

#12

1,1-Dichloroethene

Concen: 0.666 ug/L

RT: 2.565 min Scan# 381

Delta R.T. -0.013 min

Lab File: VU052018.D

Acq: 22 Nov 2022 01:00




Tgt Ion: 96 Resp: 1679


Ion Ratio Lower Upper

96 100

61 1267.6 114.2 212.0#

63 11066.7 90.9 168.7#

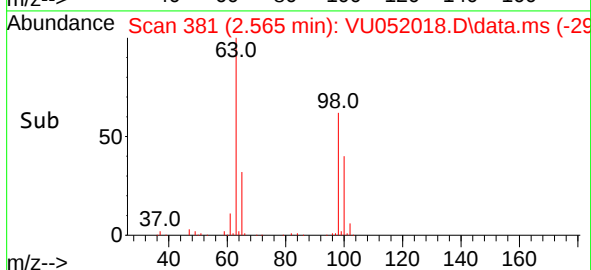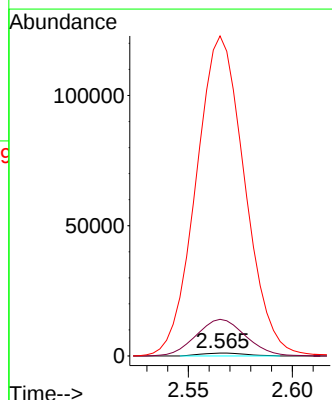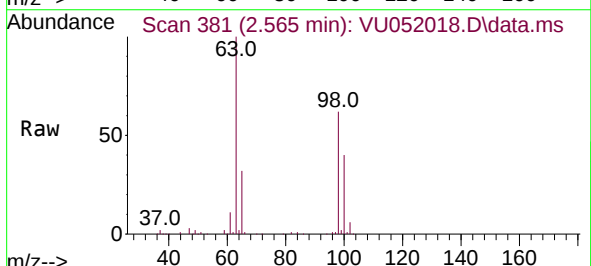

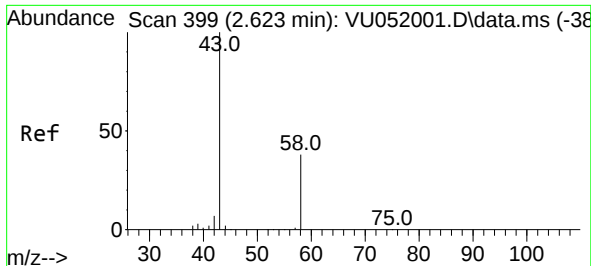

#13

Acetone

Concen: 3.061 ug/L

RT: 2.623 min Scan# 399

Delta R.T. 0.000 min

Lab File: VU052018.D

Acq: 22 Nov 2022 01:00

Instrument :

MSVOA_U





ClientSampleId :

Tgt Ion: 43 Resp: 6344

Ion Ratio Lower Upper

43 100

58 34.7 0.0 76.6

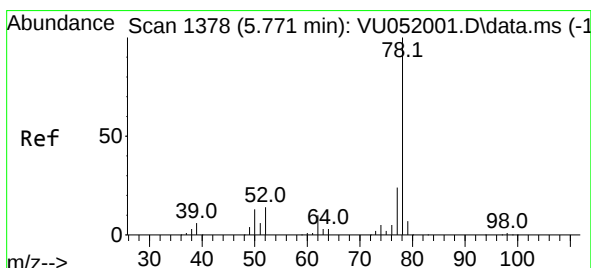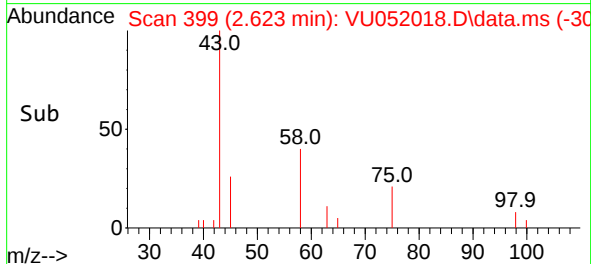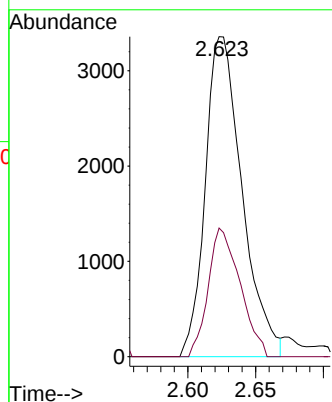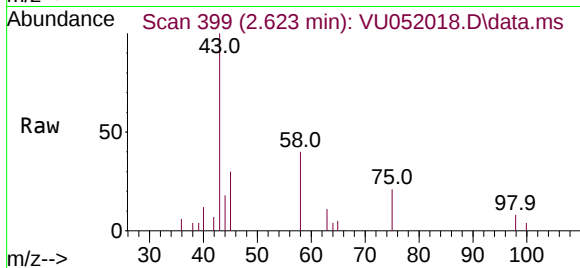

#33

Benzene

Concen: 0.851 ug/L




RT: 5.774 min Scan# 1379


Delta R.T. 0.003 min

Lab File: VU052018.D

Acq: 22 Nov 2022 01:00

Tgt Ion: 78 Resp: 10711

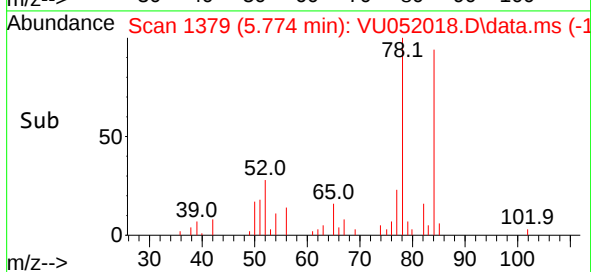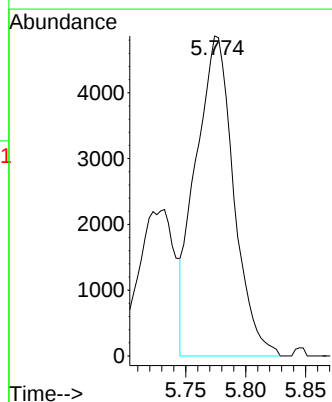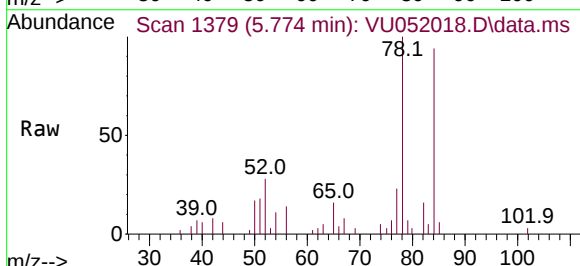

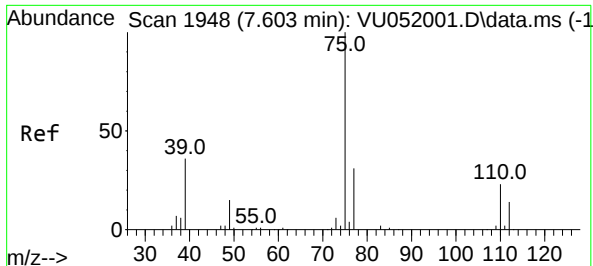

#39

cis-1,3-Dichloropropene

Concen: 0.903 ug/L

RT: 7.562 min Scan# 1948

Delta R.T. -0.042 min

Lab File: VU052018.D

Acq: 22 Nov 2022 01:00

Instrument :

MSVOA_U





ClientSampleId :

Tgt Ion: 75 Resp: 4296

Ion Ratio Lower Upper

75 100

77 48.8 22.3 41.3#

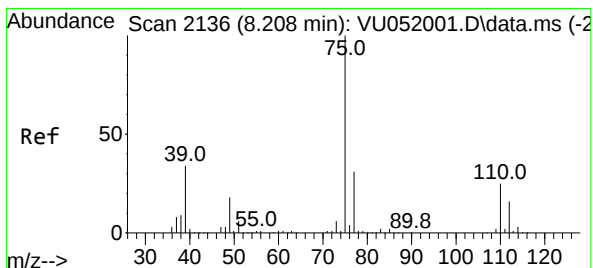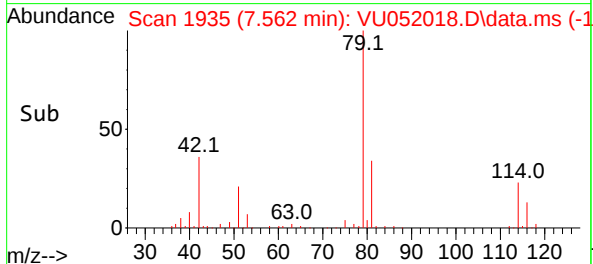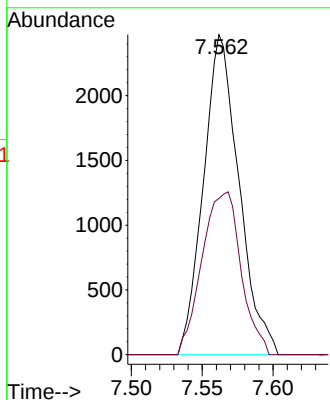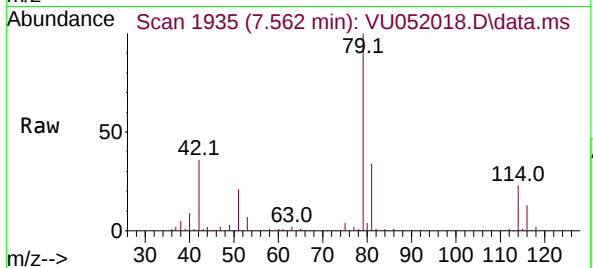

#44

trans-1,3-Dichloropropene

Concen: 0.719 ug/L

RT: 8.176 min Scan# 2126

Delta R.T. -0.032 min

Lab File: VU052018.D




Acq: 22 Nov 2022 01:00


Tgt Ion: 75 Resp: 3200

Ion Ratio Lower Upper

75 100

77 43.7 22.7 42.1#


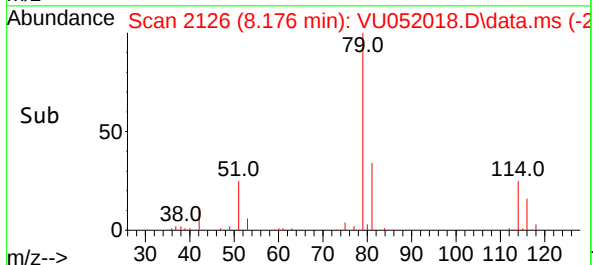
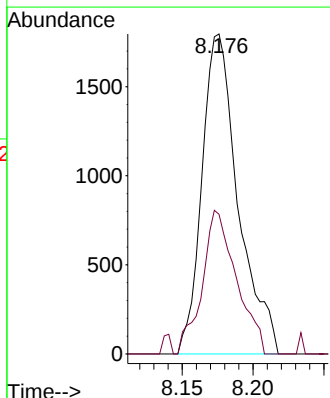
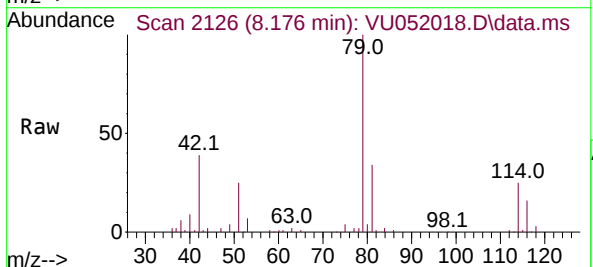


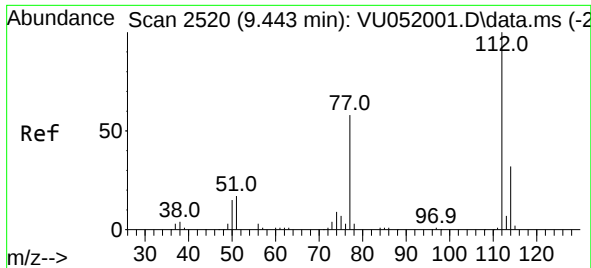

#51
Chlorobenzene
Concen: 1.918 ug/L
RT: 9.443 min Scan# 21
Delta R.T. 0.000 min
Lab File: VU052018.D
Acq: 22 Nov 2022 01:00

Instrument :
MSVOA_U
ClientSampleId :

Tgt Ion:112 Resp: 16421
Ion Ratio Lower Upper
112 100
114 29.4 22.2 41.2
77 56.0 46.5 69.7

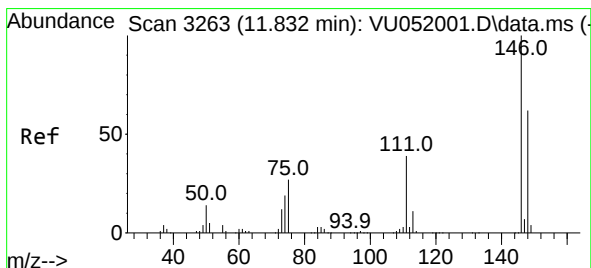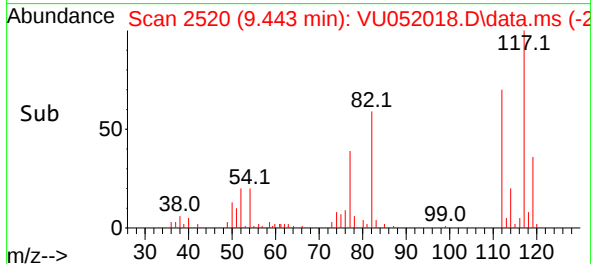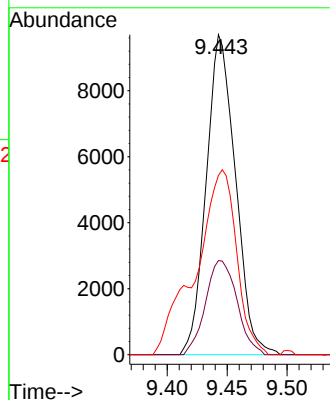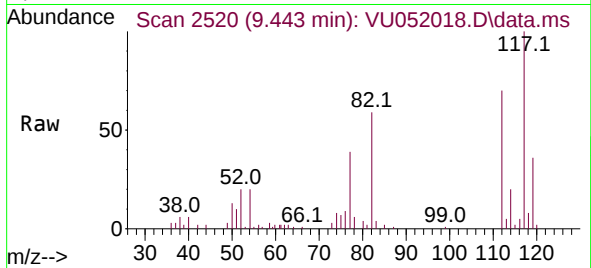

#65
1,4-Dichlorobenzene
Concen: 0.949 ug/L
RT: 11.835 min Scan# 3264
Delta R.T. 0.003 min
Lab File: VU052018.D
Acq: 22 Nov 2022 01:00

Tgt Ion:146 Resp: 4691
Ion Ratio Lower Upper
146 100
111 44.3 27.6 51.2
148 78.7 44.8 83.2

