

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
 Data File : VU052026.D
 Acq On : 22 Nov 2022 05:19
 Operator : JC/MD
 Sample : N5679-06ME
 Misc : 5.08g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COLO1ME

Quant Time: Nov 22 07:19:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Nov 22 03:27:10 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.244	114	520325	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	527820	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.813	152	223936	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.598	65	179151	39.732	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	79.460%
7) Chloroethane-d5	1.871	69	61872	17.326	ug/L	-0.03
Spiked Amount	50.000	Range	70 - 130	Recovery	=	34.660%#
11) 1,1-Dichloroethene-d2	2.540	63	226999	33.963	ug/L	-0.03
Spiked Amount	50.000	Range	60 - 125	Recovery	=	67.920%
21) 2-Butanone-d5	4.626	46	268822	99.212	ug/L	0.01
Spiked Amount	100.000	Range	40 - 130	Recovery	=	99.210%
24) Chloroform-d	5.057	84	326829	44.240	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.480%
26) 1,2-Dichloroethane-d4	5.694	65	206572	46.491	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.980%
32) Benzene-d6	5.716	84	703042	44.687	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.380%
36) 1,2-Dichloropropane-d6	6.684	67	232663	46.033	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	92.060%
41) Toluene-d8	7.896	98	623105	44.329	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.660%
43) trans-1,3-Dichloroprop...	8.179	79	95037	44.171	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	88.340%
47) 2-Hexanone-d5	8.649	63	218005	110.571	ug/L	0.02
Spiked Amount	100.000	Range	45 - 130	Recovery	=	110.570%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	390840	48.879	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	97.760%
66) 1,2-Dichlorobenzene-d4	12.192	152	236478	51.066	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.140%
Target Compounds						
					Qvalue	
46) Tetrachloroethene	8.552	164	3729	1.355	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
Data File : VU052026.D
Acq On : 22 Nov 2022 05:19
Operator : JC/MD
Sample : N5679-06ME
Misc : 5.08g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L01ME


Quant Time: Nov 22 07:19:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 22 03:27:10 2022
Response via : Initial Calibration

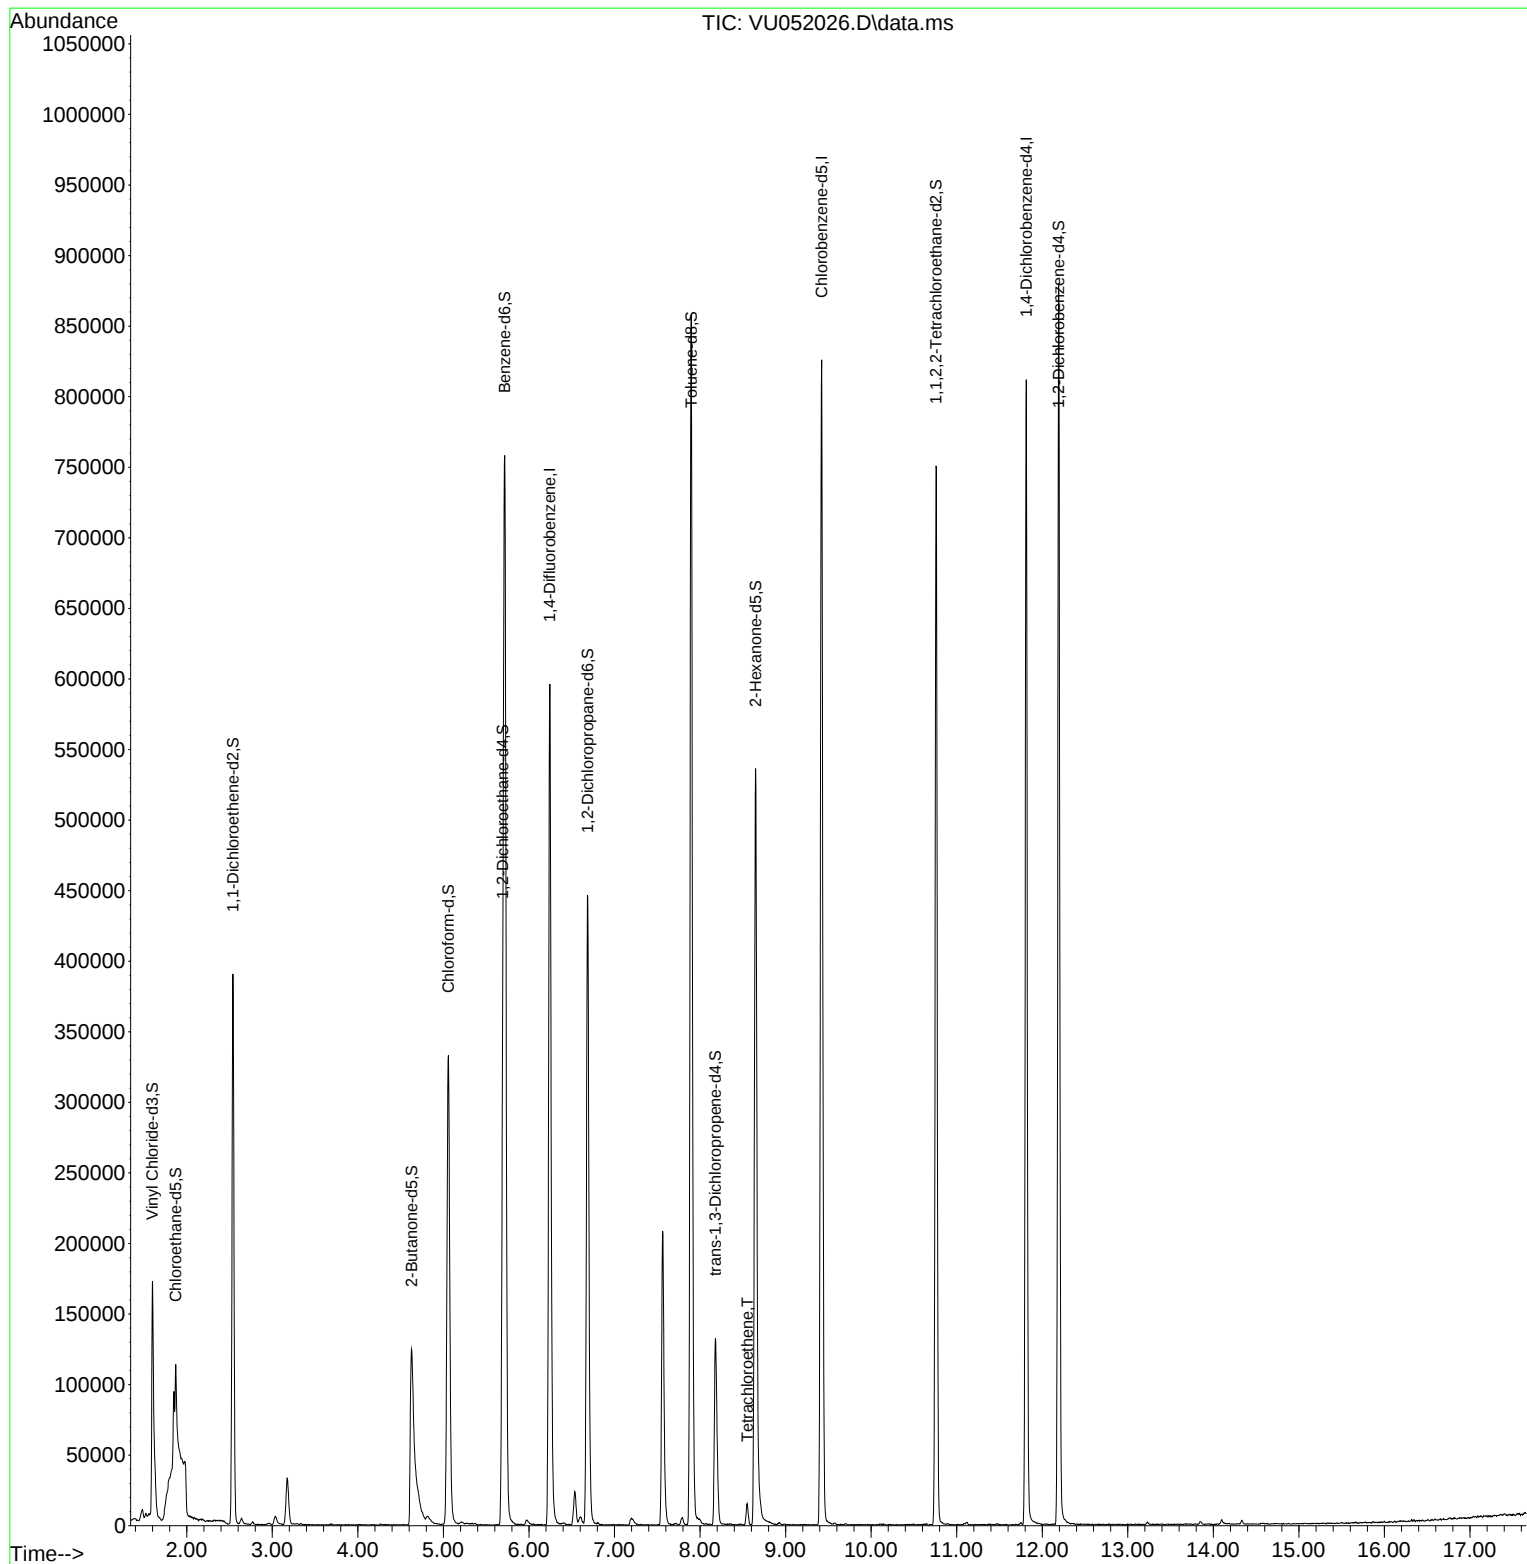

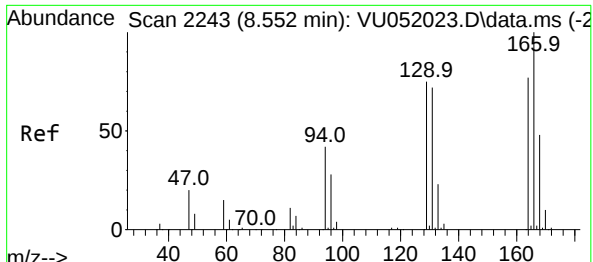

#46
 Tetrachloroethene
 Concen: 1.355 ug/L
 RT: 8.552 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: VU052026.D
 Acq: 22 Nov 2022 05:19

Instrument :
 MSVOA_U
 ClientSampleId :
 C0L01ME

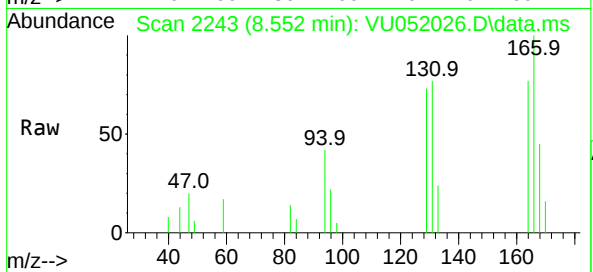

Tgt Ion:	164	Resp:	3729
Ion	Ratio	Lower	Upper
164	100		
129	95.1	67.3	124.9
131	100.1	65.2	121.2
166	130.6	89.9	166.9

