

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
 Data File : VU052002.D
 Acq On : 21 Nov 2022 17:55
 Operator : JC/MD
 Sample : VU1121WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK028

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

Signal : TIC: VU052002.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	102	rVB	274124	319121	16.28%	2.229%
2	1.912	170	178	199	rVB	206007	291923	14.89%	2.039%
3	2.565	369	381	400	rBV	403787	669447	34.15%	4.676%
4	2.848	466	469	472	rBV2	436	276	0.01%	0.002%
5	3.346	620	624	626	rBV2	1013	877	0.04%	0.006%
6	3.404	639	642	644	rBV	298	210	0.01%	0.001%
7	3.526	675	680	685	rBV2	269	359	0.02%	0.003%
8	3.552	685	688	690	rBV3	361	250	0.01%	0.002%
9	3.607	703	705	707	rBV	153	89	0.00%	0.001%
10	3.684	726	729	733	rBV2	263	201	0.01%	0.001%
11	3.816	768	770	772	rVB	236	112	0.01%	0.001%
12	3.861	779	784	785	rBV2	258	190	0.01%	0.001%
13	3.887	790	792	794	rBV2	225	89	0.00%	0.001%
14	3.925	801	804	806	rBV	182	118	0.01%	0.001%
15	3.993	822	825	833	rVB2	514	471	0.02%	0.003%
16	4.028	833	836	838	rBV2	206	149	0.01%	0.001%
17	4.060	844	846	848	rBV	148	95	0.00%	0.001%
18	4.092	853	856	859	rBV	258	177	0.01%	0.001%
19	4.176	879	882	887	rVB2	302	190	0.01%	0.001%
20	4.224	894	897	898	rBV2	245	133	0.01%	0.001%
21	4.279	910	914	918	rVB2	211	136	0.01%	0.001%
22	4.308	918	923	927	rBV2	284	295	0.02%	0.002%
23	4.340	930	933	935	rVV2	379	231	0.01%	0.002%
24	4.359	935	939	947	rVB2	375	441	0.02%	0.003%
25	4.507	981	985	988	rBV2	251	191	0.01%	0.001%
26	4.555	994	1000	1002	rBV2	262	247	0.01%	0.002%
27	4.616	1007	1019	1054	rBV	167986	418444	21.35%	2.923%
28	4.877	1099	1100	1103	rBV	354	180	0.01%	0.001%
29	5.060	1140	1157	1181	rBV	343741	761336	38.84%	5.318%
30	5.327	1238	1240	1243	rBV	191	126	0.01%	0.001%
31	5.378	1249	1256	1259	rBV5	906	826	0.04%	0.006%
32	5.452	1276	1279	1281	rBV2	459	265	0.01%	0.002%
33	5.485	1287	1289	1291	rBV2	282	143	0.01%	0.001%
34	5.501	1291	1294	1296	rBV2	279	178	0.01%	0.001%
35	5.597	1320	1324	1327	rVB3	238	177	0.01%	0.001%
36	5.648	1336	1340	1342	rVB	375	266	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
 Data File : VU052002.D
 Acq On : 21 Nov 2022 17:55
 Operator : JC/MD
 Sample : VU1121WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK028

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

37	5.722	1342	1363	1400	rBV2	721643	1960366	100.00%	13.692%
38	6.041	1457	1462	1470	rBV3	890	1196	0.06%	0.008%
39	6.115	1482	1485	1488	rBV2	740	475	0.02%	0.003%
40	6.169	1500	1502	1504	rBV	222	97	0.00%	0.001%
41	6.195	1508	1510	1512	rBV2	174	73	0.00%	0.001%
42	6.247	1512	1526	1560	rBV	587709	1137392	58.02%	7.944%
43	6.632	1643	1646	1648	rBV	240	114	0.01%	0.001%
44	6.687	1648	1663	1691	rBV	442909	881317	44.96%	6.156%
45	6.906	1728	1731	1733	rBV2	261	167	0.01%	0.001%
46	6.954	1742	1746	1749	rBV2	371	227	0.01%	0.002%
47	7.063	1778	1780	1782	rBV	86	48	0.00%	0.000%
48	7.092	1786	1789	1794	rBV2	227	247	0.01%	0.002%
49	7.304	1851	1855	1858	rBV	187	180	0.01%	0.001%
50	7.362	1870	1873	1876	rBV	222	129	0.01%	0.001%
51	7.378	1876	1878	1880	rVV	122	31	0.00%	0.000%
52	7.420	1887	1891	1893	rBV2	300	253	0.01%	0.002%
53	7.452	1897	1901	1903	rBV2	353	292	0.01%	0.002%
54	7.468	1903	1906	1911	rVV3	266	224	0.01%	0.002%
55	7.565	1923	1936	1965	rBV	221104	402013	20.51%	2.808%
56	7.732	1986	1988	1991	rVB3	497	291	0.01%	0.002%
57	7.796	2000	2008	2016	rBV4	1902	2856	0.15%	0.020%
58	7.841	2019	2022	2024	rVB3	371	167	0.01%	0.001%
59	7.896	2025	2039	2058	rBV	866716	1493855	76.20%	10.434%
60	8.176	2115	2126	2152	rBV	159562	274058	13.98%	1.914%
61	8.401	2194	2196	2202	rVB3	924	718	0.04%	0.005%
62	8.468	2214	2217	2221	rBV3	341	285	0.01%	0.002%
63	8.484	2221	2222	2227	rVV2	340	214	0.01%	0.001%
64	8.504	2227	2228	2230	rVB	366	108	0.01%	0.001%
65	8.555	2237	2244	2251	rVB4	2295	3311	0.17%	0.023%
66	8.632	2256	2268	2310	rBV2	464612	925099	47.19%	6.461%
67	8.877	2341	2344	2346	rBV2	535	380	0.02%	0.003%
68	9.018	2385	2388	2390	rBV2	196	110	0.01%	0.001%
69	9.034	2390	2393	2394	rBV2	154	90	0.00%	0.001%
70	9.160	2429	2432	2438	rBV3	392	437	0.02%	0.003%
71	9.414	2498	2511	2538	rBV	820518	1374530	70.12%	9.601%
72	9.697	2592	2599	2609	rVB6	1571	2594	0.13%	0.018%
73	9.799	2628	2631	2632	rBV	180	86	0.00%	0.001%
74	9.851	2643	2647	2648	rBV2	394	230	0.01%	0.002%
75	9.877	2653	2655	2658	rBV2	268	141	0.01%	0.001%
76	9.925	2664	2670	2672	rBV	325	314	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
 Data File : VU052002.D
 Acq On : 21 Nov 2022 17:55
 Operator : JC/MD
 Sample : VU1121WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK028

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

77	10.111	2718	2728	2731	rBV5	2094	3134	0.16%	0.022%
78	10.295	2783	2785	2788	rBV	258	147	0.01%	0.001%
79	10.394	2814	2816	2817	rBV	245	121	0.01%	0.001%
80	10.449	2830	2833	2836	rBV	300	145	0.01%	0.001%
81	10.655	2894	2897	2899	rBV2	170	94	0.00%	0.001%
82	10.754	2914	2928	2946	rBV	620869	1014862	51.77%	7.088%
83	10.979	2996	2998	3000	rBV2	194	127	0.01%	0.001%
84	11.092	3025	3033	3039	rBV4	1557	2667	0.14%	0.019%
85	11.610	3192	3194	3196	rBV	171	48	0.00%	0.000%
86	11.700	3219	3222	3224	rBV	363	276	0.01%	0.002%
87	11.745	3229	3236	3244	rVB3	4475	6014	0.31%	0.042%
88	11.809	3244	3256	3282	rBV	647336	1072778	54.72%	7.493%
89	12.192	3362	3375	3413	rBV	713068	1196468	61.03%	8.357%
90	13.137	3664	3669	3672	rBV3	502	529	0.03%	0.004%
91	13.217	3687	3694	3708	rBV4	5890	10068	0.51%	0.070%
92	13.340	3729	3732	3736	rVB2	546	399	0.02%	0.003%
93	13.841	3880	3888	3900	rBV3	11111	17553	0.90%	0.123%
94	14.089	3953	3965	3984	rBV	19518	38850	1.98%	0.271%
95	14.333	4032	4041	4052	rBV3	12154	20280	1.03%	0.142%




Sum of corrected areas: 14317234

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
Data File : VU052002.D
Acq On : 21 Nov 2022 17:55
Operator : JC/MD
Sample : VU1121WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK028

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

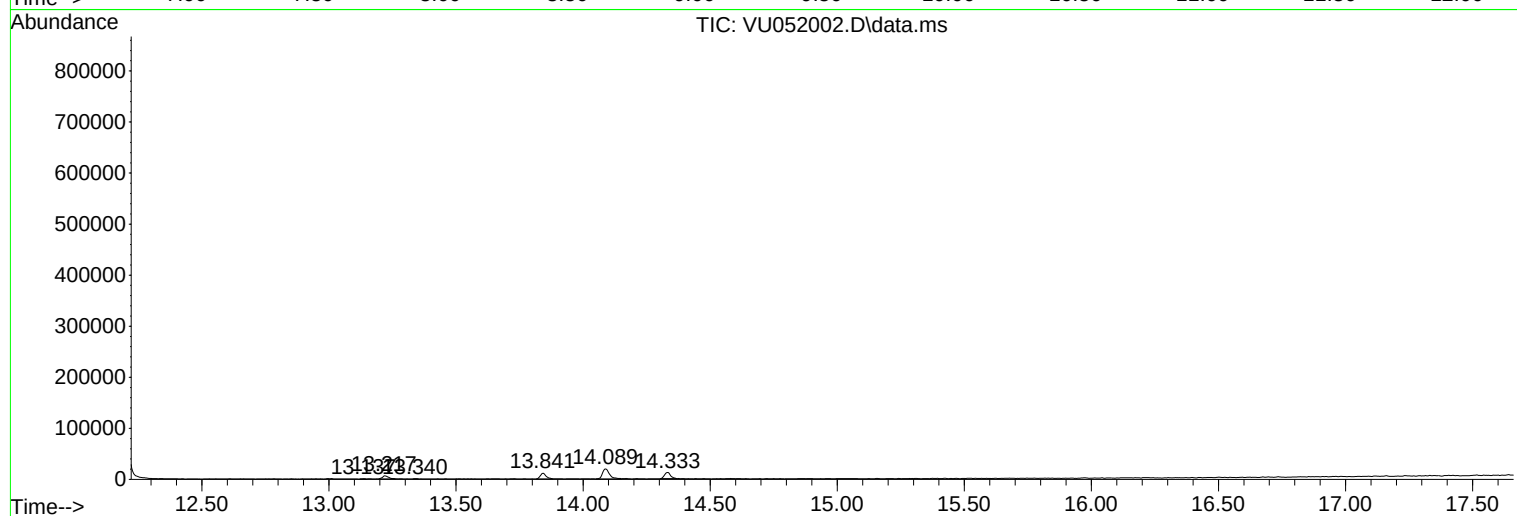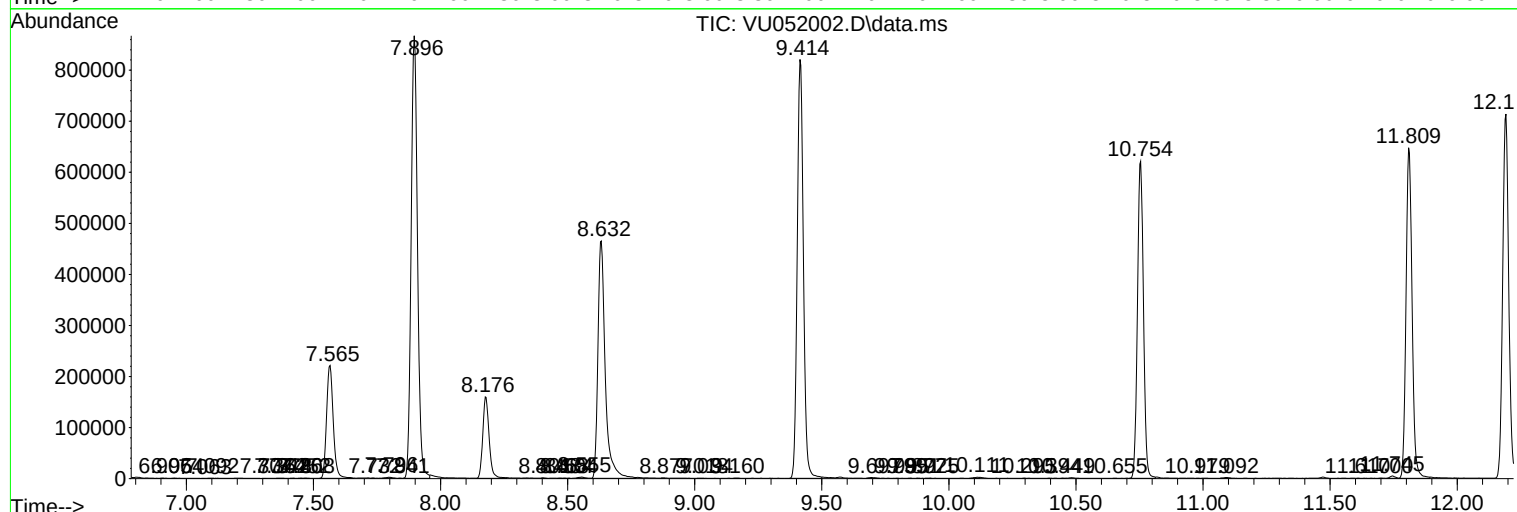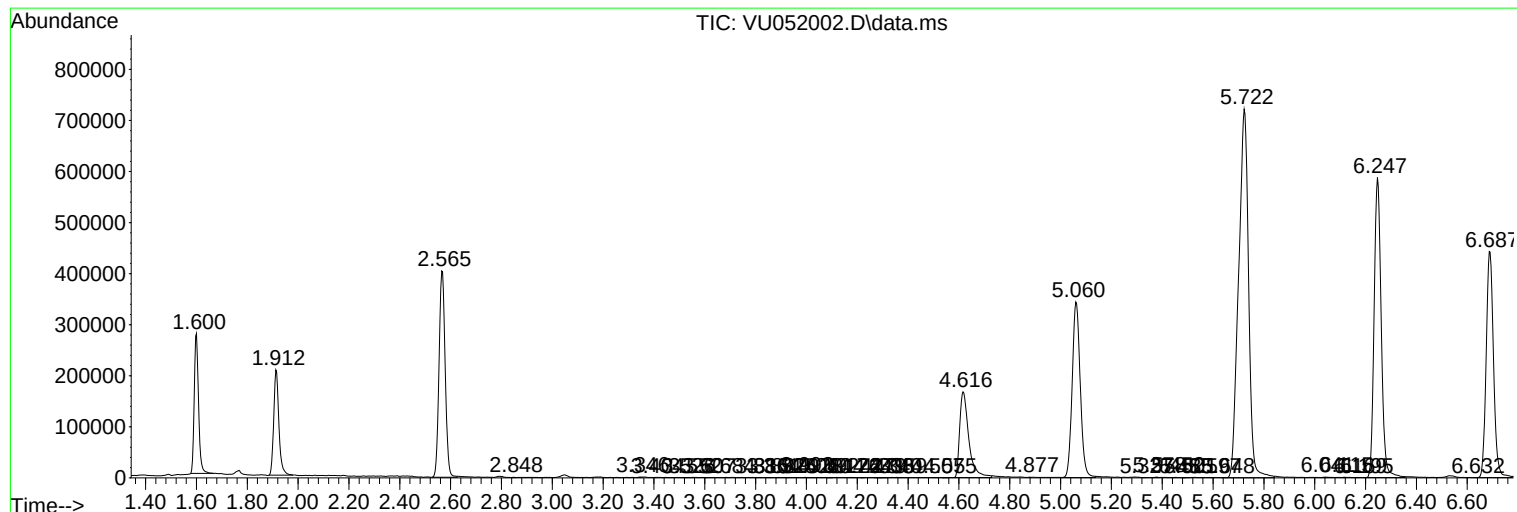

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
Data File : VU052002.D
Acq On : 21 Nov 2022 17:55
Operator : JC/MD
Sample : VU1121WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK028

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
Data File : VU052002.D
Acq On : 21 Nov 2022 17:55
Operator : JC/MD
Sample : VU1121WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK028

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc