

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
 Data File : VU052013.D
 Acq On : 21 Nov 2022 22:50
 Operator : JC/MD
 Sample : N5710-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

Signal : TIC: VU052013.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	98	rVB	263561	299445	15.90%	2.228%
2	1.906	168	176	201	rVB	187482	282782	15.02%	2.104%
3	2.565	369	381	396	rBV	379389	616024	32.72%	4.583%
4	2.922	490	492	495	rBV	242	100	0.01%	0.001%
5	3.012	516	520	521	rBV3	231	196	0.01%	0.001%
6	3.227	583	587	589	rBV2	277	203	0.01%	0.002%
7	3.269	597	600	603	rBV	288	178	0.01%	0.001%
8	3.337	617	621	623	rBV2	439	328	0.02%	0.002%
9	3.366	628	630	634	rVB2	469	282	0.01%	0.002%
10	3.385	634	636	638	rBV	154	72	0.00%	0.001%
11	3.475	659	664	668	rBV3	397	383	0.02%	0.003%
12	3.501	668	672	675	rBV2	338	286	0.02%	0.002%
13	3.562	688	691	693	rBV	211	127	0.01%	0.001%
14	3.632	710	713	717	rBV3	235	177	0.01%	0.001%
15	3.729	739	743	744	rBV	193	140	0.01%	0.001%
16	3.819	767	771	774	rVB2	335	247	0.01%	0.002%
17	3.883	790	791	793	rBV	172	82	0.00%	0.001%
18	4.067	845	848	849	rBV	174	82	0.00%	0.001%
19	4.095	854	857	859	rBV2	195	134	0.01%	0.001%
20	4.147	868	873	876	rBV2	319	269	0.01%	0.002%
21	4.166	876	879	884	rVV2	267	174	0.01%	0.001%
22	4.195	885	888	895	rVB2	324	276	0.01%	0.002%
23	4.343	931	934	936	rBV2	158	95	0.01%	0.001%
24	4.401	947	952	954	rBV2	268	232	0.01%	0.002%
25	4.420	954	958	959	rBV	212	128	0.01%	0.001%
26	4.501	979	983	984	rBV	228	140	0.01%	0.001%
27	4.555	996	1000	1002	rBV2	148	94	0.00%	0.001%
28	4.616	1007	1019	1053	rBV	175796	433420	23.02%	3.225%
29	5.060	1141	1157	1178	rBV	335005	734405	39.00%	5.464%
30	5.272	1219	1223	1225	rBV2	554	444	0.02%	0.003%
31	5.510	1295	1297	1301	rVB	343	230	0.01%	0.002%
32	5.722	1341	1363	1387	rBV2	697984	1882956	100.00%	14.009%
33	6.009	1449	1452	1454	rBV2	324	230	0.01%	0.002%
34	6.083	1471	1475	1480	rBV3	420	373	0.02%	0.003%
35	6.111	1480	1484	1485	rBV2	529	352	0.02%	0.003%
36	6.160	1496	1499	1503	rVB	313	173	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
 Data File : VU052013.D
 Acq On : 21 Nov 2022 22:50
 Operator : JC/MD
 Sample : N5710-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

37	6.189	1503	1508	1510	rBV2	111	98	0.01%	0.001%
38	6.246	1510	1526	1551	rBV	527056	1007597	53.51%	7.497%
39	6.539	1606	1617	1626	rBV8	3439	6792	0.36%	0.051%
40	6.687	1647	1663	1691	rBV	438247	859655	45.65%	6.396%
41	6.918	1731	1735	1736	rBV	321	152	0.01%	0.001%
42	6.954	1743	1746	1749	rBV3	175	130	0.01%	0.001%
43	6.976	1752	1753	1758	rVB2	145	67	0.00%	0.000%
44	7.021	1765	1767	1769	rBV2	300	136	0.01%	0.001%
45	7.054	1774	1777	1779	rBV3	260	175	0.01%	0.001%
46	7.102	1790	1792	1795	rBV	135	95	0.01%	0.001%
47	7.176	1812	1815	1816	rBV2	293	193	0.01%	0.001%
48	7.259	1839	1841	1846	rVB2	296	167	0.01%	0.001%
49	7.320	1857	1860	1864	rBV2	116	70	0.00%	0.001%
50	7.565	1923	1936	1964	rBV	210788	377761	20.06%	2.811%
51	7.896	2024	2039	2059	rBV	816948	1401960	74.46%	10.431%
52	8.176	2115	2126	2144	rBV	146009	250449	13.30%	1.863%
53	8.336	2173	2176	2177	rBV2	378	187	0.01%	0.001%
54	8.513	2229	2231	2235	rBV2	233	182	0.01%	0.001%
55	8.555	2235	2244	2251	rBV6	3464	5805	0.31%	0.043%
56	8.632	2256	2268	2310	rBV2	498926	969698	51.50%	7.215%
57	8.960	2367	2370	2374	rVB	461	340	0.02%	0.003%
58	8.986	2375	2378	2379	rBV	228	111	0.01%	0.001%
59	9.147	2426	2428	2431	rBV	270	166	0.01%	0.001%
60	9.166	2431	2434	2435	rBV	247	146	0.01%	0.001%
61	9.246	2456	2459	2460	rBV	169	95	0.01%	0.001%
62	9.295	2472	2474	2475	rBV	138	66	0.00%	0.000%
63	9.356	2491	2493	2496	rBV	238	117	0.01%	0.001%
64	9.414	2497	2511	2536	rBV	744238	1232377	65.45%	9.169%
65	9.671	2589	2591	2593	rBV	266	136	0.01%	0.001%
66	9.738	2609	2612	2615	rBV2	264	201	0.01%	0.001%
67	9.754	2615	2617	2626	rVB2	409	330	0.02%	0.002%
68	10.012	2695	2697	2703	rVB2	272	186	0.01%	0.001%
69	10.041	2703	2706	2708	rBV	183	97	0.01%	0.001%
70	10.102	2720	2725	2728	rBV4	495	506	0.03%	0.004%
71	10.224	2755	2763	2764	rBV	374	362	0.02%	0.003%
72	10.340	2796	2799	2804	rBV2	211	188	0.01%	0.001%
73	10.372	2804	2809	2812	rBV	401	331	0.02%	0.002%
74	10.449	2830	2833	2835	rBV	302	186	0.01%	0.001%
75	10.565	2865	2869	2872	rVB2	184	155	0.01%	0.001%
76	10.590	2872	2877	2881	rBV2	289	249	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
 Data File : VU052013.D
 Acq On : 21 Nov 2022 22:50
 Operator : JC/MD
 Sample : N5710-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

77	10.616	2882	2885	2887	rBV	254	173	0.01%	0.001%
78	10.651	2892	2896	2900	rVB2	246	249	0.01%	0.002%
79	10.677	2900	2904	2909	rBV2	259	247	0.01%	0.002%
80	10.751	2909	2927	2947	rBV	635879	1039760	55.22%	7.736%
81	11.037	3014	3016	3019	rBV	228	181	0.01%	0.001%
82	11.089	3029	3032	3035	rBV4	684	484	0.03%	0.004%
83	11.159	3052	3054	3060	rBV3	232	201	0.01%	0.001%
84	11.185	3060	3062	3065	rBV	308	173	0.01%	0.001%
85	11.285	3088	3093	3095	rBV	411	403	0.02%	0.003%
86	11.471	3147	3151	3156	rBV3	515	542	0.03%	0.004%
87	11.507	3156	3162	3164	rBV2	300	338	0.02%	0.003%
88	11.809	3243	3256	3283	rBV	564367	900733	47.84%	6.702%
89	11.999	3312	3315	3318	rBV2	677	502	0.03%	0.004%
90	12.066	3329	3336	3344	rBV5	5339	7837	0.42%	0.058%
91	12.192	3361	3375	3400	rBV	668341	1110846	58.99%	8.265%
92	12.423	3445	3447	3448	rBV	249	88	0.00%	0.001%
93	12.581	3494	3496	3498	rBV	289	120	0.01%	0.001%
94	12.664	3520	3522	3525	rBV	269	190	0.01%	0.001%
95	12.751	3546	3549	3551	rBV2	464	274	0.01%	0.002%
96	13.044	3637	3640	3642	rBV2	427	289	0.02%	0.002%
97	13.262	3701	3708	3715	rBV3	575	1097	0.06%	0.008%
98	13.429	3757	3760	3761	rBV	325	161	0.01%	0.001%
99	13.474	3770	3774	3775	rBV2	479	328	0.02%	0.002%
100	13.844	3884	3889	3898	rBV5	1513	2392	0.13%	0.018%




Sum of corrected areas: 13440581

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
Data File : VU052013.D
Acq On : 21 Nov 2022 22:50
Operator : JC/MD
Sample : N5710-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

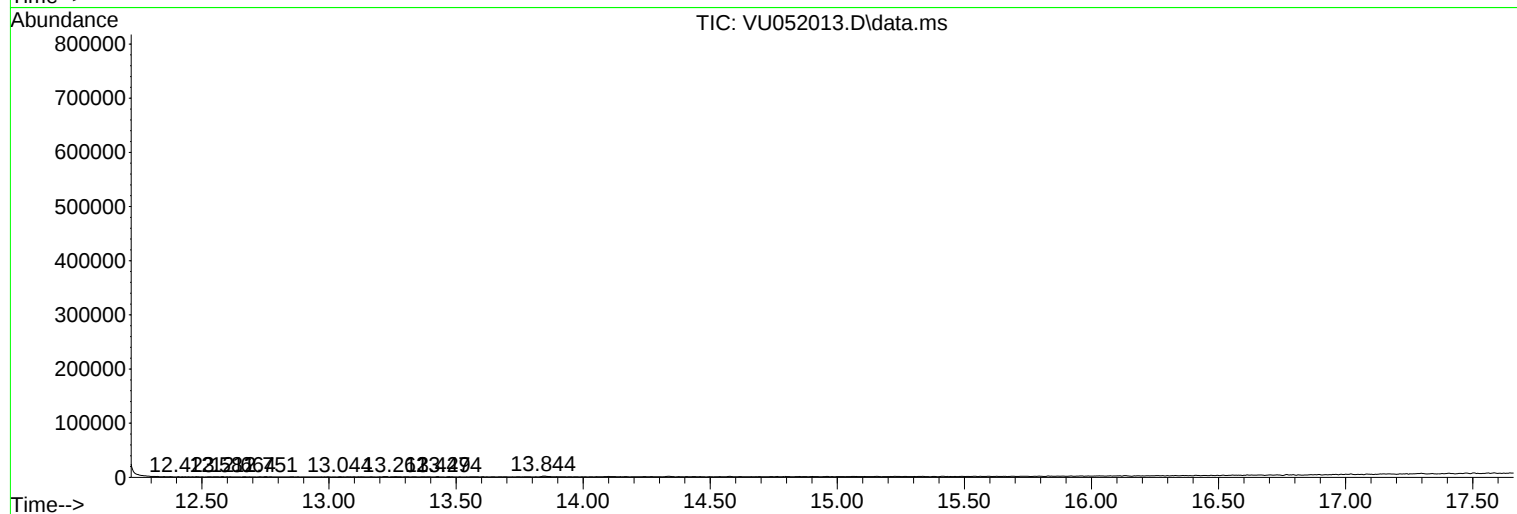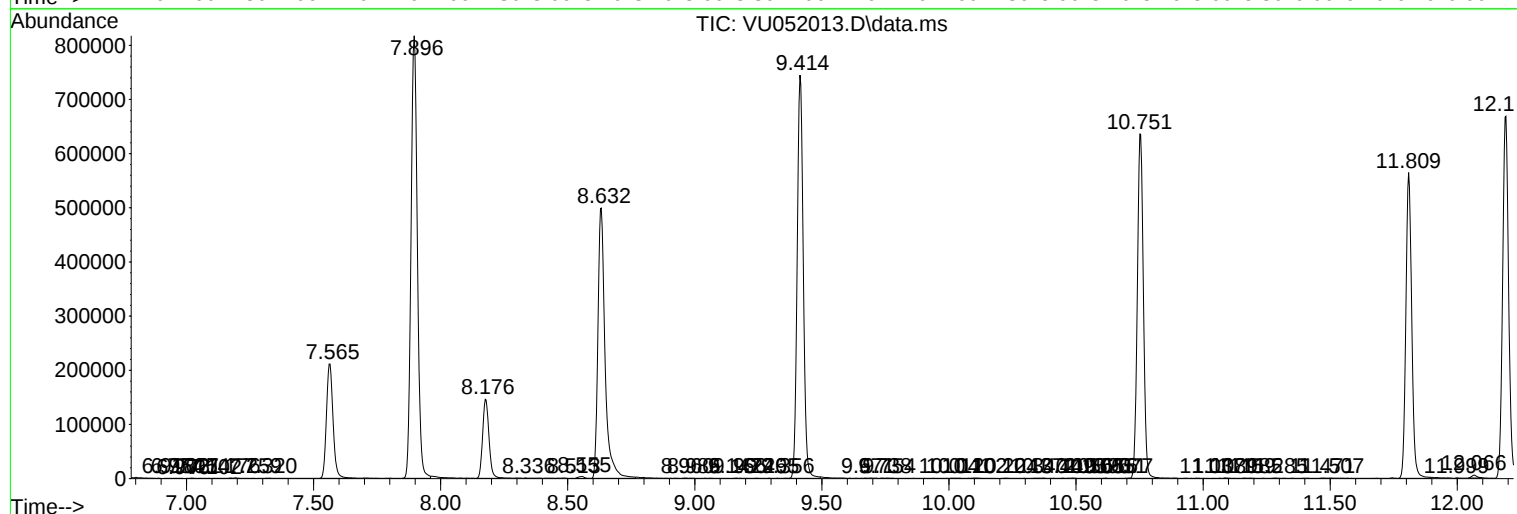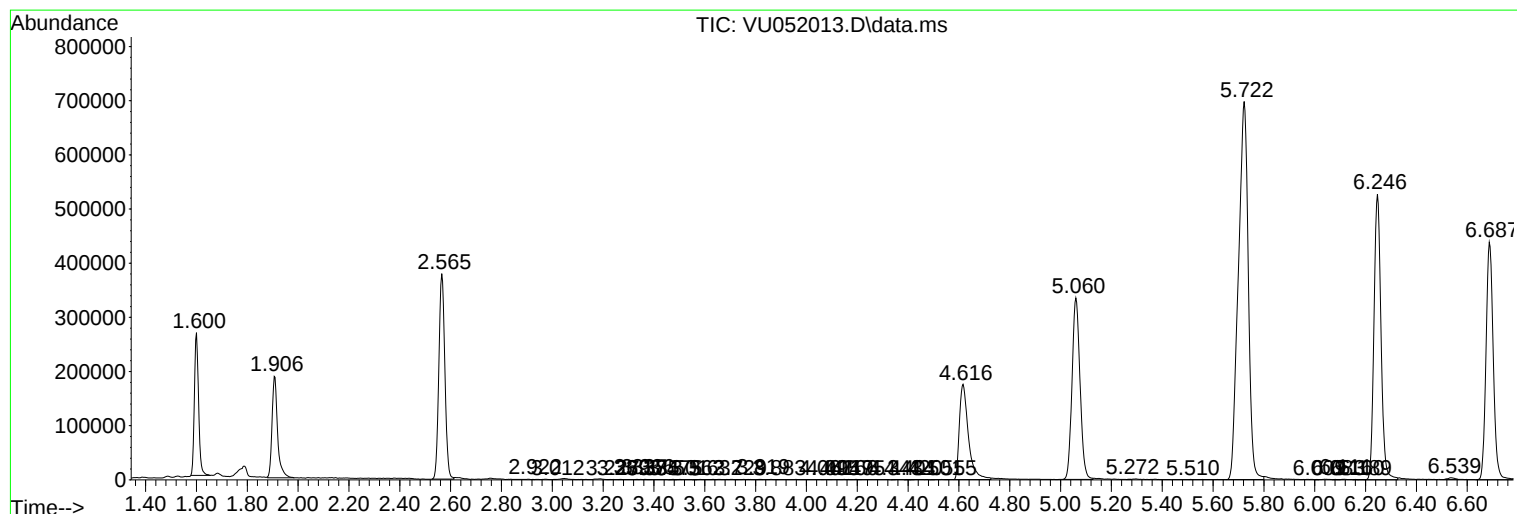

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
Data File : VU052013.D
Acq On : 21 Nov 2022 22:50
Operator : JC/MD
Sample : N5710-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
Data File : VU052013.D
Acq On : 21 Nov 2022 22:50
Operator : JC/MD
Sample : N5710-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc