

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
 Data File : VU052015.D
 Acq On : 21 Nov 2022 23:42
 Operator : JC/MD
 Sample : N5716-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A0B24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

Signal : TIC: VU052015.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	97	rBV	232835	270673	15.54%	2.136%
2	1.906	167	176	197	rVB	172391	255311	14.65%	2.015%
3	2.565	368	381	397	rBV	341636	557740	32.01%	4.402%
4	2.758	438	441	447	rVB2	1382	1189	0.07%	0.009%
5	2.861	468	473	478	rVB2	463	505	0.03%	0.004%
6	2.893	479	483	487	rVB3	302	271	0.02%	0.002%
7	3.041	524	529	538	rBV4	1286	2023	0.12%	0.016%
8	3.080	538	541	546	rVB4	725	650	0.04%	0.005%
9	3.186	561	574	590	rVB	4168	8572	0.49%	0.068%
10	3.366	619	630	639	rVB7	1404	3097	0.18%	0.024%
11	3.697	724	733	750	rVB6	3427	7262	0.42%	0.057%
12	3.764	750	754	755	rBV2	350	211	0.01%	0.002%
13	3.909	793	799	804	rVB2	312	376	0.02%	0.003%
14	4.273	908	912	915	rBV2	272	220	0.01%	0.002%
15	4.533	981	993	1001	rBV5	2787	5188	0.30%	0.041%
16	4.617	1007	1019	1057	rBV	168738	420565	24.14%	3.319%
17	4.916	1109	1112	1117	rVB3	313	273	0.02%	0.002%
18	5.060	1140	1157	1185	rBV	307023	681002	39.09%	5.374%
19	5.279	1220	1225	1226	rBV	806	616	0.04%	0.005%
20	5.295	1228	1230	1235	rVB2	1028	825	0.05%	0.007%
21	5.382	1254	1257	1261	rVB4	458	336	0.02%	0.003%
22	5.449	1274	1278	1280	rBV3	356	244	0.01%	0.002%
23	5.498	1289	1293	1297	rVV2	277	263	0.02%	0.002%
24	5.523	1297	1301	1303	rVV	385	208	0.01%	0.002%
25	5.552	1306	1310	1313	rVV2	272	202	0.01%	0.002%
26	5.723	1340	1363	1394	rBV2	639788	1742208	100.00%	13.749%
27	5.964	1434	1438	1440	rBV3	270	209	0.01%	0.002%
28	6.034	1457	1460	1469	rVB3	841	850	0.05%	0.007%
29	6.073	1469	1472	1474	rBV	356	286	0.02%	0.002%
30	6.247	1512	1526	1549	rBV	509153	981466	56.33%	7.746%
31	6.420	1577	1580	1582	rBV2	401	224	0.01%	0.002%
32	6.536	1604	1616	1629	rVB10	2848	6032	0.35%	0.048%
33	6.597	1629	1635	1640	rBV4	534	715	0.04%	0.006%
34	6.687	1647	1663	1695	rBV	410768	800853	45.97%	6.320%
35	6.964	1744	1749	1750	rBV3	283	212	0.01%	0.002%
36	7.044	1769	1774	1777	rBV3	324	300	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
 Data File : VU052015.D
 Acq On : 21 Nov 2022 23:42
 Operator : JC/MD
 Sample : N5716-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A0B24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

37	7.179	1811	1816	1817	rBV	385	317	0.02%	0.003%
38	7.192	1817	1820	1823	rVV2	391	265	0.02%	0.002%
39	7.459	1900	1903	1909	rVB2	246	206	0.01%	0.002%
40	7.562	1923	1935	1965	rBV	191883	346009	19.86%	2.731%
41	7.729	1984	1987	1989	rVB	469	215	0.01%	0.002%
42	7.800	2006	2009	2016	rVB2	610	559	0.03%	0.004%
43	7.835	2016	2020	2024	rBV2	449	413	0.02%	0.003%
44	7.896	2024	2039	2072	rBV	734993	1284890	73.75%	10.140%
45	8.057	2086	2089	2091	rBV2	429	324	0.02%	0.003%
46	8.176	2115	2126	2147	rBV	137060	231199	13.27%	1.825%
47	8.269	2153	2155	2159	rVB2	367	234	0.01%	0.002%
48	8.378	2186	2189	2192	rBV3	409	205	0.01%	0.002%
49	8.468	2208	2217	2227	rVB4	862	1890	0.11%	0.015%
50	8.552	2237	2243	2251	rBV6	2823	3691	0.21%	0.029%
51	8.632	2255	2268	2304	rBV2	475944	919721	52.79%	7.258%
52	8.867	2336	2341	2343	rVB3	427	293	0.02%	0.002%
53	8.915	2353	2356	2360	rVB	460	341	0.02%	0.003%
54	8.944	2360	2365	2370	rBV3	408	458	0.03%	0.004%
55	9.067	2400	2403	2407	rVB2	392	218	0.01%	0.002%
56	9.208	2444	2447	2453	rVB2	321	258	0.01%	0.002%
57	9.414	2498	2511	2553	rVV	731746	1224253	70.27%	9.662%
58	9.597	2567	2568	2573	rVB3	590	339	0.02%	0.003%
59	9.642	2579	2582	2586	rBV	284	267	0.02%	0.002%
60	9.880	2653	2656	2664	rVB2	207	208	0.01%	0.002%
61	10.105	2723	2726	2730	rBV	325	231	0.01%	0.002%
62	10.333	2794	2797	2799	rBV	339	239	0.01%	0.002%
63	10.369	2803	2808	2813	rBV2	326	425	0.02%	0.003%
64	10.443	2828	2831	2837	rVB	287	227	0.01%	0.002%
65	10.693	2906	2909	2912	rVB	370	222	0.01%	0.002%
66	10.751	2915	2927	2946	rBV	598444	974732	55.95%	7.692%
67	10.886	2964	2969	2971	rBV4	547	542	0.03%	0.004%
68	10.935	2982	2984	2990	rVB2	393	302	0.02%	0.002%
69	11.092	3031	3033	3036	rVB2	567	301	0.02%	0.002%
70	11.465	3144	3149	3150	rBV2	282	232	0.01%	0.002%
71	11.703	3220	3223	3226	rBV2	329	212	0.01%	0.002%
72	11.742	3232	3235	3244	rVB3	468	563	0.03%	0.004%
73	11.809	3244	3256	3282	rBV	547125	887862	50.96%	7.007%
74	12.073	3333	3338	3350	rVB6	1294	1888	0.11%	0.015%
75	12.124	3350	3354	3357	rBV2	291	219	0.01%	0.002%
76	12.189	3361	3374	3400	rBV	621106	1025693	58.87%	8.095%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
 Data File : VU052015.D
 Acq On : 21 Nov 2022 23:42
 Operator : JC/MD
 Sample : N5716-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A0B24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

77	12.343	3420	3422	3423	rBV	471	216	0.01%	0.002%
78	12.391	3435	3437	3439	rBV2	385	207	0.01%	0.002%
79	12.446	3451	3454	3458	rBV2	273	210	0.01%	0.002%
80	12.536	3477	3482	3483	rBV2	342	286	0.02%	0.002%
81	12.629	3506	3511	3516	rVB2	343	383	0.02%	0.003%
82	12.652	3516	3518	3522	rBV	263	209	0.01%	0.002%
83	12.883	3588	3590	3596	rVB3	460	377	0.02%	0.003%
84	13.198	3685	3688	3691	rBV2	327	209	0.01%	0.002%
85	13.343	3730	3733	3737	rBV3	488	371	0.02%	0.003%
86	13.465	3767	3771	3774	rBV2	473	323	0.02%	0.003%
87	13.491	3774	3779	3783	rVV3	462	491	0.03%	0.004%
88	13.600	3809	3813	3815	rBV2	612	490	0.03%	0.004%
89	13.635	3821	3824	3827	rVB	464	266	0.02%	0.002%
90	13.680	3836	3838	3843	rVV	242	254	0.01%	0.002%
91	13.742	3851	3857	3860	rBV2	331	416	0.02%	0.003%
92	13.844	3887	3889	3891	rBV3	611	241	0.01%	0.002%
93	13.960	3920	3925	3927	rBV2	636	543	0.03%	0.004%
94	14.250	4013	4015	4017	rBV2	380	248	0.01%	0.002%
95	14.282	4023	4025	4032	rVB2	529	357	0.02%	0.003%
96	14.340	4037	4043	4050	rBV4	813	1128	0.06%	0.009%
97	14.455	4077	4079	4085	rBV2	361	336	0.02%	0.003%
98	14.941	4227	4230	4234	rBV2	640	613	0.04%	0.005%
99	15.243	4321	4324	4330	rBV3	577	599	0.03%	0.005%
100	15.561	4419	4423	4424	rBV2	773	607	0.03%	0.005%




Sum of corrected areas: 12671220

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
Data File : VU052015.D
Acq On : 21 Nov 2022 23:42
Operator : JC/MD
Sample : N5716-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A0B24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

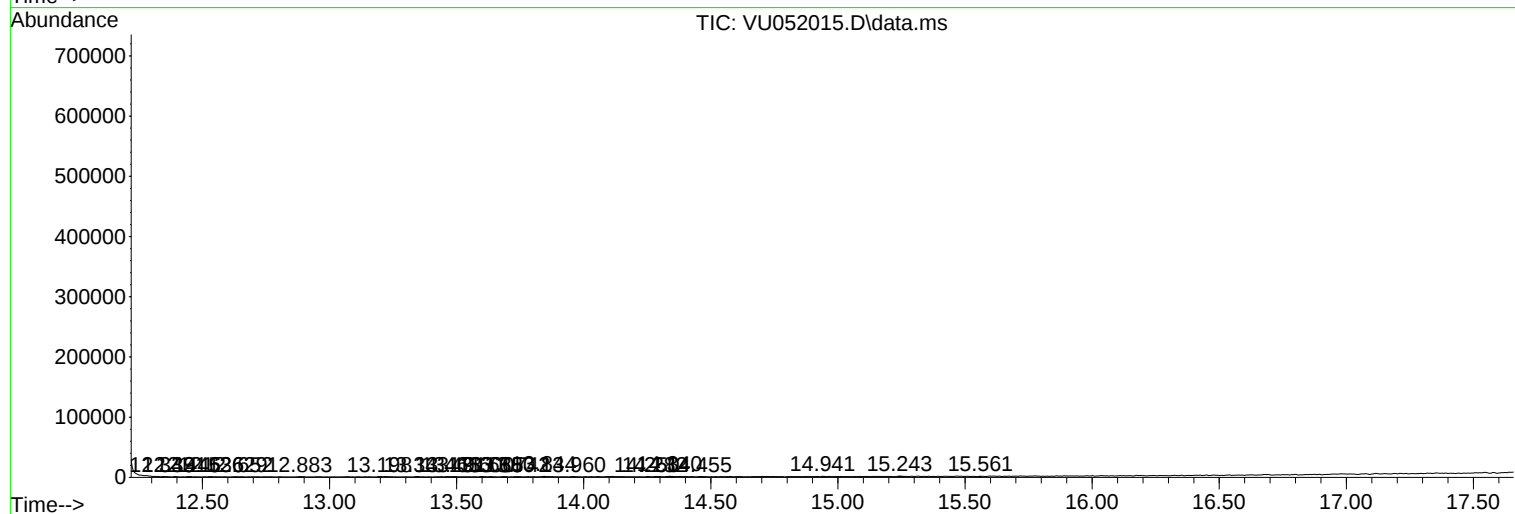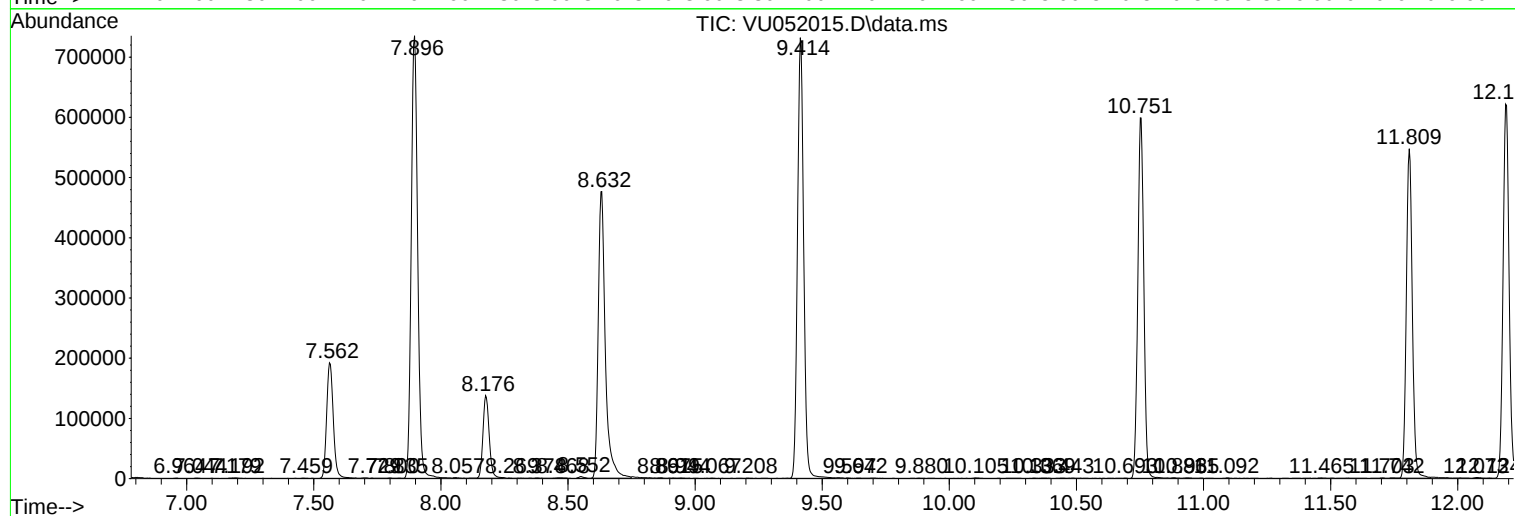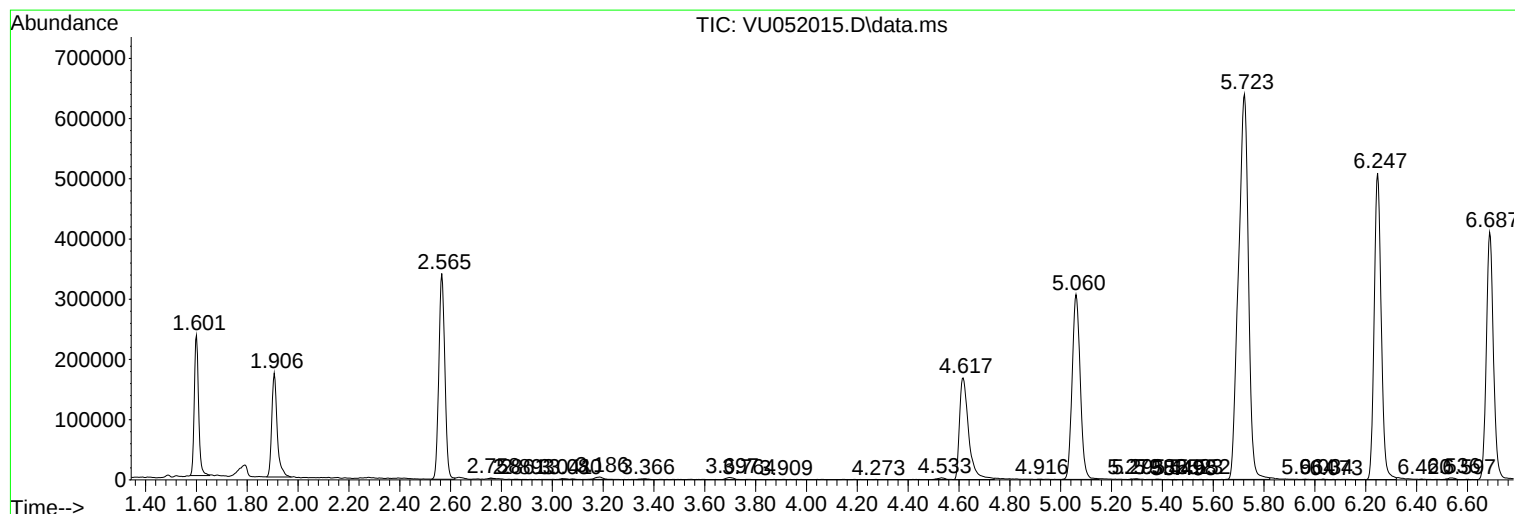

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
Data File : VU052015.D
Acq On : 21 Nov 2022 23:42
Operator : JC/MD
Sample : N5716-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A0B24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
Data File : VU052015.D
Acq On : 21 Nov 2022 23:42
Operator : JC/MD
Sample : N5716-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A0B24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc