

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
 Data File : VU052016.D
 Acq On : 22 Nov 2022 00:07
 Operator : JC/MD
 Sample : N5716-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A0B25

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

Signal : TIC: VU052016.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	102	rBV	235308	279409	15.79%	2.180%
2	1.903	167	175	205	rVB	170858	263531	14.89%	2.056%
3	2.565	368	381	395	rBV	347404	561748	31.74%	4.383%
4	2.736	430	434	437	rBV3	473	426	0.02%	0.003%
5	2.765	439	443	445	rBV2	701	597	0.03%	0.005%
6	2.829	461	463	470	rBV2	296	260	0.01%	0.002%
7	2.941	493	498	499	rBV	352	251	0.01%	0.002%
8	3.041	522	529	542	rVB7	1572	3516	0.20%	0.027%
9	3.096	542	546	551	rBV2	267	257	0.01%	0.002%
10	3.176	561	571	573	rBV3	4207	5187	0.29%	0.040%
11	3.311	610	613	618	rVB2	348	276	0.02%	0.002%
12	3.395	636	639	643	rVB2	370	293	0.02%	0.002%
13	3.575	690	695	696	rBV	238	207	0.01%	0.002%
14	3.671	722	725	731	rVB3	219	208	0.01%	0.002%
15	3.723	738	741	746	rVB2	400	301	0.02%	0.002%
16	3.755	746	751	755	rBV2	311	286	0.02%	0.002%
17	4.353	933	937	940	rVB2	301	258	0.01%	0.002%
18	4.617	1003	1019	1058	rBV	171061	420621	23.77%	3.282%
19	5.060	1139	1157	1179	rBV	323682	720741	40.72%	5.623%
20	5.285	1221	1227	1228	rBV2	989	937	0.05%	0.007%
21	5.417	1264	1268	1273	rBV	261	223	0.01%	0.002%
22	5.491	1286	1291	1293	rBV3	373	266	0.02%	0.002%
23	5.723	1340	1363	1392	rBV2	653022	1769875	100.00%	13.809%
24	6.034	1458	1460	1464	rVB2	331	208	0.01%	0.002%
25	6.195	1505	1510	1512	rBV2	289	276	0.02%	0.002%
26	6.247	1512	1526	1548	rBV	524890	984180	55.61%	7.679%
27	6.430	1581	1583	1586	rVB3	494	237	0.01%	0.002%
28	6.533	1607	1615	1629	rVB8	2940	5329	0.30%	0.042%
29	6.594	1629	1634	1637	rBV2	241	246	0.01%	0.002%
30	6.623	1641	1643	1648	rVB2	347	222	0.01%	0.002%
31	6.687	1648	1663	1689	rBV	412597	808663	45.69%	6.309%
32	6.877	1718	1722	1726	rVB2	318	256	0.01%	0.002%
33	6.996	1756	1759	1764	rBV	328	303	0.02%	0.002%
34	7.028	1765	1769	1773	rVV	418	317	0.02%	0.002%
35	7.099	1787	1791	1794	rBV2	381	341	0.02%	0.003%
36	7.195	1813	1821	1823	rBV5	777	1011	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
 Data File : VU052016.D
 Acq On : 22 Nov 2022 00:07
 Operator : JC/MD
 Sample : N5716-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A0B25

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

37	7.407	1884	1887	1893	rVB2	262	307	0.02%	0.002%
38	7.562	1922	1935	1958	rBV	198051	350291	19.79%	2.733%
39	7.764	1995	1998	2000	rVB2	398	204	0.01%	0.002%
40	7.809	2010	2012	2017	rVB2	489	337	0.02%	0.003%
41	7.896	2022	2039	2062	rBV	751069	1301756	73.55%	10.157%
42	8.083	2095	2097	2100	rBV3	403	282	0.02%	0.002%
43	8.176	2114	2126	2143	rBV	139102	233875	13.21%	1.825%
44	8.465	2208	2216	2219	rBV4	836	971	0.05%	0.008%
45	8.549	2236	2242	2252	rBV7	2278	3306	0.19%	0.026%
46	8.629	2255	2267	2304	rBV2	480749	938164	53.01%	7.320%
47	8.999	2379	2382	2389	rVB2	318	353	0.02%	0.003%
48	9.063	2398	2402	2405	rVV3	419	289	0.02%	0.002%
49	9.163	2430	2433	2437	rVB4	380	253	0.01%	0.002%
50	9.202	2441	2445	2448	rVB2	322	240	0.01%	0.002%
51	9.414	2497	2511	2531	rBV	743776	1212472	68.51%	9.460%
52	9.645	2581	2583	2587	rVB2	628	423	0.02%	0.003%
53	9.703	2596	2601	2606	rVB2	639	686	0.04%	0.005%
54	9.790	2623	2628	2631	rVB	338	291	0.02%	0.002%
55	9.819	2631	2637	2639	rBV	272	314	0.02%	0.002%
56	9.857	2645	2649	2652	rBV2	334	278	0.02%	0.002%
57	10.073	2713	2716	2720	rBV2	270	227	0.01%	0.002%
58	10.311	2787	2790	2794	rVB	292	224	0.01%	0.002%
59	10.369	2802	2808	2810	rBV	242	219	0.01%	0.002%
60	10.420	2820	2824	2827	rBV2	412	337	0.02%	0.003%
61	10.478	2837	2842	2844	rBV2	427	392	0.02%	0.003%
62	10.513	2850	2853	2859	rBV2	206	238	0.01%	0.002%
63	10.568	2866	2870	2874	rVB2	311	267	0.02%	0.002%
64	10.677	2902	2904	2909	rVB2	352	269	0.02%	0.002%
65	10.751	2910	2927	2951	rBV	624406	1002281	56.63%	7.820%
66	10.883	2965	2968	2971	rVB3	586	365	0.02%	0.003%
67	10.996	3001	3003	3007	rVV2	314	223	0.01%	0.002%
68	11.041	3013	3017	3024	rBV2	305	364	0.02%	0.003%
69	11.095	3028	3034	3037	rBV3	483	477	0.03%	0.004%
70	11.324	3100	3105	3108	rBV2	422	375	0.02%	0.003%
71	11.446	3140	3143	3145	rBV2	357	206	0.01%	0.002%
72	11.481	3150	3154	3158	rVB3	619	517	0.03%	0.004%
73	11.507	3158	3162	3164	rBV	330	260	0.01%	0.002%
74	11.571	3178	3182	3185	rVB2	401	307	0.02%	0.002%
75	11.594	3185	3189	3192	rBV2	321	274	0.02%	0.002%
76	11.674	3211	3214	3217	rVB	369	207	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
 Data File : VU052016.D
 Acq On : 22 Nov 2022 00:07
 Operator : JC/MD
 Sample : N5716-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A0B25

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

77	11.732	3223	3232	3234	rBV	557	631	0.04%	0.005%
78	11.745	3234	3236	3241	rVB2	560	360	0.02%	0.003%
79	11.809	3243	3256	3282	rBV	552162	885668	50.04%	6.910%
80	11.996	3311	3314	3317	rBV3	393	284	0.02%	0.002%
81	12.054	3330	3332	3335	rBV2	299	226	0.01%	0.002%
82	12.189	3360	3374	3398	rBV	615348	1038378	58.67%	8.102%
83	12.407	3439	3442	3445	rBV2	357	250	0.01%	0.002%
84	12.472	3459	3462	3465	rBV2	314	252	0.01%	0.002%
85	12.536	3478	3482	3489	rVB4	566	563	0.03%	0.004%
86	12.751	3545	3549	3553	rBV	247	281	0.02%	0.002%
87	13.005	3624	3628	3630	rBV2	452	259	0.01%	0.002%
88	13.217	3691	3694	3696	rBV2	426	314	0.02%	0.002%
89	13.291	3714	3717	3720	rBV	319	220	0.01%	0.002%
90	13.542	3793	3795	3799	rVB2	559	346	0.02%	0.003%
91	13.571	3800	3804	3806	rBV	479	339	0.02%	0.003%
92	13.713	3845	3848	3852	rBV2	297	273	0.02%	0.002%
93	13.848	3886	3890	3898	rBV5	787	1094	0.06%	0.009%
94	13.928	3912	3915	3919	rBV3	368	315	0.02%	0.002%
95	14.262	4016	4019	4022	rVB	657	380	0.02%	0.003%
96	14.414	4063	4066	4068	rBV3	370	259	0.01%	0.002%
97	14.790	4179	4183	4186	rBV2	558	519	0.03%	0.004%
98	15.053	4262	4265	4267	rBV2	587	346	0.02%	0.003%
99	15.696	4463	4465	4468	rBV3	659	408	0.02%	0.003%
100	15.725	4472	4474	4476	rBV	549	254	0.01%	0.002%




Sum of corrected areas: 12816603

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
Data File : VU052016.D
Acq On : 22 Nov 2022 00:07
Operator : JC/MD
Sample : N5716-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A0B25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

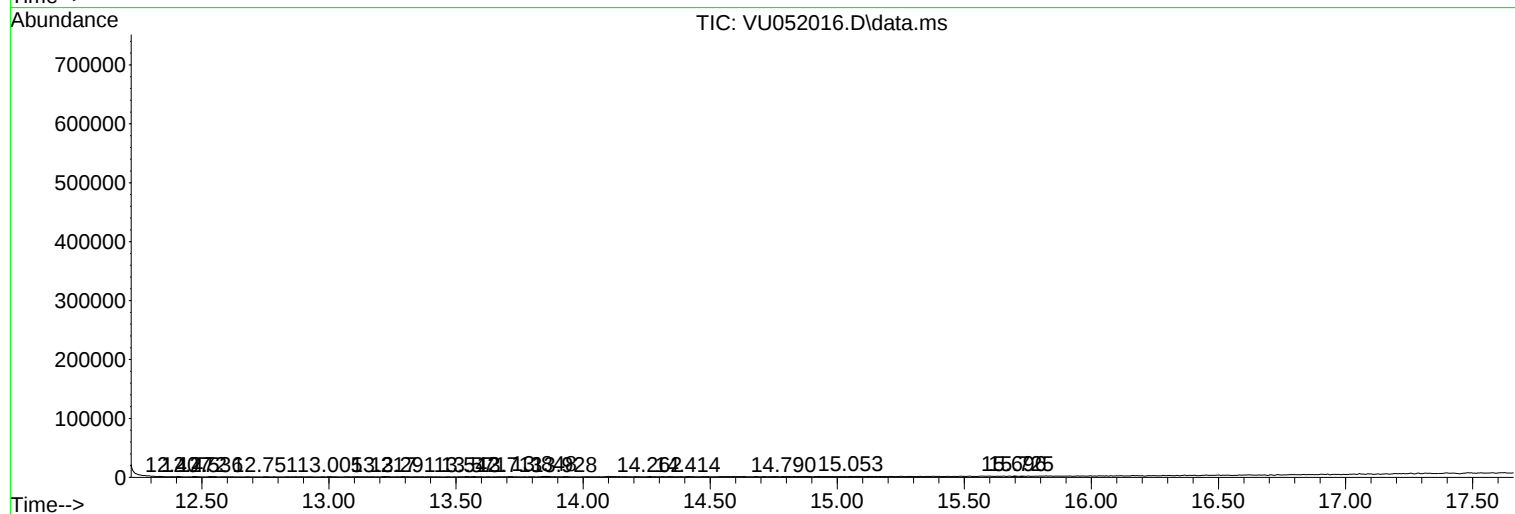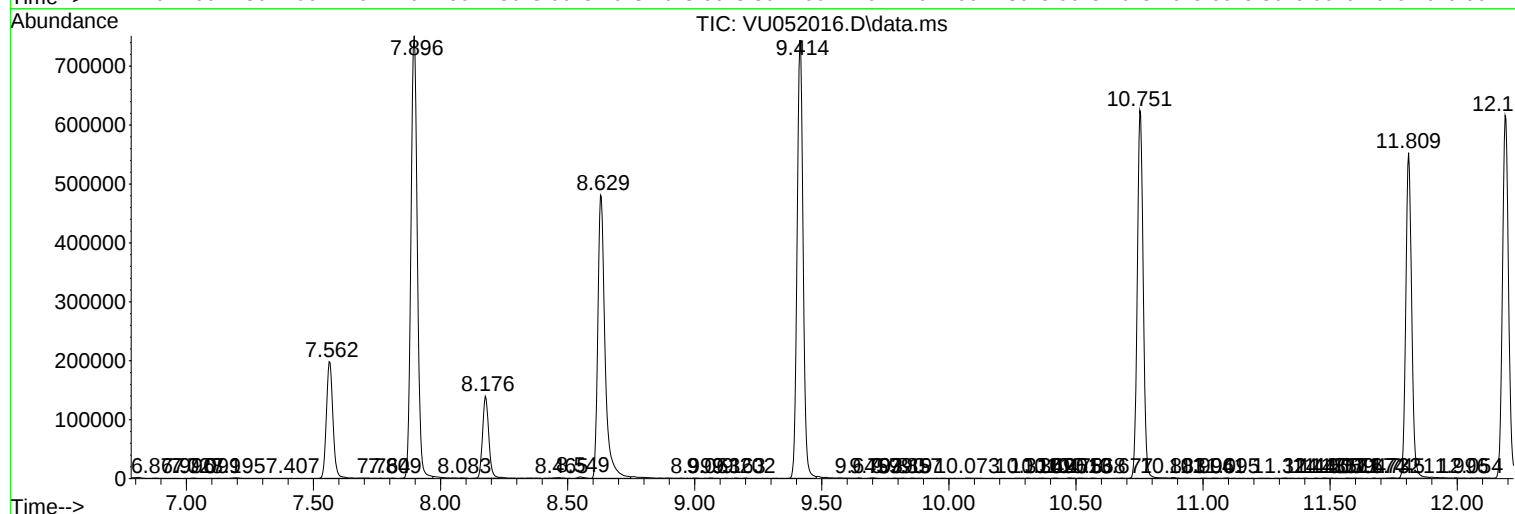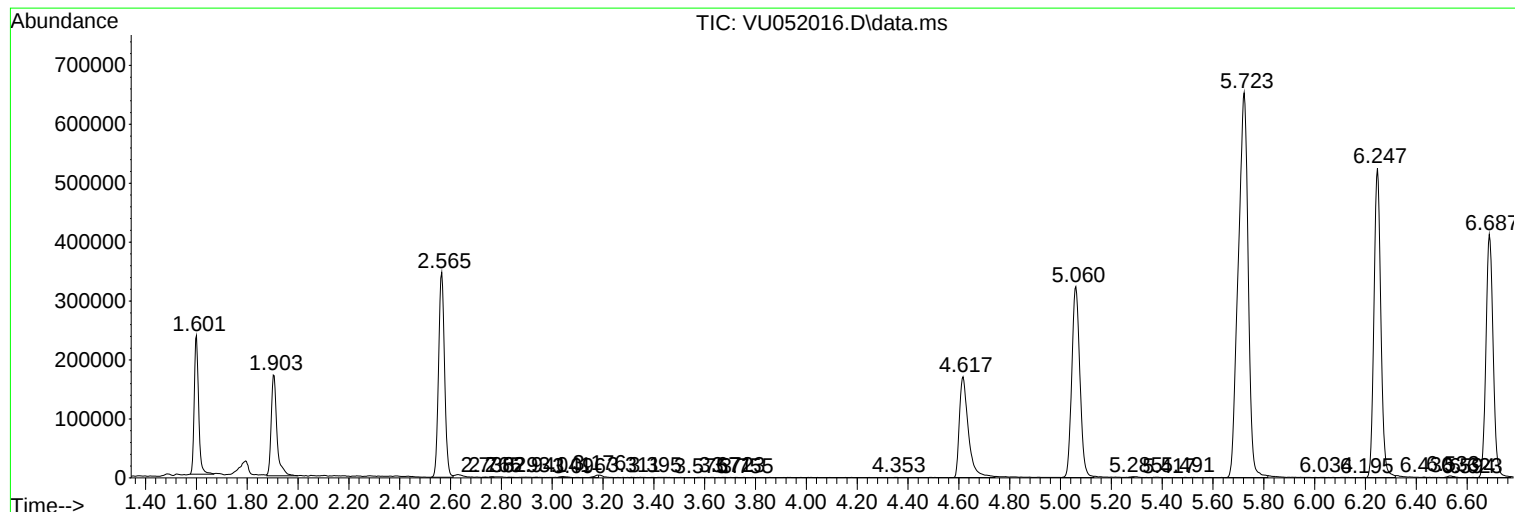

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
Data File : VU052016.D
Acq On : 22 Nov 2022 00:07
Operator : JC/MD
Sample : N5716-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A0B25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
Data File : VU052016.D
Acq On : 22 Nov 2022 00:07
Operator : JC/MD
Sample : N5716-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A0B25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------