

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
 Data File : VU052018.D
 Acq On : 22 Nov 2022 01:00
 Operator : JC/MD
 Sample : N5737-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4346

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M

Title : VOC Analysis

Signal : TIC: VU052018.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	97	rVB	232038	269648	15.16%	2.032%
2	1.906	168	176	199	rVB	170346	254464	14.31%	1.917%
3	2.375	315	322	338	rVB	32467	49238	2.77%	0.371%
4	2.565	368	381	394	rBV	337027	552382	31.06%	4.162%
5	2.845	464	468	474	rVB2	405	419	0.02%	0.003%
6	2.922	490	492	494	rBV	341	211	0.01%	0.002%
7	2.964	501	505	507	rBV2	499	433	0.02%	0.003%
8	3.031	523	526	529	rBV3	896	760	0.04%	0.006%
9	3.083	539	542	545	rBV2	400	253	0.01%	0.002%
10	3.118	551	553	555	rBV	284	156	0.01%	0.001%
11	3.179	556	572	589	rVV	62745	144971	8.15%	1.092%
12	3.588	696	699	701	rBV2	308	219	0.01%	0.002%
13	3.655	717	720	725	rVB2	331	211	0.01%	0.002%
14	3.687	725	730	732	rBV2	363	273	0.02%	0.002%
15	3.777	753	758	761	rBV3	337	286	0.02%	0.002%
16	3.813	766	769	772	rBV	203	208	0.01%	0.002%
17	3.858	781	783	786	rBV3	378	191	0.01%	0.001%
18	3.874	786	788	791	rVV2	304	177	0.01%	0.001%
19	3.993	815	825	838	rVB3	1171	2779	0.16%	0.021%
20	4.051	838	843	845	rBV2	245	225	0.01%	0.002%
21	4.166	875	879	881	rBV2	261	163	0.01%	0.001%
22	4.273	908	912	918	rBV2	279	287	0.02%	0.002%
23	4.305	918	922	924	rBV2	363	208	0.01%	0.002%
24	4.359	935	939	944	rVB2	207	230	0.01%	0.002%
25	4.398	948	951	956	rBV2	192	201	0.01%	0.002%
26	4.617	1002	1019	1046	rBV	176708	435737	24.50%	3.283%
27	5.060	1140	1157	1179	rBV	325672	724411	40.73%	5.458%
28	5.269	1219	1222	1223	rBV2	350	190	0.01%	0.001%
29	5.289	1223	1228	1229	rBV	799	627	0.04%	0.005%
30	5.327	1238	1240	1242	rBV	377	179	0.01%	0.001%
31	5.340	1242	1244	1248	rVV4	300	244	0.01%	0.002%
32	5.575	1313	1317	1319	rBV2	249	205	0.01%	0.002%
33	5.588	1319	1321	1327	rVB2	515	360	0.02%	0.003%
34	5.723	1341	1363	1394	rBV2	647953	1778416	100.00%	13.400%
35	5.944	1429	1432	1433	rBV2	439	254	0.01%	0.002%
36	6.102	1478	1481	1483	rVB2	427	242	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
 Data File : VU052018.D
 Acq On : 22 Nov 2022 01:00
 Operator : JC/MD
 Sample : N5737-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4346

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

37	6.118	1483	1486	1490	rBV3	456	384	0.02%	0.003%
38	6.163	1498	1500	1505	rVB3	416	175	0.01%	0.001%
39	6.192	1505	1509	1512	rBV	252	237	0.01%	0.002%
40	6.247	1512	1526	1560	rBV	521297	996521	56.03%	7.509%
41	6.462	1591	1593	1597	rBV	394	326	0.02%	0.002%
42	6.687	1649	1663	1683	rBV	410677	798078	44.88%	6.013%
43	6.854	1713	1715	1720	rVB2	374	301	0.02%	0.002%
44	6.883	1720	1724	1725	rBV2	343	181	0.01%	0.001%
45	6.961	1738	1748	1765	rBV2	20726	39816	2.24%	0.300%
46	7.141	1799	1804	1806	rVB2	261	163	0.01%	0.001%
47	7.163	1806	1811	1813	rBV2	517	406	0.02%	0.003%
48	7.282	1841	1848	1853	rBV	379	368	0.02%	0.003%
49	7.362	1867	1873	1876	rBV2	220	202	0.01%	0.002%
50	7.562	1920	1935	1961	rBV2	196013	351423	19.76%	2.648%
51	7.732	1985	1988	1992	rVB4	609	366	0.02%	0.003%
52	7.755	1992	1995	1997	rBV2	481	322	0.02%	0.002%
53	7.800	2004	2009	2014	rBV3	456	545	0.03%	0.004%
54	7.848	2021	2024	2025	rBV2	336	174	0.01%	0.001%
55	7.896	2025	2039	2068	rVV	756350	1305052	73.38%	9.833%
56	8.176	2115	2126	2148	rBV	135384	230351	12.95%	1.736%
57	8.346	2176	2179	2181	rBV2	402	278	0.02%	0.002%
58	8.382	2187	2190	2195	rVB3	544	441	0.02%	0.003%
59	8.404	2195	2197	2201	rBV3	393	321	0.02%	0.002%
60	8.488	2213	2223	2232	rVB7	3151	6515	0.37%	0.049%
61	8.546	2237	2241	2242	rBV2	1715	1130	0.06%	0.009%
62	8.629	2256	2267	2301	rBV3	457712	897646	50.47%	6.764%
63	8.928	2359	2360	2367	rVB2	445	285	0.02%	0.002%
64	8.960	2367	2370	2374	rBV2	447	314	0.02%	0.002%
65	8.999	2379	2382	2384	rVV2	298	227	0.01%	0.002%
66	9.121	2417	2420	2422	rBV	352	223	0.01%	0.002%
67	9.266	2459	2465	2467	rBV2	493	489	0.03%	0.004%
68	9.337	2484	2487	2489	rBV3	392	235	0.01%	0.002%
69	9.414	2497	2511	2547	rBV	740273	1280290	71.99%	9.647%
70	9.632	2577	2579	2582	rBV2	354	214	0.01%	0.002%
71	9.694	2590	2598	2610	rVB3	6467	11191	0.63%	0.084%
72	9.758	2610	2618	2628	rBV5	3214	4947	0.28%	0.037%
73	9.796	2628	2630	2633	rVB2	325	181	0.01%	0.001%
74	9.925	2667	2670	2674	rBV2	180	150	0.01%	0.001%
75	10.031	2698	2703	2705	rBV	325	284	0.02%	0.002%
76	10.099	2717	2724	2733	rBV3	2565	3751	0.21%	0.028%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
 Data File : VU052018.D
 Acq On : 22 Nov 2022 01:00
 Operator : JC/MD
 Sample : N5737-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4346

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

77	10.179	2745	2749	2751	rBV2	461	310	0.02%	0.002%
78	10.484	2835	2844	2853	rVV2	11484	17889	1.01%	0.135%
79	10.751	2914	2927	2947	rBV	602379	978188	55.00%	7.370%
80	10.899	2966	2973	2974	rBV5	3765	3494	0.20%	0.026%
81	11.089	3029	3032	3036	rVB2	764	516	0.03%	0.004%
82	11.134	3044	3046	3051	rVB3	1060	766	0.04%	0.006%
83	11.237	3072	3078	3080	rBV2	257	281	0.02%	0.002%
84	11.407	3123	3131	3133	rBV4	708	721	0.04%	0.005%
85	11.584	3182	3186	3187	rBV3	482	306	0.02%	0.002%
86	11.745	3230	3236	3242	rVB5	995	1239	0.07%	0.009%
87	11.809	3243	3256	3278	rBV	593672	967331	54.39%	7.289%
88	12.002	3313	3316	3325	rVB3	1464	1785	0.10%	0.013%
89	12.063	3325	3335	3337	rBV3	8398	9725	0.55%	0.073%
90	12.189	3361	3374	3401	rBV	673571	1102404	61.99%	8.306%
91	12.362	3426	3428	3431	rBV2	863	598	0.03%	0.005%
92	12.571	3484	3493	3501	rBV2	5986	9379	0.53%	0.071%
93	12.681	3518	3527	3531	rBV7	3099	4597	0.26%	0.035%
94	12.764	3550	3553	3555	rBV	332	273	0.02%	0.002%
95	12.970	3610	3617	3625	rVB3	5805	7253	0.41%	0.055%
96	13.025	3631	3634	3636	rBV2	410	248	0.01%	0.002%
97	13.124	3660	3665	3668	rBV3	495	561	0.03%	0.004%
98	13.301	3712	3720	3726	rBV3	1503	2206	0.12%	0.017%
99	13.365	3737	3740	3742	rBV	480	223	0.01%	0.002%
100	13.452	3761	3767	3778	rVB4	5098	7608	0.43%	0.057%




Sum of corrected areas: 13271862

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
Data File : VU052018.D
Acq On : 22 Nov 2022 01:00
Operator : JC/MD
Sample : N5737-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4346

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

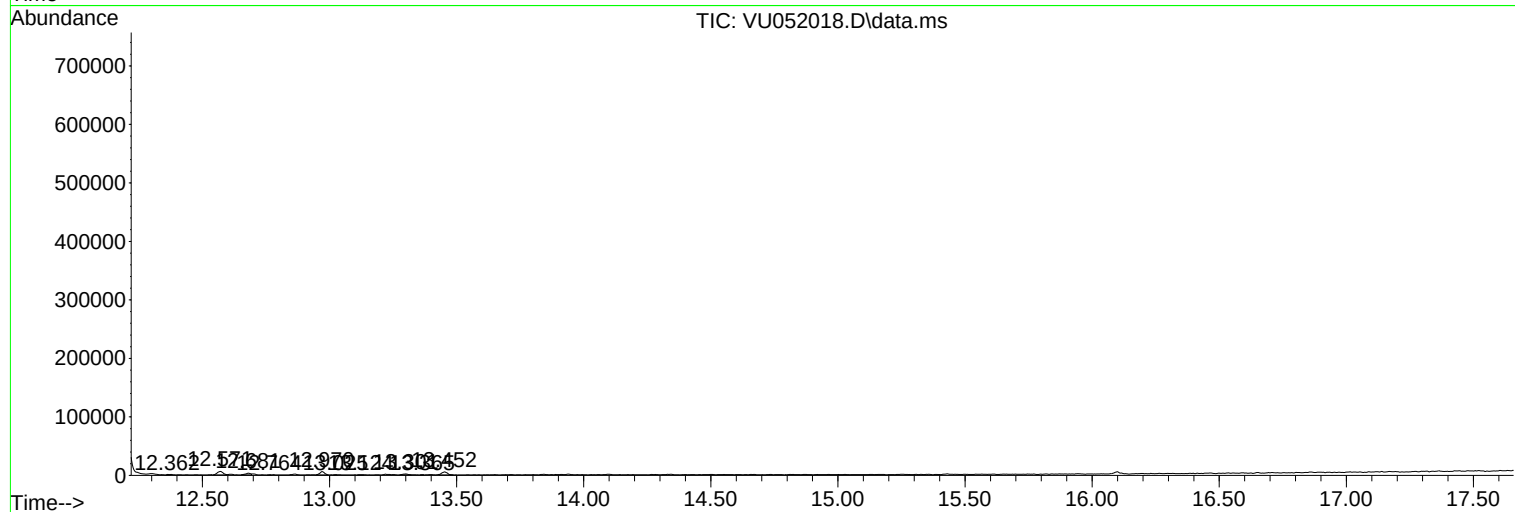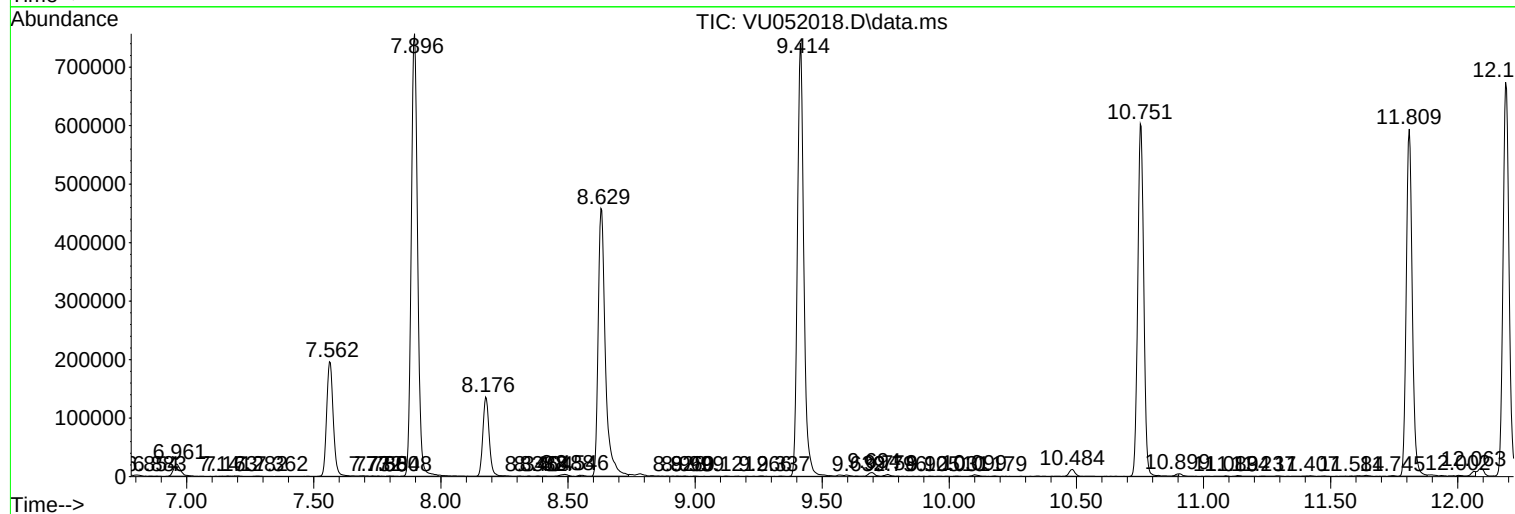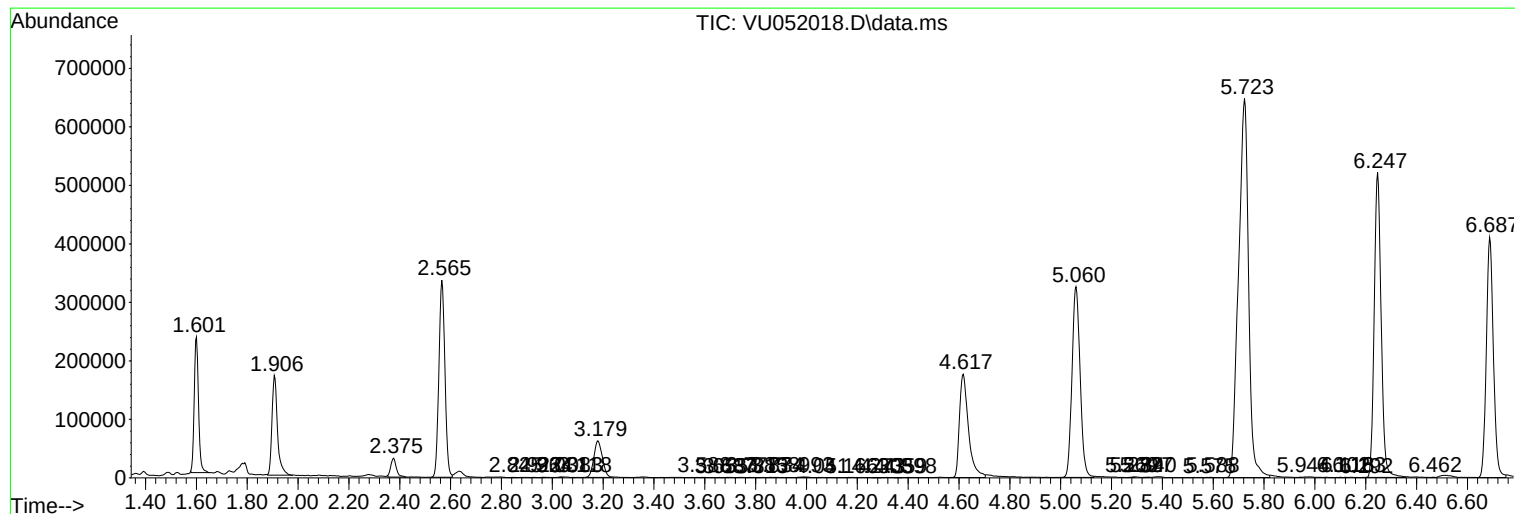

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
Data File : VU052018.D
Acq On : 22 Nov 2022 01:00
Operator : JC/MD
Sample : N5737-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4346

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
Data File : VU052018.D
Acq On : 22 Nov 2022 01:00
Operator : JC/MD
Sample : N5737-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4346

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc