

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
 Data File : VU052019.D
 Acq On : 22 Nov 2022 01:26
 Operator : JC/MD
 Sample : N5737-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4347

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

Signal : TIC: VU052019.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.395	13	17	24	rVB	8647	8231	0.47%	0.061%
2	1.601	72	81	96	rBV	233810	273174	15.46%	2.035%
3	1.906	168	176	197	rVB	170430	256898	14.54%	1.914%
4	2.376	313	322	338	rVB	30934	47210	2.67%	0.352%
5	2.565	367	381	392	rBV	334308	546153	30.90%	4.068%
6	2.623	392	399	422	rVB2	49728	96533	5.46%	0.719%
7	2.954	492	502	514	rBV3	4477	8935	0.51%	0.067%
8	3.048	523	531	542	rBV5	1458	2639	0.15%	0.020%
9	3.179	553	572	598	rBV2	74579	176237	9.97%	1.313%
10	3.347	621	624	626	rBV3	442	372	0.02%	0.003%
11	3.359	626	628	635	rVB5	1000	906	0.05%	0.007%
12	3.970	814	818	819	rBV2	647	415	0.02%	0.003%
13	3.990	820	824	826	rBV4	600	568	0.03%	0.004%
14	4.186	882	885	888	rBV	339	290	0.02%	0.002%
15	4.305	916	922	926	rVB2	258	306	0.02%	0.002%
16	4.350	933	936	943	rVB2	290	319	0.02%	0.002%
17	4.527	988	991	997	rVB3	635	604	0.03%	0.004%
18	4.617	1005	1019	1051	rBV2	176938	447008	25.29%	3.330%
19	4.906	1105	1109	1111	rBV2	296	245	0.01%	0.002%
20	5.060	1141	1157	1179	rBV	331313	734716	41.57%	5.473%
21	5.327	1237	1240	1246	rBV3	408	521	0.03%	0.004%
22	5.385	1250	1258	1268	rVB7	1627	2969	0.17%	0.022%
23	5.723	1339	1363	1390	rBV2	637834	1767251	100.00%	13.164%
24	5.967	1435	1439	1452	rVB3	1651	2165	0.12%	0.016%
25	6.015	1452	1454	1456	rVV	449	259	0.01%	0.002%
26	6.041	1460	1462	1466	rVB3	704	380	0.02%	0.003%
27	6.099	1475	1480	1484	rBV3	412	420	0.02%	0.003%
28	6.134	1488	1491	1497	rVV4	493	474	0.03%	0.004%
29	6.247	1512	1526	1548	rBV	516055	979102	55.40%	7.293%
30	6.501	1596	1605	1608	rBV4	5320	7391	0.42%	0.055%
31	6.687	1643	1663	1682	rBV	402324	783879	44.36%	5.839%
32	6.964	1739	1749	1774	rVB2	17369	35259	2.00%	0.263%
33	7.192	1814	1820	1830	rBV5	980	1637	0.09%	0.012%
34	7.308	1853	1856	1863	rBV	265	266	0.02%	0.002%
35	7.340	1863	1866	1870	rBV2	267	267	0.02%	0.002%
36	7.562	1923	1935	1953	rBV	193756	347200	19.65%	2.586%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
 Data File : VU052019.D
 Acq On : 22 Nov 2022 01:26
 Operator : JC/MD
 Sample : N5737-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4347

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

37	7.690	1973	1975	1980	rBV5	421	304	0.02%	0.002%
38	7.896	2025	2039	2059	rBV	748673	1283126	72.61%	9.557%
39	8.176	2114	2126	2144	rBV2	134640	232864	13.18%	1.735%
40	8.485	2211	2222	2232	rVV7	4227	6999	0.40%	0.052%
41	8.546	2237	2241	2250	rBV4	1615	2282	0.13%	0.017%
42	8.629	2256	2267	2300	rBV2	453785	889972	50.36%	6.629%
43	8.845	2331	2334	2337	rBV2	293	241	0.01%	0.002%
44	8.922	2355	2358	2362	rBV2	408	343	0.02%	0.003%
45	8.996	2377	2381	2384	rBV3	309	244	0.01%	0.002%
46	9.112	2414	2417	2422	rVB2	399	291	0.02%	0.002%
47	9.166	2428	2434	2438	rBV2	598	689	0.04%	0.005%
48	9.272	2463	2467	2470	rVV3	909	818	0.05%	0.006%
49	9.337	2483	2487	2489	rBV2	558	463	0.03%	0.003%
50	9.414	2498	2511	2540	rBV	723851	1275706	72.19%	9.502%
51	9.578	2554	2562	2565	rBV4	2346	3332	0.19%	0.025%
52	9.694	2587	2598	2608	rBV3	8618	14484	0.82%	0.108%
53	9.755	2608	2617	2625	rVV3	4107	6692	0.38%	0.050%
54	9.835	2637	2642	2644	rBV2	722	761	0.04%	0.006%
55	10.015	2696	2698	2702	rVB2	369	252	0.01%	0.002%
56	10.050	2705	2709	2713	rVV4	342	399	0.02%	0.003%
57	10.105	2713	2726	2738	rVV5	3145	5559	0.31%	0.041%
58	10.481	2834	2843	2855	rVB2	15381	24816	1.40%	0.185%
59	10.542	2860	2862	2869	rVB2	445	402	0.02%	0.003%
60	10.703	2907	2912	2913	rBV3	453	323	0.02%	0.002%
61	10.751	2914	2927	2948	rBV	606568	974329	55.13%	7.257%
62	10.906	2965	2975	2984	rVB3	5662	9256	0.52%	0.069%
63	11.140	3043	3048	3055	rVB5	757	888	0.05%	0.007%
64	11.295	3090	3096	3099	rBV3	1040	1014	0.06%	0.008%
65	11.414	3130	3133	3134	rBV2	724	369	0.02%	0.003%
66	11.465	3144	3149	3155	rBV2	462	603	0.03%	0.004%
67	11.555	3171	3177	3180	rBV4	796	885	0.05%	0.007%
68	11.610	3189	3194	3197	rBV2	814	850	0.05%	0.006%
69	11.636	3198	3202	3218	rVB7	2803	4311	0.24%	0.032%
70	11.809	3243	3256	3278	rBV	585494	966705	54.70%	7.201%
71	12.002	3309	3316	3317	rBV4	1207	1207	0.07%	0.009%
72	12.063	3326	3335	3338	rBV3	9201	12592	0.71%	0.094%
73	12.189	3362	3374	3402	rBV	659845	1101929	62.35%	8.208%
74	12.353	3423	3425	3427	rBV2	497	291	0.02%	0.002%
75	12.382	3430	3434	3439	rVB5	779	791	0.04%	0.006%
76	12.571	3484	3493	3499	rBV3	9569	13849	0.78%	0.103%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
 Data File : VU052019.D
 Acq On : 22 Nov 2022 01:26
 Operator : JC/MD
 Sample : N5737-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4347

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

77	12.681	3520	3527	3540	rVV3	4658	6825	0.39%	0.051%
78	12.841	3573	3577	3578	rBV2	432	275	0.02%	0.002%
79	12.864	3578	3584	3591	rVB3	1318	1623	0.09%	0.012%
80	12.896	3591	3594	3596	rBV2	578	432	0.02%	0.003%
81	12.935	3603	3606	3609	rBV	495	422	0.02%	0.003%
82	12.973	3610	3618	3628	rVB4	7045	11350	0.64%	0.085%
83	13.018	3629	3632	3637	rBV2	549	443	0.03%	0.003%
84	13.291	3711	3717	3727	rBV5	2210	3254	0.18%	0.024%
85	13.407	3751	3753	3759	rVB3	759	592	0.03%	0.004%
86	13.452	3759	3767	3777	rBV6	6849	10053	0.57%	0.075%
87	13.761	3859	3863	3866	rBV	570	515	0.03%	0.004%
88	13.848	3887	3890	3896	rVB4	998	945	0.05%	0.007%
89	13.877	3896	3899	3901	rBV3	494	279	0.02%	0.002%
90	13.893	3901	3904	3906	rBV3	440	290	0.02%	0.002%
91	13.909	3906	3909	3912	rBV2	548	276	0.02%	0.002%
92	13.938	3915	3918	3920	rBV2	577	393	0.02%	0.003%
93	14.028	3942	3946	3950	rBV2	397	393	0.02%	0.003%
94	14.282	4023	4025	4029	rBV2	395	245	0.01%	0.002%
95	14.635	4133	4135	4139	rBV3	309	240	0.01%	0.002%
96	14.806	4183	4188	4191	rBV4	787	838	0.05%	0.006%
97	14.976	4238	4241	4243	rBV3	525	368	0.02%	0.003%
98	15.346	4354	4356	4359	rBV2	513	349	0.02%	0.003%
99	15.410	4373	4376	4378	rBV2	1049	826	0.05%	0.006%
100	16.092	4581	4588	4600	rBV3	7456	11708	0.66%	0.087%




Sum of corrected areas: 13425364

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
Data File : VU052019.D
Acq On : 22 Nov 2022 01:26
Operator : JC/MD
Sample : N5737-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4347

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

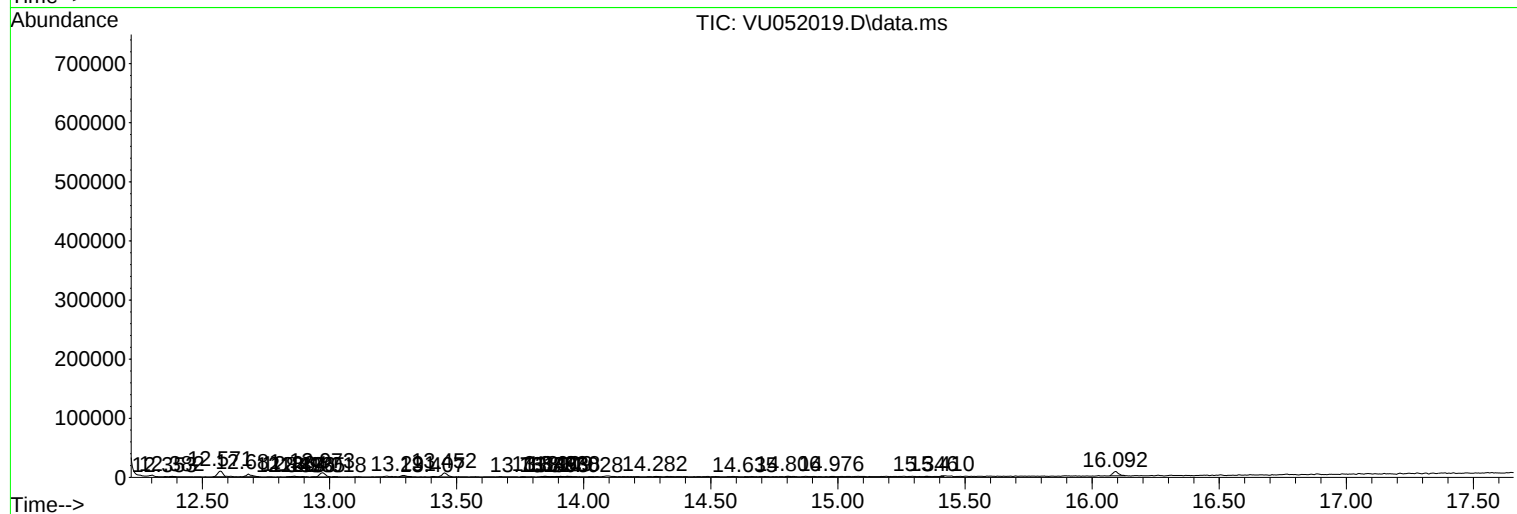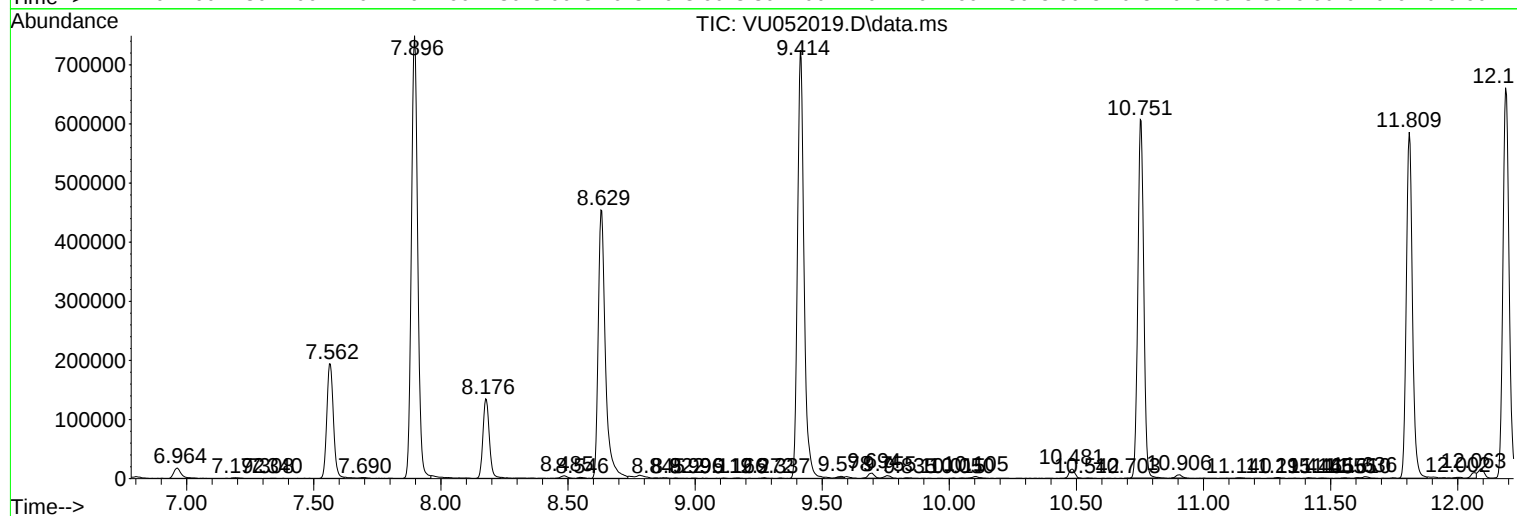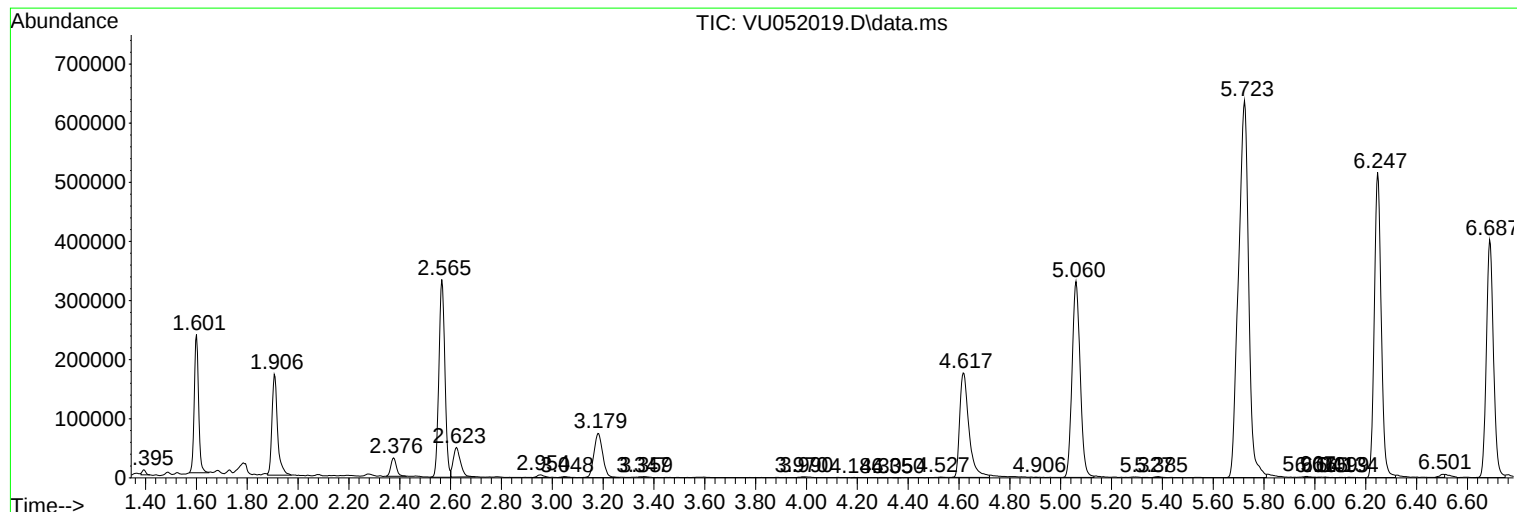

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
Data File : VU052019.D
Acq On : 22 Nov 2022 01:26
Operator : JC/MD
Sample : N5737-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4347

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
Data File : VU052019.D
Acq On : 22 Nov 2022 01:26
Operator : JC/MD
Sample : N5737-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4347

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------