

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
 Data File : VU052031.D
 Acq On : 22 Nov 2022 08:21
 Operator : JC/MD
 Sample : VU1121WBL03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK030

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

Signal : TIC: VU052031.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	103	rBV	282432	334340	16.82%	2.376%
2	1.903	167	175	199	rVB	201654	302010	15.19%	2.147%
3	2.565	368	381	398	rBV	406261	666425	33.52%	4.737%
4	2.896	481	484	487	rVB2	382	255	0.01%	0.002%
5	2.916	488	490	494	rBV2	243	136	0.01%	0.001%
6	2.961	500	504	509	rVB2	770	629	0.03%	0.004%
7	2.996	513	515	518	rVV	403	260	0.01%	0.002%
8	3.044	520	530	550	rVB3	9880	19921	1.00%	0.142%
9	3.118	550	553	556	rBV2	211	178	0.01%	0.001%
10	3.183	557	573	595	rVV	24270	56983	2.87%	0.405%
11	3.337	619	621	623	rBV	216	125	0.01%	0.001%
12	3.353	623	626	627	rBV3	570	325	0.02%	0.002%
13	3.488	664	668	671	rVB2	185	123	0.01%	0.001%
14	3.507	671	674	677	rBV	210	125	0.01%	0.001%
15	3.527	677	680	682	rBV2	193	136	0.01%	0.001%
16	3.594	697	701	704	rBV	393	363	0.02%	0.003%
17	3.675	722	726	729	rVB2	187	130	0.01%	0.001%
18	3.774	753	757	760	rBV2	166	158	0.01%	0.001%
19	3.829	771	774	776	rBV2	180	120	0.01%	0.001%
20	3.851	778	781	785	rVB3	319	222	0.01%	0.002%
21	3.967	809	817	819	rBV2	208	204	0.01%	0.001%
22	4.147	869	873	877	rVB2	152	167	0.01%	0.001%
23	4.173	877	881	884	rBV	266	202	0.01%	0.001%
24	4.192	884	887	890	rBV2	196	125	0.01%	0.001%
25	4.221	894	896	901	rVB	332	162	0.01%	0.001%
26	4.250	901	905	907	rBV3	341	230	0.01%	0.002%
27	4.266	907	910	914	rVB2	325	224	0.01%	0.002%
28	4.404	951	953	958	rVB	242	168	0.01%	0.001%
29	4.443	958	965	968	rBV2	251	279	0.01%	0.002%
30	4.559	995	1001	1004	rBV2	165	161	0.01%	0.001%
31	4.617	1004	1019	1049	rBV	174696	432518	21.76%	3.074%
32	4.996	1133	1137	1140	rBV3	273	243	0.01%	0.002%
33	5.060	1140	1157	1180	rBV	347877	764070	38.43%	5.431%
34	5.292	1222	1229	1232	rBV4	1135	1592	0.08%	0.011%
35	5.366	1246	1252	1255	rBV2	466	493	0.02%	0.004%
36	5.414	1265	1267	1273	rVB2	219	122	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
 Data File : VU052031.D
 Acq On : 22 Nov 2022 08:21
 Operator : JC/MD
 Sample : VU1121WBL03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK030

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

37	5.469	1280	1284	1289	rBV2	144	172	0.01%	0.001%
38	5.523	1299	1301	1305	rBV3	268	172	0.01%	0.001%
39	5.723	1342	1363	1387	rBV2	742276	1988079	100.00%	14.130%
40	5.967	1437	1439	1445	rVB2	770	445	0.02%	0.003%
41	6.028	1455	1458	1459	rBV2	335	212	0.01%	0.002%
42	6.160	1496	1499	1503	rVB3	277	220	0.01%	0.002%
43	6.247	1511	1526	1557	rBV	553721	1062532	53.45%	7.552%
44	6.530	1606	1614	1626	rVB8	3819	7326	0.37%	0.052%
45	6.687	1644	1663	1693	rBV	451936	888091	44.67%	6.312%
46	6.858	1714	1716	1718	rBV3	250	158	0.01%	0.001%
47	6.893	1724	1727	1733	rBV3	478	368	0.02%	0.003%
48	6.922	1733	1736	1737	rBV3	225	109	0.01%	0.001%
49	6.964	1746	1749	1753	rVB3	342	223	0.01%	0.002%
50	7.019	1764	1766	1769	rBV	349	181	0.01%	0.001%
51	7.067	1773	1781	1784	rBV3	265	284	0.01%	0.002%
52	7.102	1789	1792	1796	rVB	291	171	0.01%	0.001%
53	7.182	1815	1817	1818	rBV2	325	139	0.01%	0.001%
54	7.279	1844	1847	1848	rBV	196	116	0.01%	0.001%
55	7.414	1885	1889	1893	rBV	318	294	0.01%	0.002%
56	7.462	1901	1904	1907	rBV	154	114	0.01%	0.001%
57	7.562	1923	1935	1955	rBV	212611	374975	18.86%	2.665%
58	7.764	1995	1998	2000	rVB3	470	207	0.01%	0.001%
59	7.787	2000	2005	2013	rBV6	809	1208	0.06%	0.009%
60	7.842	2019	2022	2024	rBV2	209	125	0.01%	0.001%
61	7.896	2024	2039	2071	rBV	869954	1497973	75.35%	10.647%
62	8.176	2115	2126	2146	rBV2	145095	248727	12.51%	1.768%
63	8.395	2191	2194	2196	rBV	364	265	0.01%	0.002%
64	8.446	2206	2210	2213	rBV	593	535	0.03%	0.004%
65	8.488	2221	2223	2225	rVB	320	124	0.01%	0.001%
66	8.510	2227	2230	2233	rVB	515	325	0.02%	0.002%
67	8.555	2233	2244	2248	rBV5	1817	2646	0.13%	0.019%
68	8.578	2248	2251	2254	rBV	484	353	0.02%	0.003%
69	8.629	2255	2267	2303	rBV2	485375	939669	47.27%	6.679%
70	8.964	2369	2371	2372	rBV	341	140	0.01%	0.001%
71	8.999	2379	2382	2387	rVB3	305	231	0.01%	0.002%
72	9.031	2389	2392	2396	rVB3	381	256	0.01%	0.002%
73	9.060	2397	2401	2403	rBV	457	300	0.02%	0.002%
74	9.279	2466	2469	2471	rVB2	264	156	0.01%	0.001%
75	9.301	2471	2476	2480	rBV2	323	384	0.02%	0.003%
76	9.414	2498	2511	2532	rBV	785579	1293697	65.07%	9.195%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
 Data File : VU052031.D
 Acq On : 22 Nov 2022 08:21
 Operator : JC/MD
 Sample : VU1121WBL03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK030

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

77	9.639	2577	2581	2584	rBV3	508	419	0.02%	0.003%
78	9.948	2674	2677	2681	rVB2	303	227	0.01%	0.002%
79	9.996	2688	2692	2694	rBV2	225	174	0.01%	0.001%
80	10.089	2718	2721	2722	rBV	354	191	0.01%	0.001%
81	10.102	2722	2725	2728	rVV3	649	573	0.03%	0.004%
82	10.292	2781	2784	2789	rBV2	314	217	0.01%	0.002%
83	10.317	2789	2792	2799	rVB2	240	200	0.01%	0.001%
84	10.375	2804	2810	2812	rBV2	366	317	0.02%	0.002%
85	10.391	2812	2815	2818	rBV2	228	131	0.01%	0.001%
86	10.481	2840	2843	2850	rVB2	663	646	0.03%	0.005%
87	10.645	2880	2894	2903	rBV5	1480	3069	0.15%	0.022%
88	10.751	2915	2927	2946	rBV	646264	1046173	52.62%	7.436%
89	10.909	2973	2976	2981	rVB	451	316	0.02%	0.002%
90	10.938	2982	2985	2989	rBV2	379	268	0.01%	0.002%
91	11.308	3097	3100	3103	rBV	209	161	0.01%	0.001%
92	11.465	3142	3149	3151	rBV3	766	917	0.05%	0.007%
93	11.739	3229	3234	3235	rBV2	1489	959	0.05%	0.007%
94	11.809	3243	3256	3279	rBV	592312	957350	48.15%	6.804%
95	12.189	3361	3374	3403	rBV	705045	1152515	57.97%	8.191%
96	12.507	3470	3473	3474	rBV	390	210	0.01%	0.001%
97	12.526	3477	3479	3481	rBV2	289	152	0.01%	0.001%
98	12.758	3549	3551	3554	rBV	303	183	0.01%	0.001%
99	13.841	3883	3888	3901	rBV5	2712	4559	0.23%	0.032%
100	14.333	4036	4041	4050	rVB5	3268	4216	0.21%	0.030%




Sum of corrected areas: 14069769

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
Data File : VU052031.D
Acq On : 22 Nov 2022 08:21
Operator : JC/MD
Sample : VU1121WBL03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK030

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

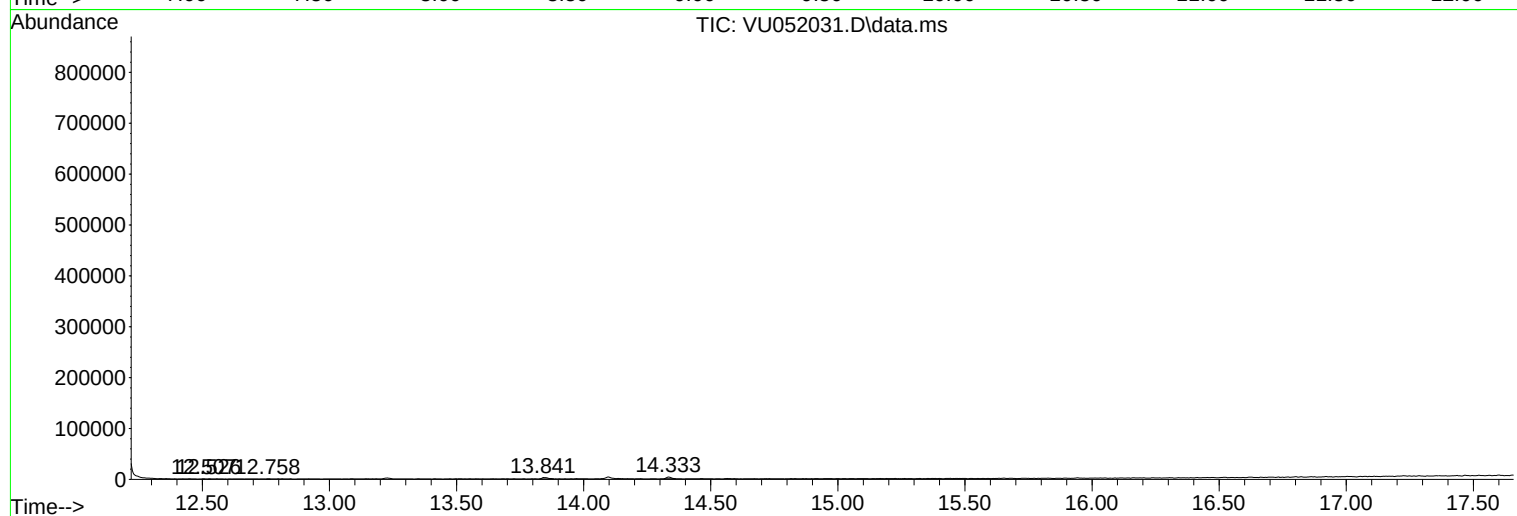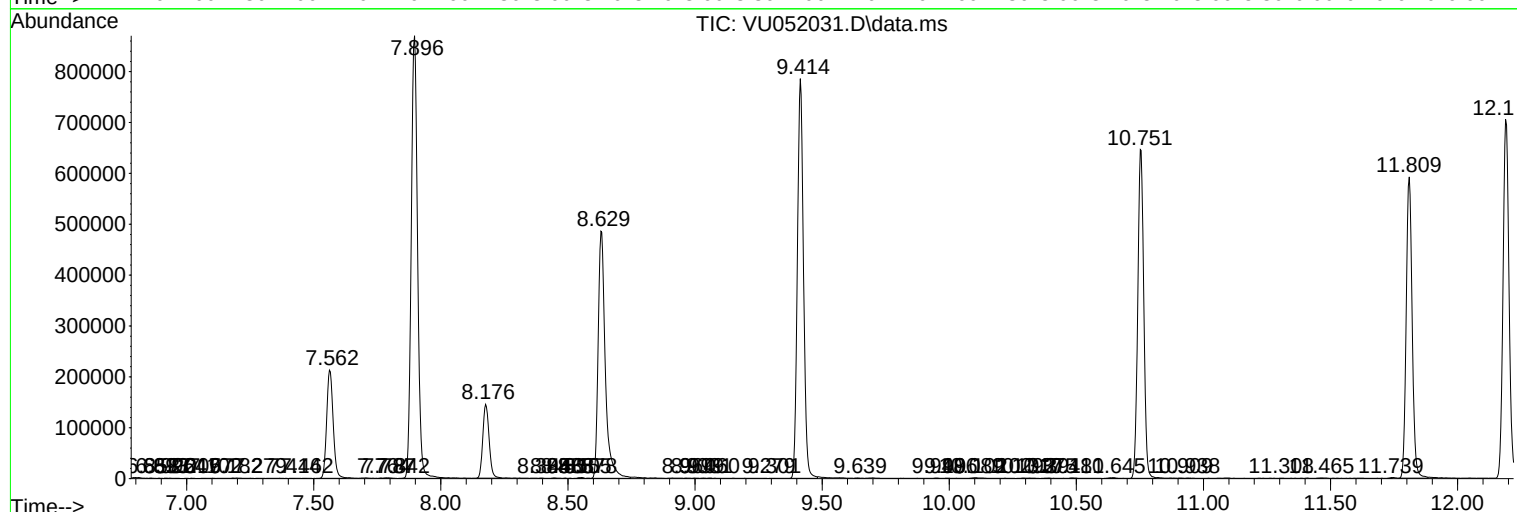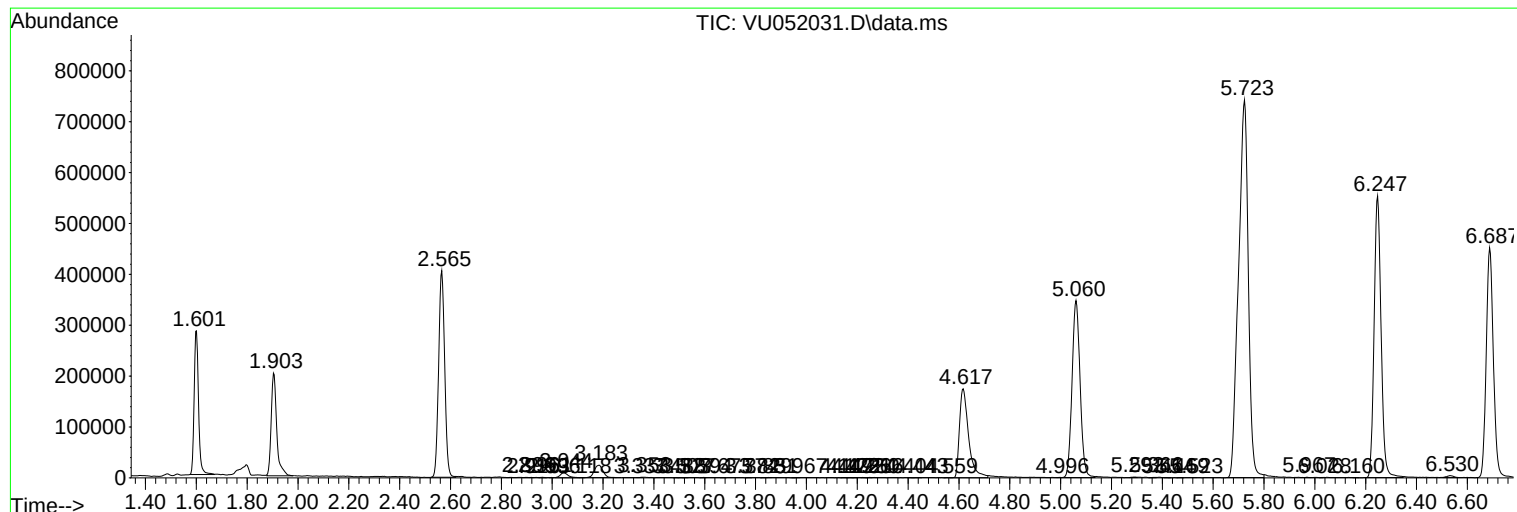

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
Data File : VU052031.D
Acq On : 22 Nov 2022 08:21
Operator : JC/MD
Sample : VU1121WBL03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK030

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
Data File : VU052031.D
Acq On : 22 Nov 2022 08:21
Operator : JC/MD
Sample : VU1121WBL03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK030

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc