

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
 Data File : VU052033.D
 Acq On : 22 Nov 2022 10:01
 Operator : JC/MD
 Sample : N5716-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A0B23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

Signal : TIC: VU052033.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	99	rBV	220496	256240	15.17%	2.061%
2	1.912	169	178	203	rVB	165487	248960	14.74%	2.002%
3	2.372	318	321	324	rBV3	953	927	0.05%	0.007%
4	2.568	368	382	395	rBV	328493	537176	31.80%	4.321%
5	2.707	422	425	427	rBV2	428	276	0.02%	0.002%
6	2.752	434	439	448	rBV4	1504	2179	0.13%	0.018%
7	2.854	464	471	473	rBV3	484	637	0.04%	0.005%
8	2.951	498	501	505	rVB2	337	292	0.02%	0.002%
9	2.977	505	509	510	rBV	304	213	0.01%	0.002%
10	3.041	524	529	531	rBV2	1108	1050	0.06%	0.008%
11	3.186	557	574	585	rBV	4693	10052	0.60%	0.081%
12	3.356	618	627	628	rBV3	1763	1854	0.11%	0.015%
13	3.697	722	733	734	rBV3	4226	5003	0.30%	0.040%
14	3.964	813	816	820	rVB2	293	236	0.01%	0.002%
15	3.999	823	827	830	rBV	331	240	0.01%	0.002%
16	4.530	979	992	1008	rVB4	3287	7486	0.44%	0.060%
17	4.616	1008	1019	1046	rBV	159749	389793	23.08%	3.135%
18	5.060	1141	1157	1183	rBV	299163	659527	39.04%	5.305%
19	5.285	1221	1227	1229	rBV3	805	751	0.04%	0.006%
20	5.382	1248	1257	1264	rVB3	497	902	0.05%	0.007%
21	5.552	1305	1310	1312	rBV	220	201	0.01%	0.002%
22	5.723	1341	1363	1384	rBV2	619467	1689198	100.00%	13.587%
23	5.967	1437	1439	1444	rVB3	678	476	0.03%	0.004%
24	5.993	1444	1447	1450	rBV3	413	391	0.02%	0.003%
25	6.050	1463	1465	1473	rVB2	477	565	0.03%	0.005%
26	6.089	1473	1477	1480	rBV2	325	309	0.02%	0.002%
27	6.124	1484	1488	1492	rVB	405	306	0.02%	0.002%
28	6.247	1511	1526	1558	rBV	515306	991184	58.68%	7.972%
29	6.587	1629	1632	1634	rBV2	429	264	0.02%	0.002%
30	6.687	1645	1663	1696	rBV	390005	776556	45.97%	6.246%
31	6.948	1742	1744	1751	rBV2	271	248	0.01%	0.002%
32	6.983	1751	1755	1758	rVV	334	223	0.01%	0.002%
33	7.060	1777	1779	1782	rBV	370	306	0.02%	0.002%
34	7.102	1788	1792	1799	rVB3	374	482	0.03%	0.004%
35	7.195	1814	1821	1824	rBV3	713	762	0.05%	0.006%
36	7.230	1830	1832	1837	rVB2	403	251	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
 Data File : VU052033.D
 Acq On : 22 Nov 2022 10:01
 Operator : JC/MD
 Sample : N5716-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A0B23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

37	7.259	1837	1841	1843	rBV	502	257	0.02%	0.002%
38	7.468	1903	1906	1911	rVB	309	260	0.02%	0.002%
39	7.504	1911	1917	1921	rBV2	216	279	0.02%	0.002%
40	7.565	1922	1936	1966	rBV	187710	340919	20.18%	2.742%
41	7.748	1990	1993	1997	rBV3	311	255	0.02%	0.002%
42	7.796	2002	2008	2015	rBV5	1355	1816	0.11%	0.015%
43	7.829	2016	2018	2025	rVB3	302	217	0.01%	0.002%
44	7.896	2025	2039	2073	rBV	721891	1263151	74.78%	10.160%
45	8.176	2115	2126	2146	rBV	133328	227274	13.45%	1.828%
46	8.269	2152	2155	2158	rVB4	704	435	0.03%	0.003%
47	8.340	2175	2177	2178	rBV	586	240	0.01%	0.002%
48	8.353	2178	2181	2184	rVV2	382	300	0.02%	0.002%
49	8.552	2238	2243	2253	rVB3	1531	1771	0.10%	0.014%
50	8.629	2255	2267	2306	rBV2	430436	859082	50.86%	6.910%
51	9.015	2382	2387	2390	rVB3	446	372	0.02%	0.003%
52	9.034	2390	2393	2399	rBV2	398	374	0.02%	0.003%
53	9.237	2454	2456	2462	rVB3	339	322	0.02%	0.003%
54	9.275	2462	2468	2472	rBV3	415	484	0.03%	0.004%
55	9.414	2498	2511	2539	rBV	725368	1220166	72.23%	9.814%
56	9.658	2585	2587	2590	rVB2	420	230	0.01%	0.002%
57	9.700	2590	2600	2604	rBV2	1263	1895	0.11%	0.015%
58	9.928	2668	2671	2677	rVB2	438	467	0.03%	0.004%
59	9.983	2684	2688	2691	rBV2	225	235	0.01%	0.002%
60	10.041	2703	2706	2710	rBV3	292	262	0.02%	0.002%
61	10.118	2720	2730	2736	rBV5	1583	2402	0.14%	0.019%
62	10.185	2746	2751	2752	rBV	392	299	0.02%	0.002%
63	10.359	2800	2805	2808	rBV2	240	284	0.02%	0.002%
64	10.491	2837	2846	2852	rVV5	984	1698	0.10%	0.014%
65	10.552	2862	2865	2871	rVB2	315	295	0.02%	0.002%
66	10.603	2877	2881	2888	rVB	503	575	0.03%	0.005%
67	10.652	2888	2896	2900	rBV2	528	652	0.04%	0.005%
68	10.754	2915	2928	2948	rBV	568449	922262	54.60%	7.418%
69	11.015	3007	3009	3013	rVB2	384	201	0.01%	0.002%
70	11.047	3013	3019	3022	rBV2	287	361	0.02%	0.003%
71	11.086	3027	3031	3033	rBV2	482	429	0.03%	0.003%
72	11.722	3224	3229	3231	rBV2	365	340	0.02%	0.003%
73	11.748	3234	3237	3239	rBV3	597	397	0.02%	0.003%
74	11.809	3244	3256	3289	rBV	570780	938952	55.59%	7.552%
75	11.986	3309	3311	3318	rVB5	364	329	0.02%	0.003%
76	12.063	3332	3335	3338	rBV	325	301	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
 Data File : VU052033.D
 Acq On : 22 Nov 2022 10:01
 Operator : JC/MD
 Sample : N5716-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A0B23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

77	12.089	3341	3343	3350	rVB3	777	707	0.04%	0.006%
78	12.192	3361	3375	3396	rBV	622075	1026431	60.76%	8.256%
79	12.372	3427	3431	3435	rVB5	565	392	0.02%	0.003%
80	12.533	3478	3481	3485	rVB2	461	326	0.02%	0.003%
81	12.561	3487	3490	3495	rVV2	440	308	0.02%	0.002%
82	12.632	3508	3512	3517	rBV2	341	312	0.02%	0.003%
83	12.719	3536	3539	3543	rVB	412	291	0.02%	0.002%
84	12.774	3554	3556	3560	rVB2	348	202	0.01%	0.002%
85	12.896	3591	3594	3596	rBV	304	202	0.01%	0.002%
86	12.986	3618	3622	3627	rBV3	384	365	0.02%	0.003%
87	13.134	3665	3668	3670	rBV	381	195	0.01%	0.002%
88	13.227	3687	3697	3704	rBV4	3707	6016	0.36%	0.048%
89	13.327	3723	3728	3732	rVB3	412	343	0.02%	0.003%
90	13.452	3765	3767	3770	rVB2	350	205	0.01%	0.002%
91	13.484	3774	3777	3781	rBV2	370	296	0.02%	0.002%
92	13.542	3791	3795	3797	rBV	342	281	0.02%	0.002%
93	13.626	3817	3821	3823	rBV2	303	226	0.01%	0.002%
94	13.848	3884	3890	3900	rBV2	2742	3338	0.20%	0.027%
95	14.012	3938	3941	3945	rBV	300	275	0.02%	0.002%
96	14.086	3961	3964	3965	rBV	511	288	0.02%	0.002%
97	14.102	3965	3969	3976	rVV3	805	1094	0.06%	0.009%
98	14.282	4023	4025	4030	rVB3	624	414	0.02%	0.003%
99	14.333	4030	4041	4053	rBV5	7597	13442	0.80%	0.108%
100	14.960	4234	4236	4240	rVB2	560	300	0.02%	0.002%




Sum of corrected areas: 12432605

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
Data File : VU052033.D
Acq On : 22 Nov 2022 10:01
Operator : JC/MD
Sample : N5716-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A0B23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

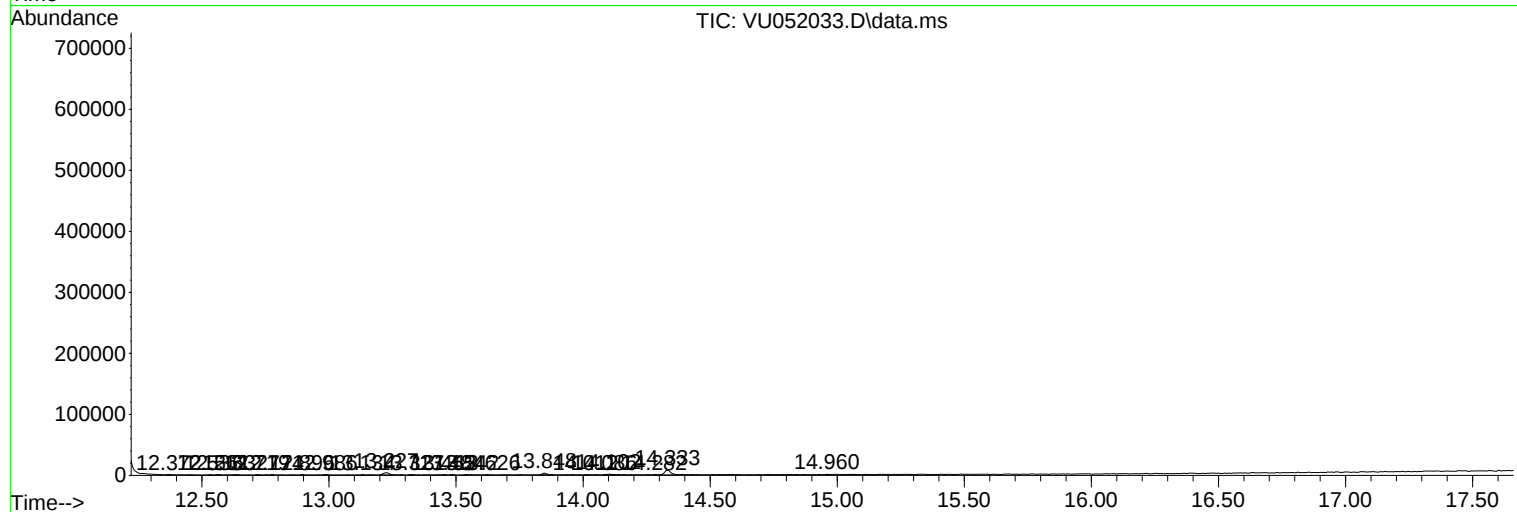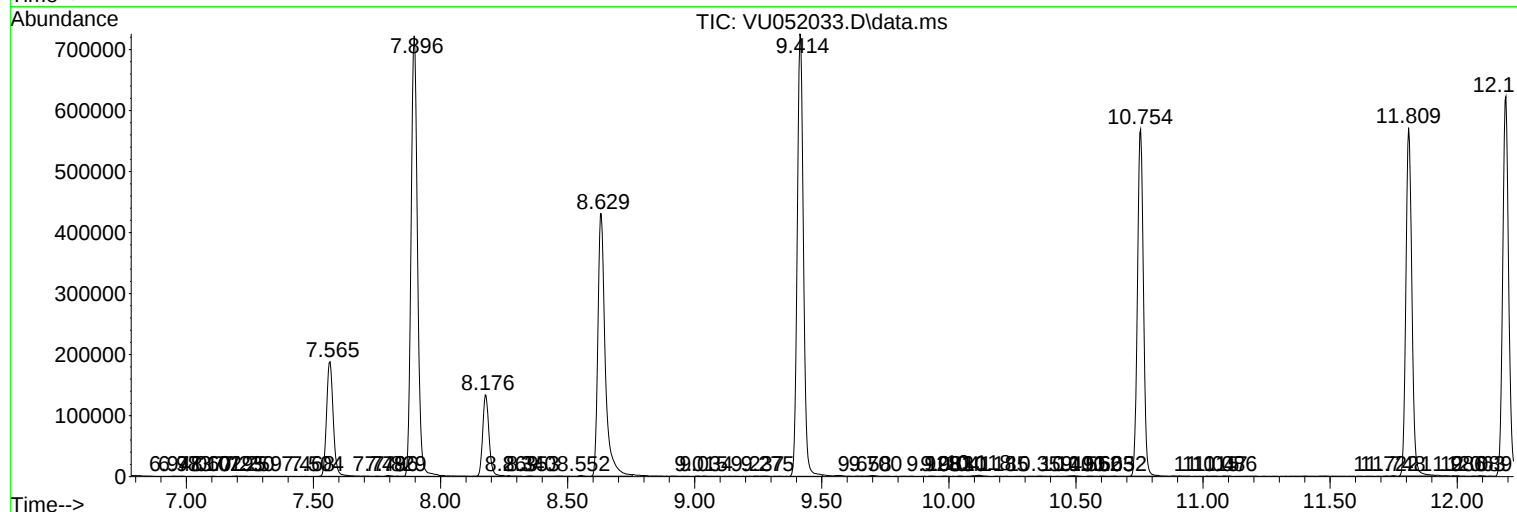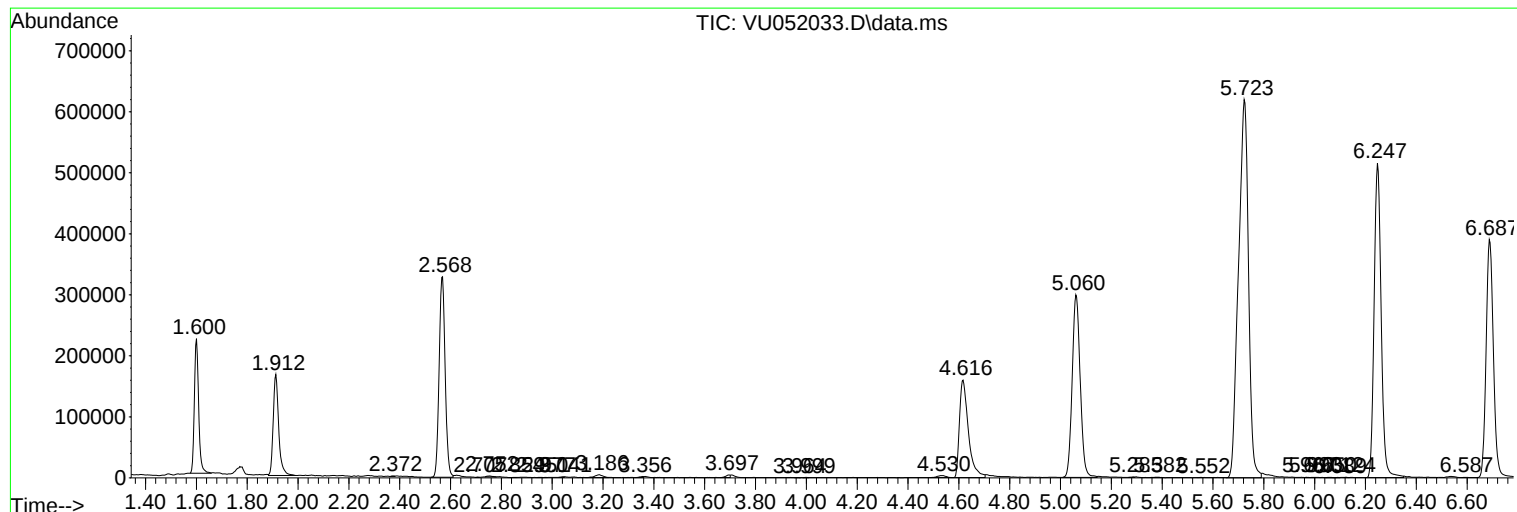

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
Data File : VU052033.D
Acq On : 22 Nov 2022 10:01
Operator : JC/MD
Sample : N5716-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A0B23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
Data File : VU052033.D
Acq On : 22 Nov 2022 10:01
Operator : JC/MD
Sample : N5716-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A0B23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc