


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112122\
Data File : VU051991.D
Acq On : 21 Nov 2022 09:27
Operator : JC/MD
Sample : BFB147
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB147

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Title : VOC Analysis
Last Update : Tue Nov 22 07:34:37 2022

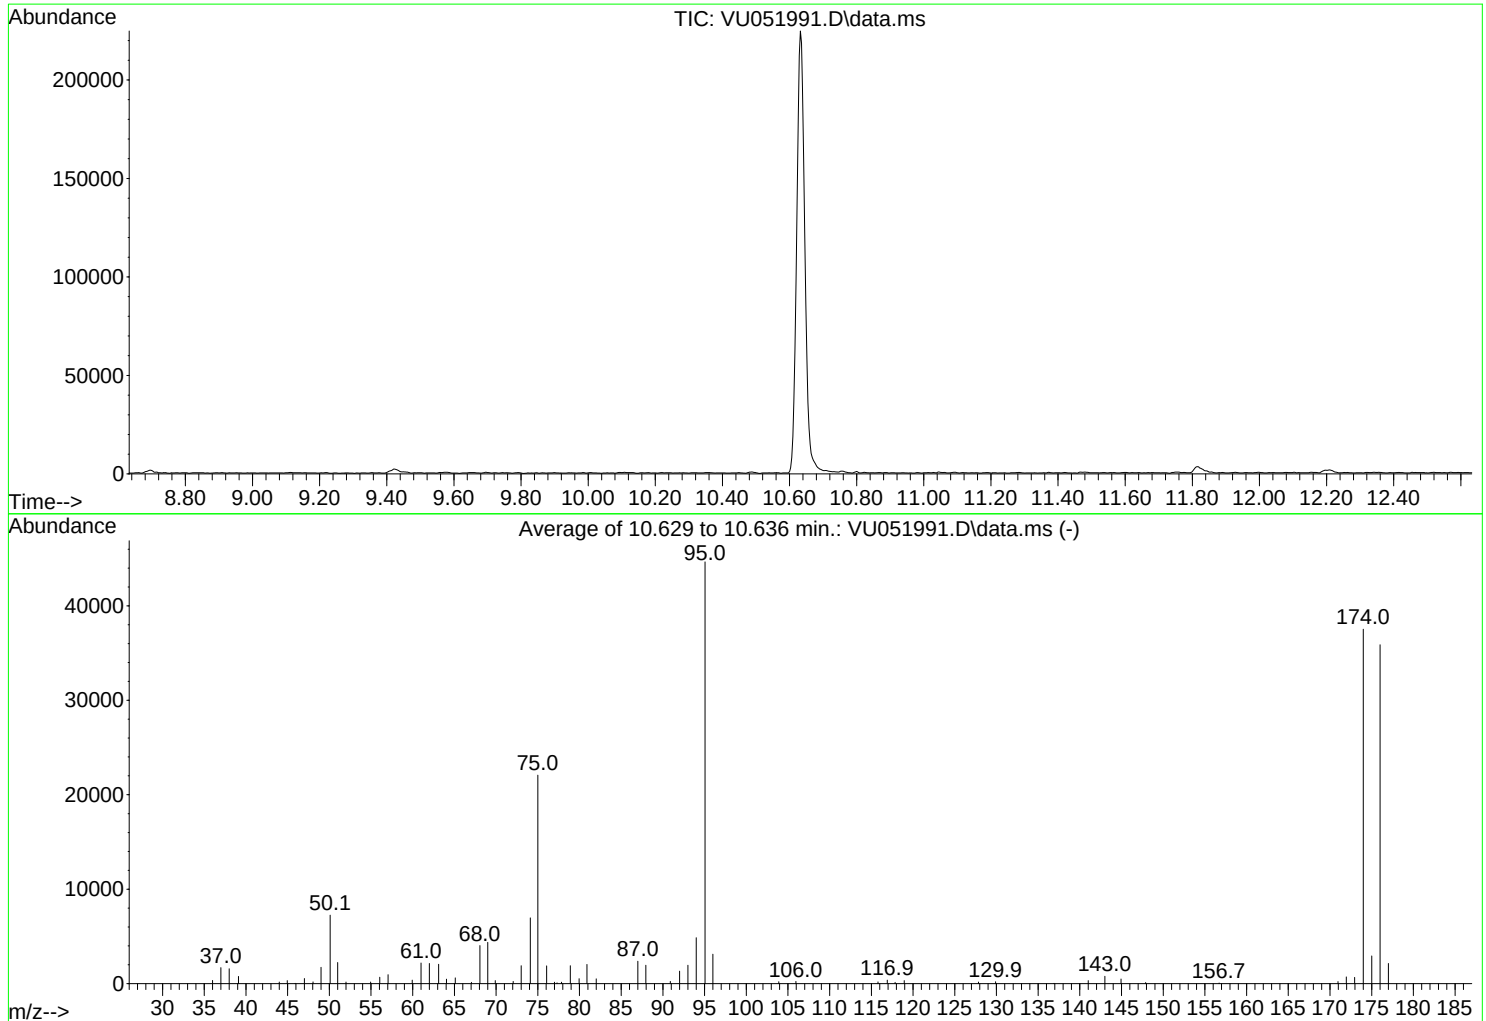

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	7257	PASS
75	95	30	80	49.4	22080	PASS
95	95	100	100	100.0	44659	PASS
96	95	5	9	7.0	3120	PASS
173	174	0.00	2	1.8	663	PASS
174	95	50	120	84.0	37531	PASS
175	174	5	9	7.8	2936	PASS
176	174	95	101	95.6	35875	PASS
177	176	5	9	5.9	2128	PASS

m/z	Abundance
40.00	132.0
44.00	371.0

Instrument :
MSVOA_U
ClientSampleId :
BFB147

m/z	Abundance
36.00	302.0
37.00	1764.0
38.00	1646.0
39.10	794.0
40.10	115.0
44.00	496.0
44.90	312.0
47.00	505.0
48.00	230.0
49.00	1664.0
50.10	7340.0
51.00	2162.0
52.00	192.0
55.00	179.0
56.00	681.0
57.10	915.0
59.90	324.0
61.00	2091.0
62.00	2033.0
63.10	1984.0
64.00	487.0
65.10	595.0
67.00	130.0
68.10	4028.0
69.00	4237.0
69.90	325.0
72.10	235.0
73.00	1982.0
74.10	6738.0
75.00	22256.0
76.10	1900.0
77.00	256.0
77.90	157.0
78.90	1911.0
79.90	515.0
80.90	1942.0
82.00	456.0
87.00	2147.0
88.00	2033.0
90.90	251.0
92.00	1353.0
93.00	1930.0
94.00	5015.0
95.00	44456.0
96.00	2942.0
103.90	146.0
105.90	224.0
115.80	178.0
116.90	404.0
117.80	125.0
119.00	372.0
127.80	196.0
129.90	188.0
136.90	105.0
141.00	330.0
143.00	787.0
145.00	501.0
147.90	137.0
156.70	110.0
170.90	296.0
171.90	713.0
173.00	651.0
174.00	37520.0
175.00	2827.0
176.00	36800.0
177.00	2068.0

Instrument :
MSVOA_U
ClientSampleId :
BFB147

m/z	Abundance
36.00	349.0
37.00	1724.0
38.00	1635.0
39.10	783.0
44.00	566.0
45.00	339.0
47.00	525.0
48.10	207.0
49.00	1837.0
50.10	7389.0
51.00	2293.0
52.00	182.0
55.00	181.0
56.00	710.0
57.00	977.0
59.90	368.0
61.00	2242.0
62.00	2226.0
63.10	2114.0
64.10	485.0
65.10	626.0
67.10	144.0
68.10	4089.0
69.00	4481.0
69.90	334.0
72.00	236.0
73.00	1954.0
74.10	7244.0
75.00	22888.0
76.10	1979.0
77.00	218.0
77.80	166.0
78.90	1953.0
79.90	528.0
80.90	2126.0
82.00	531.0
87.00	2489.0
87.90	1989.0
90.90	254.0
92.00	1341.0
93.00	1988.0
94.00	4992.0
95.00	45656.0
96.00	3243.0
103.90	215.0
106.00	246.0
115.80	207.0
116.90	371.0
117.90	141.0
119.00	340.0
127.80	167.0
129.90	216.0
141.00	328.0
143.00	804.0
145.00	507.0
147.90	137.0
156.70	107.0
171.00	210.0
172.00	727.0
173.00	695.0
174.00	38752.0
175.00	2999.0
176.00	36912.0
177.00	2146.0

Instrument :
MSVOA_U
ClientSampleId :
BFB147

m/z	Abundance
36.00	389.0
37.00	1594.0
38.00	1461.0
39.10	724.0
40.00	143.0
44.00	550.0
45.00	342.0
45.90	116.0
47.00	611.0
48.10	149.0
49.00	1700.0
50.10	7041.0
51.00	2238.0
52.00	160.0
54.90	169.0
56.10	654.0
57.00	969.0
60.00	407.0
61.00	2211.0
62.00	2134.0
63.10	2077.0
64.00	441.0
65.10	607.0
67.10	113.0
68.00	3980.0
69.00	4375.0
69.90	305.0
72.00	235.0
73.00	1755.0
74.10	6910.0
75.00	21096.0
76.00	1771.0
77.30	257.0
77.80	155.0
78.90	1833.0
80.00	519.0
80.90	2056.0
82.00	565.0
87.00	2496.0
87.90	1805.0
90.90	185.0
92.00	1268.0
93.00	1919.0
94.00	4591.0
95.10	43864.0
96.00	3175.0
103.90	273.0
106.00	230.0
115.80	188.0
116.90	359.0
117.90	153.0
118.90	280.0
127.90	127.0
129.90	188.0
141.00	305.0
143.00	777.0
144.90	462.0
147.90	107.0
171.00	137.0
172.00	672.0
172.90	644.0
174.00	36320.0
175.00	2981.0
176.00	33912.0
177.00	2171.0

Instrument :
MSVOA_U
ClientSampleId :
BFB147