


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112123\
 Data File : VU056538.D
 Acq On : 21 Nov 2023 08:21
 Operator : MD/SY
 Sample : BFB079
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB079

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Nov 22 00:29:26 2023

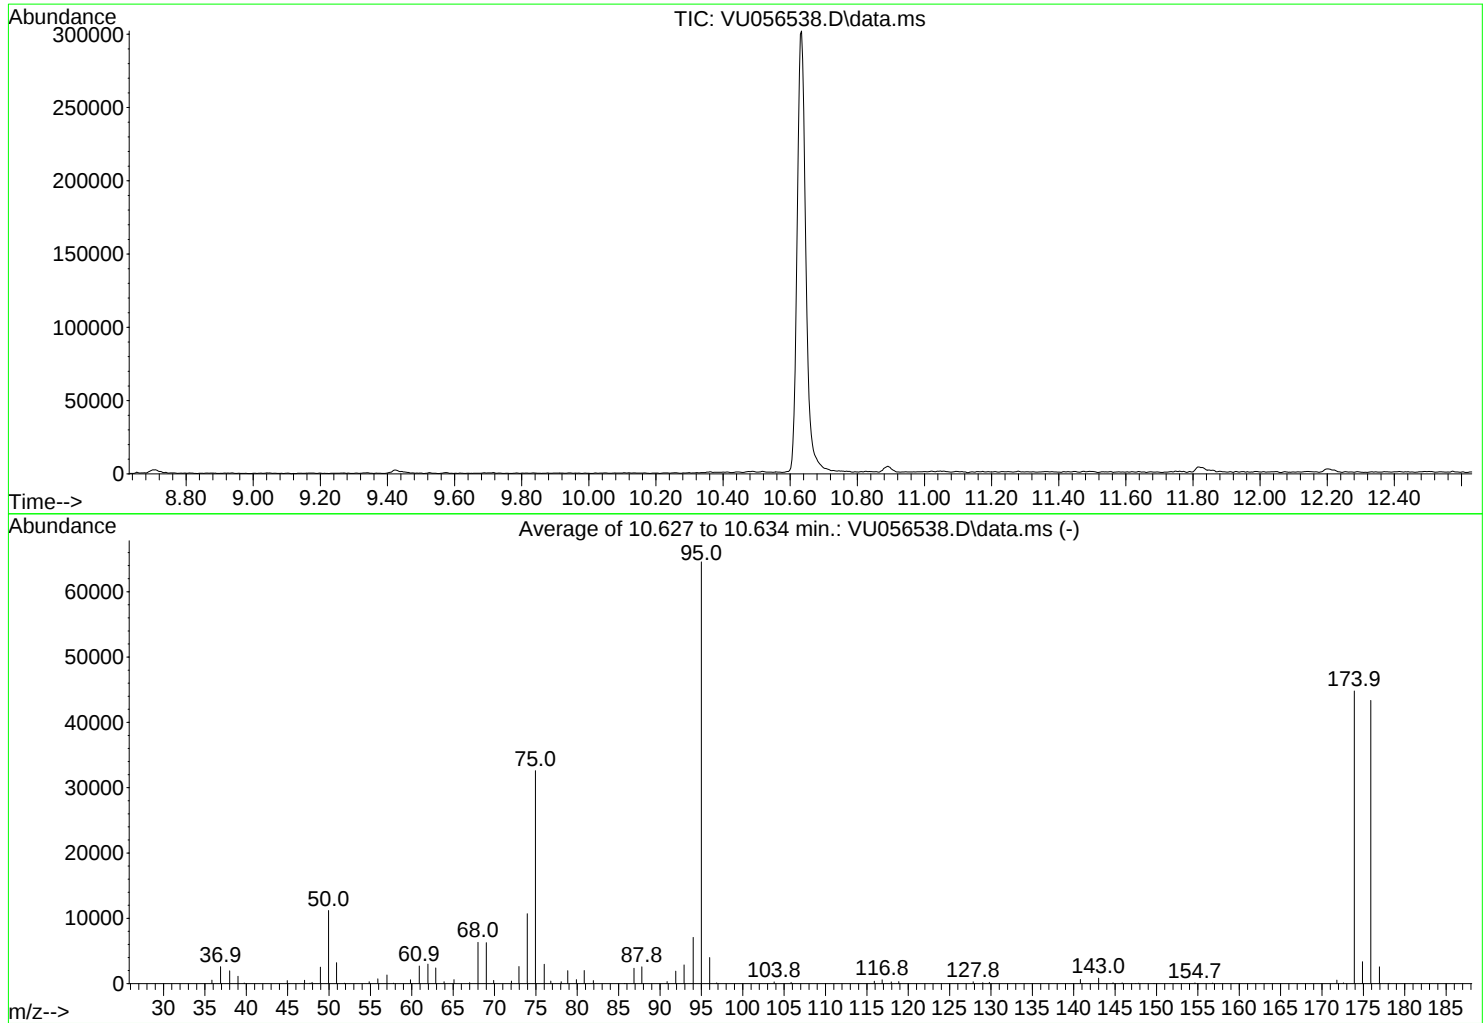

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2892

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	11206	PASS
75	95	30	80	50.5	32611	PASS
95	95	100	100	100.0	64576	PASS
96	95	5	9	6.2	3990	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	69.4	44797	PASS
175	174	5	9	7.5	3351	PASS
176	174	95	101	96.8	43368	PASS
177	176	5	9	5.9	2566	PASS

m/z	Abundance
35.80	585.0
38.00	222.0
39.80	182.0
43.80	538.0

Instrument :
MSVOA_U
ClientSampleId :
BFB079

m/z	Abundance
35.90	1155.0
36.90	2565.0
38.00	2173.0
39.00	1018.0
39.80	273.0
43.80	563.0
44.90	520.0
47.10	545.0
47.70	230.0
48.90	2513.0
50.00	11221.0
50.90	2949.0
54.80	296.0
55.90	788.0
57.00	1344.0
57.80	115.0
59.90	633.0
60.90	2471.0
62.00	3112.0
62.90	2236.0
64.00	319.0
65.10	563.0
67.00	167.0
68.00	5524.0
69.00	6046.0
69.90	561.0
72.10	404.0
73.00	2443.0
73.90	9986.0
74.90	30872.0
76.00	2668.0
76.80	384.0
78.10	264.0
78.90	2019.0
79.90	532.0
80.80	1807.0
81.90	384.0
86.80	2180.0
87.80	2226.0
90.80	318.0
91.90	1780.0
92.90	2579.0
94.00	6590.0
95.00	61472.0
96.00	3732.0
96.90	145.0
103.80	251.0
105.80	175.0
115.90	403.0
116.80	518.0
118.00	258.0
118.80	266.0
127.90	276.0
129.00	143.0
129.80	203.0
140.80	540.0
143.00	772.0
144.80	140.0
145.90	129.0
147.80	130.0
149.70	100.0
154.60	134.0
156.80	134.0
171.80	507.0
172.60	358.0
173.90	40552.0
174.90	3275.0
175.90	39264.0
177.00	2389.0

Instrument :
MSVOA_U
ClientSampleId :
BFB079

m/z	Abundance
35.90	1165.0
36.90	2680.0
38.00	2233.0
39.00	1208.0
39.80	295.0
43.90	506.0
45.00	458.0
47.10	491.0
47.90	274.0
48.90	2631.0
50.00	11564.0
50.90	3279.0
51.90	110.0
54.90	318.0
55.90	745.0
57.00	1303.0
57.80	122.0
59.90	540.0
60.90	2781.0
62.00	3044.0
62.90	2407.0
63.90	278.0
65.10	598.0
67.00	140.0
68.00	6421.0
69.00	6383.0
69.90	500.0
72.10	422.0
72.90	2754.0
74.00	11033.0
74.90	33496.0
76.00	3064.0
76.80	411.0
78.00	291.0
78.90	2022.0
79.90	632.0
80.90	2028.0
81.90	482.0
85.70	109.0
86.80	2323.0
87.80	2715.0
90.90	330.0
91.90	2036.0
92.90	2924.0
94.00	7366.0
95.00	66400.0
96.00	4150.0
96.80	120.0
103.80	263.0
105.90	200.0
115.90	378.0
116.80	627.0
118.00	275.0
118.90	341.0
127.80	300.0
129.00	152.0
129.80	214.0
140.80	668.0
143.00	884.0
144.70	145.0
145.80	122.0
147.50	108.0
147.90	116.0
154.60	141.0
156.80	131.0
171.80	551.0
173.90	46016.0
174.90	3504.0
175.90	44696.0
176.90	2579.0

Instrument :
MSVOA_U
ClientSampleId :
BFB079

m/z	Abundance
35.90	1028.0
36.90	2562.0
38.00	2169.0
39.00	1148.0
39.70	255.0
44.00	481.0
45.00	407.0
47.00	475.0
48.00	349.0
49.00	2431.0
49.90	10832.0
50.90	3388.0
51.80	144.0
54.90	269.0
55.90	661.0
57.00	1289.0
59.80	583.0
60.90	2853.0
61.90	2825.0
62.90	2543.0
63.80	323.0
65.10	657.0
67.00	123.0
68.00	7052.0
69.00	6352.0
69.90	387.0
72.00	378.0
73.00	2694.0
74.00	11105.0
75.00	33464.0
76.00	3182.0
76.80	424.0
78.00	303.0
78.80	1949.0
79.90	671.0
80.90	2232.0
82.00	530.0
85.90	102.0
86.90	2558.0
87.80	2819.0
90.90	315.0
91.90	1943.0
92.90	3135.0
94.00	7311.0
95.00	65856.0
96.00	4088.0
96.80	127.0
103.80	286.0
105.90	202.0
115.90	300.0
116.90	640.0
117.90	298.0
118.90	368.0
127.80	302.0
129.00	151.0
129.80	187.0
140.80	707.0
143.00	854.0
144.70	152.0
145.80	142.0
154.70	122.0
171.80	593.0
173.90	47824.0
174.90	3275.0
175.90	46144.0
176.90	2729.0
178.10	126.0

Instrument :
MSVOA_U
ClientSampleId :
BFB079