

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112124\
 Data File : VU061917.D
 Acq On : 21 Nov 2024 14:58
 Operator : MD/SY
 Sample : P4885-10DL 5X
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BG3Q6DL

Quant Time: Nov 21 23:08:44 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR112024WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Nov 21 23:06:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	162814	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	162094	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	62874	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	47494	5.947	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	119.000%
7) Chloroethane-d5	1.904	69	39555	5.599	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	112.000%
11) 1,1-Dichloroethene-d2	2.560	65	20958	6.569	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	131.400%#
20) 2-Butanone-d5	4.611	46	105119	41.915	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	83.840%
24) Chloroform-d	5.052	84	95209	4.887	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.800%
26) 1,2-Dichloroethane-d4	5.695	65	50111	4.998	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.000%
32) Benzene-d6	5.717	84	185472	5.873	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	117.400%
36) 1,2-Dichloropropane-d6	6.682	67	59710	5.564	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	111.200%
41) Toluene-d8	7.891	98	157350	5.974	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	119.400%
43) trans-1,3-Dichloroprop...	8.174	79	18910	4.760	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.200%
46) 2-Hexanone-d5	8.624	63	73072	40.298	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	80.600%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	48692	4.541	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.800%
66) 1,2-Dichlorobenzene-d4	12.187	152	49244	5.297	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.000%
Target Compounds						Qvalue
16) Methylene chloride	3.036	84	8613	0.657	ug/L	93
18) trans-1,2-Dichloroethene	3.351	96	2961	0.257	ug/L	80
22) cis-1,2-Dichloroethene	4.660	96	13861	1.067	ug/L	99
29) 1,1,1-Trichloroethane	5.306	97	11540	0.618	ug/L	99
34) Trichloroethene	6.534	95	98744	7.558	ug/L	98
42) Toluene	7.965	91	10004	0.195	ug/L	92
47) Tetrachloroethene	8.547	164	20656	2.174	ug/L	94
51) Chlorobenzene	9.441	112	6452	0.183	ug/L	97
53) m,p-Xylene	9.688	106	3320	0.153	ug/L	87
67) 1,2-Dichlorobenzene	12.209	146	3963	0.209	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112124\
Data File : VU061917.D
Acq On : 21 Nov 2024 14:58
Operator : MD/SY
Sample : P4885-10DL 5X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG3Q6DL

Quant Time: Nov 21 23:08:44 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR112024WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Nov 21 23:06:37 2024
Response via : Initial Calibration

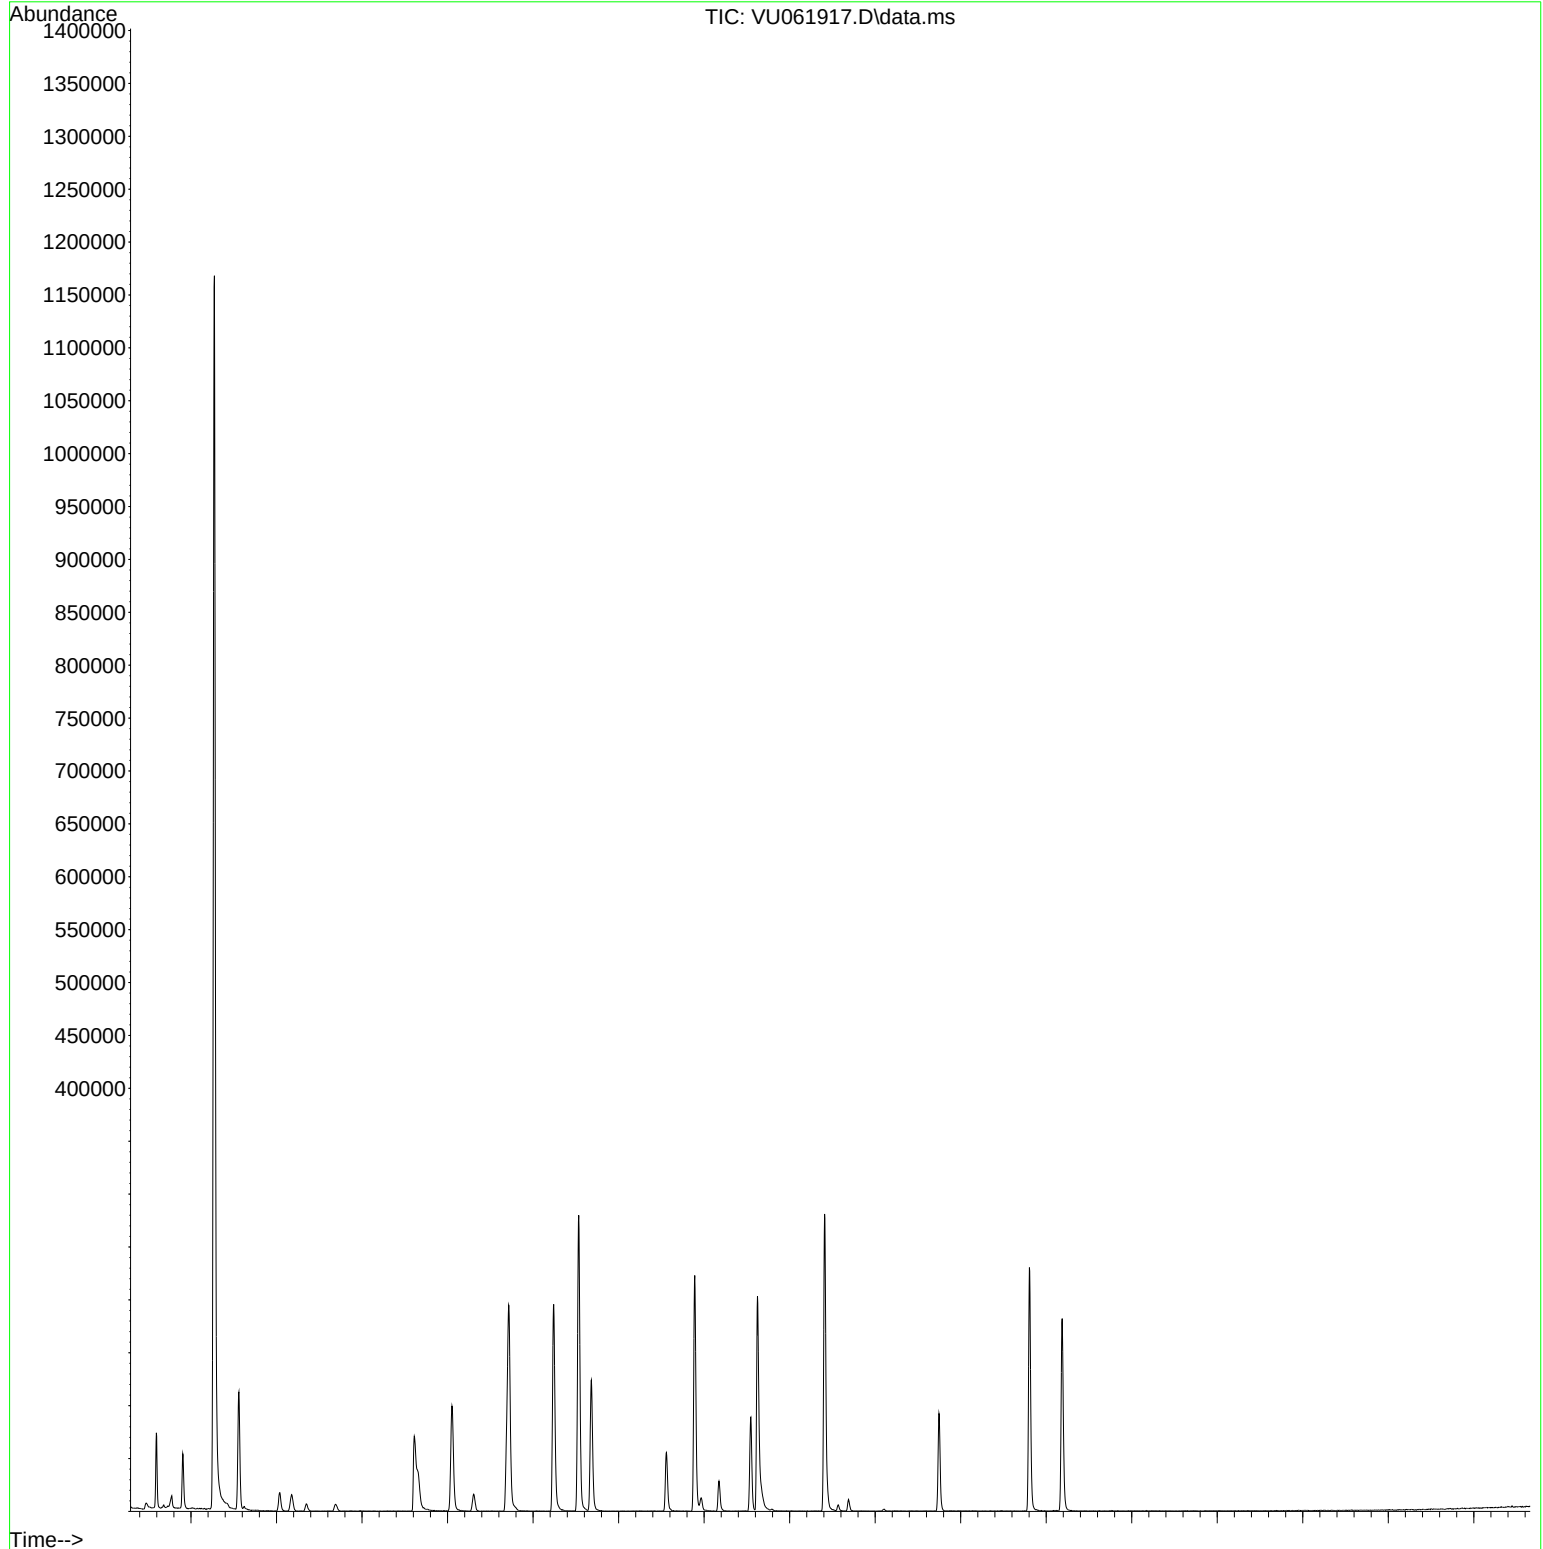

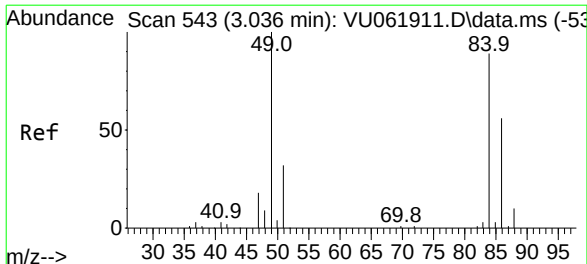

#16

Methylene chloride

Concen: 0.657 ug/L

RT: 3.036 min Scan# 54

Delta R.T. -0.000 min

Lab File: VU061917.D


Acq: 21 Nov 2024 14:58

Instrument :




MSVOA_U

ClientSampleId :

BG3Q6DL

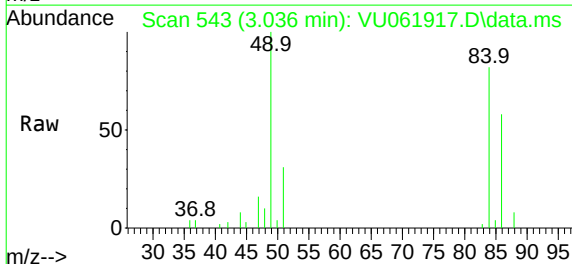

Tgt Ion:	84	Resp:	8613
Ion	Ratio	Lower	Upper
84	100		
86	70.7	43.5	80.7
49	121.9	81.9	152.1

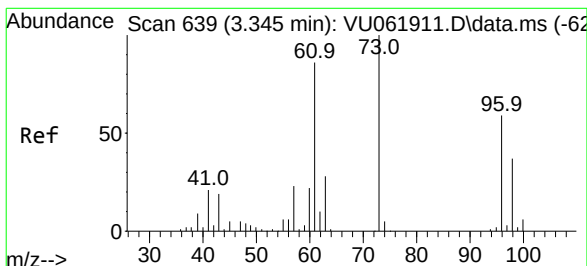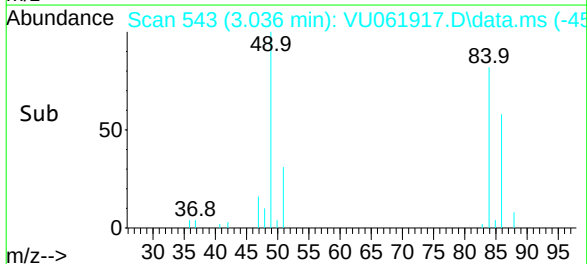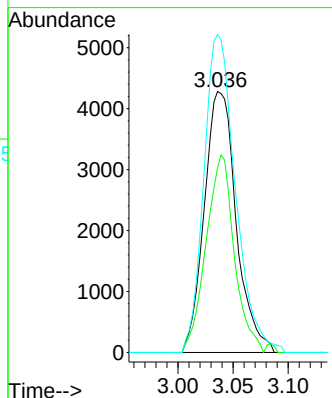

#18

trans-1,2-Dichloroethene

Concen: 0.257 ug/L




RT: 3.351 min Scan# 641


Delta R.T. 0.006 min

Lab File: VU061917.D

Acq: 21 Nov 2024 14:58

Tgt Ion:	96	Resp:	2961
Ion	Ratio	Lower	Upper
96	100		
61	121.5	104.2	193.4
98	51.3	45.7	84.9


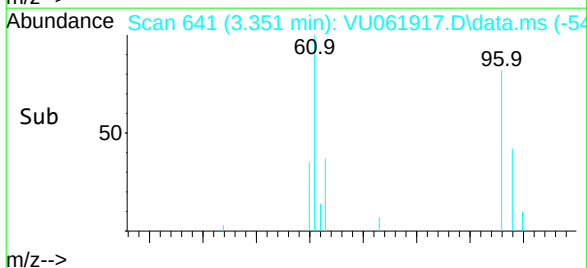
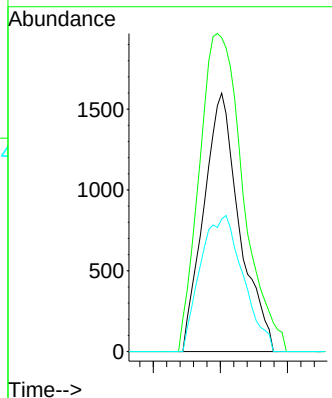
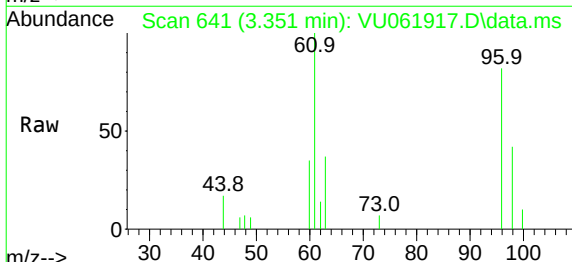


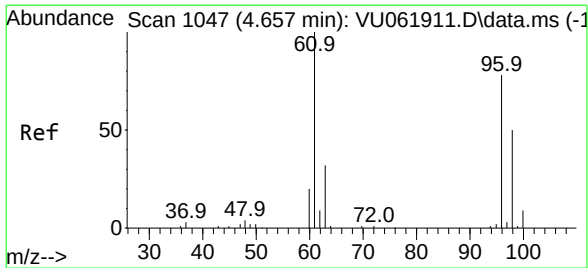

#22
cis-1,2-Dichloroethene
Concen: 1.067 ug/L
RT: 4.660 min Scan# 1047
Delta R.T. 0.003 min
Lab File: VU061917.D
Acq: 21 Nov 2024 14:58




Instrument :
MSVOA_U
ClientSampleId :
BG3Q6DL


Tgt Ion: 96	Resp: 13861
Ion Ratio	Lower Upper
96 100	
61 129.8	92.0 170.8
98 63.5	44.5 82.7

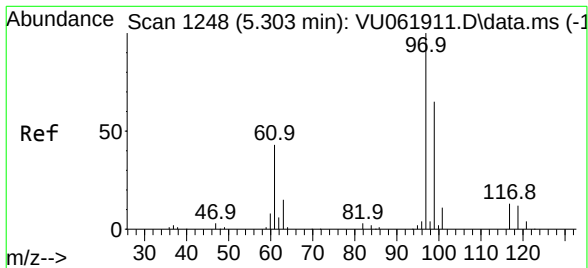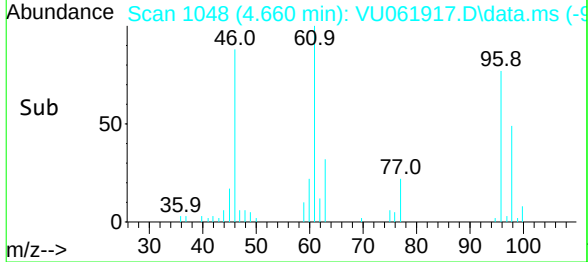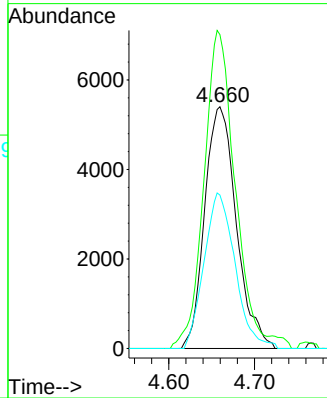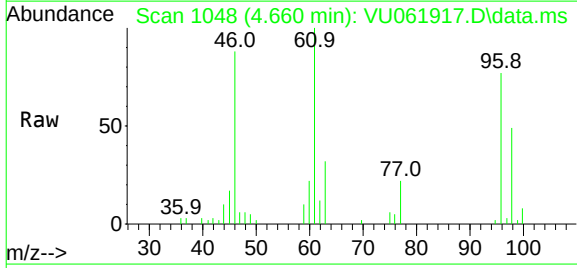

#29
1,1,1-Trichloroethane
Concen: 0.618 ug/L
RT: 5.306 min Scan# 1249
Delta R.T. 0.003 min
Lab File: VU061917.D
Acq: 21 Nov 2024 14:58


Tgt Ion: 97	Resp: 11540
Ion Ratio	Lower Upper
97 100	
99 64.6	51.4 77.2
61 48.5	37.8 56.6

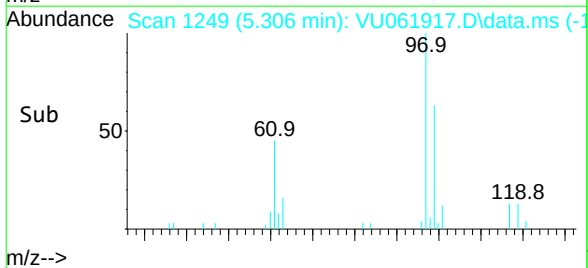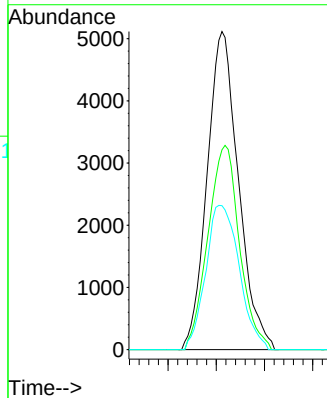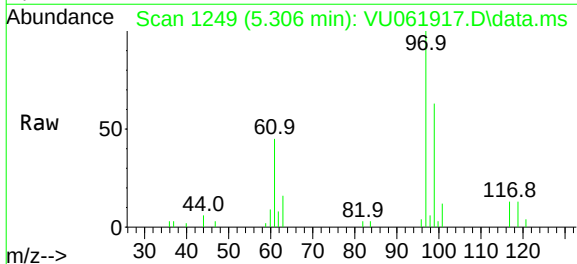



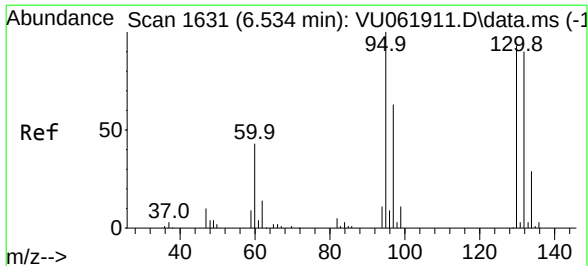


#34
Trichloroethene
Concen: 7.558 ug/L
RT: 6.534 min Scan# 1631
Delta R.T. -0.000 min
Lab File: VU061917.D
Acq: 21 Nov 2024 14:58

Instrument :
MSVOA_U
ClientSampleId :
BG3Q6DL



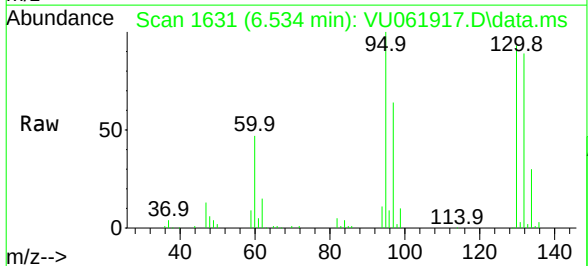



Tgt Ion:	95	Resp:	98744
Ion	Ratio	Lower	Upper
95	100		
97	64.1	45.9	85.3
132	88.6	63.8	118.4
130	92.6	65.5	121.7

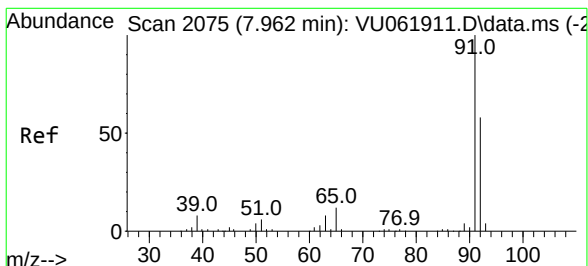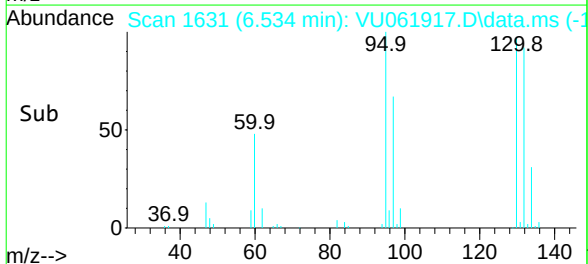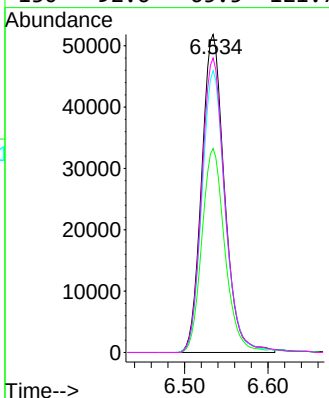

#42
Toluene
Concen: 0.195 ug/L
RT: 7.965 min Scan# 2076
Delta R.T. 0.003 min
Lab File: VU061917.D
Acq: 21 Nov 2024 14:58


Tgt Ion:	91	Resp:	10004
Ion	Ratio	Lower	Upper
91	100		
92	50.0	39.0	72.4

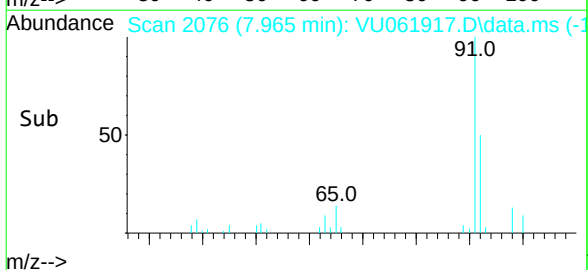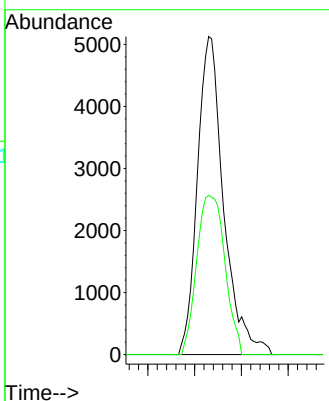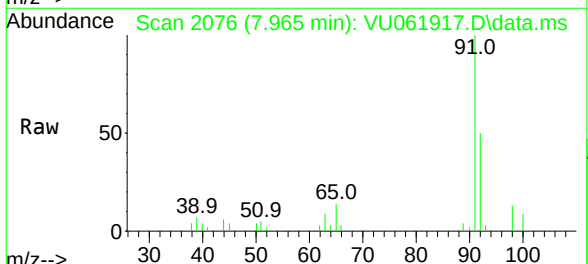



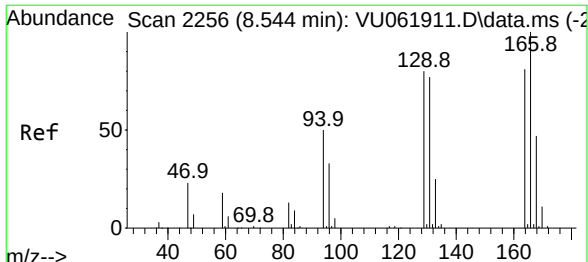


#47
Tetrachloroethene
Concen: 2.174 ug/L
RT: 8.547 min Scan# 2256
Delta R.T. 0.003 min
Lab File: VU061917.D
Acq: 21 Nov 2024 14:58

Instrument :
MSVOA_U
ClientSampleId :
BG3Q6DL



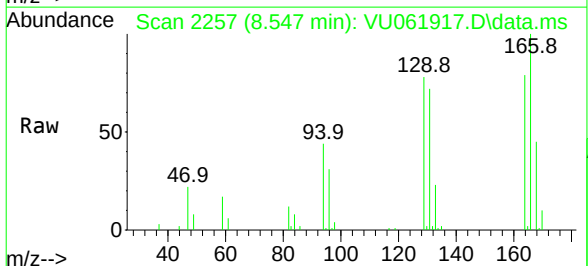



Tgt Ion	Ratio	Lower	Upper
164	100		
129	99.2	73.2	136.0
131	91.6	72.3	134.3
166	126.8	90.2	167.4

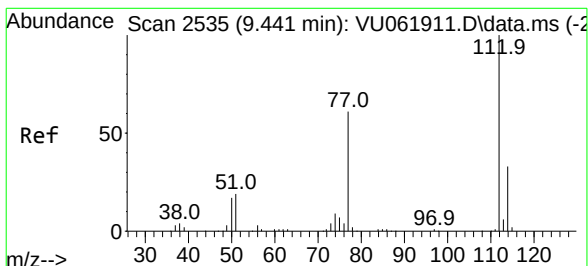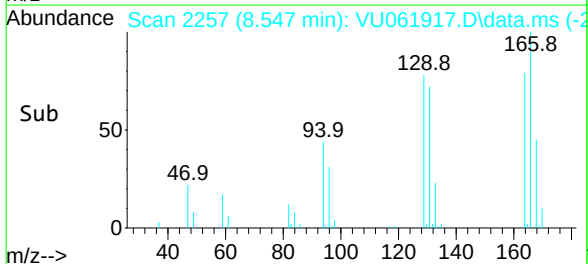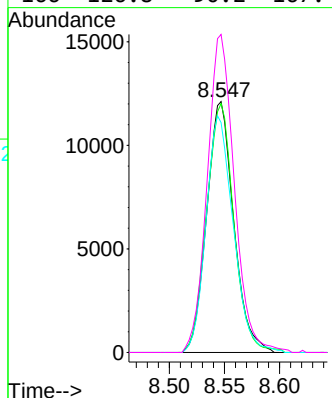

#51
Chlorobenzene
Concen: 0.183 ug/L
RT: 9.441 min Scan# 2535
Delta R.T. -0.000 min
Lab File: VU061917.D
Acq: 21 Nov 2024 14:58

Tgt Ion	Ratio	Lower	Upper
112	100		
114	35.1	23.0	42.6
77	65.3	50.5	75.7

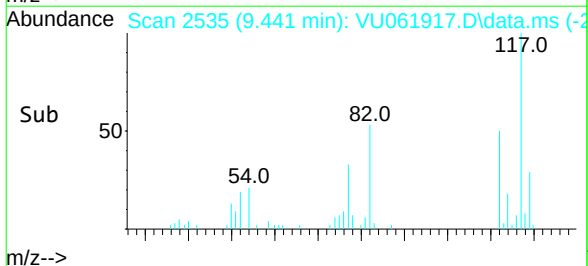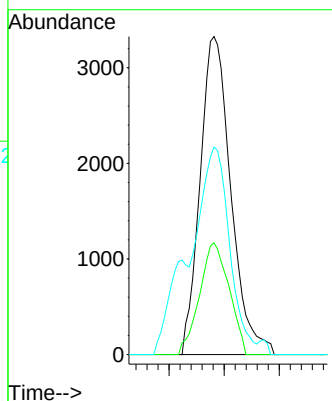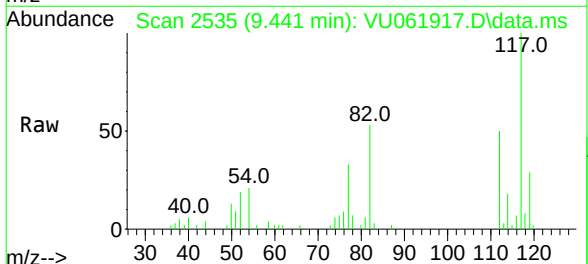

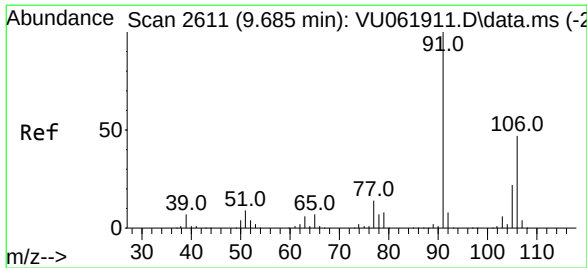

#53

m,p-Xylene

Concen: 0.153 ug/L

RT: 9.688 min Scan# 2611

Delta R.T. 0.003 min

Lab File: VU061917.D

Acq: 21 Nov 2024 14:58

Instrument :

MSVOA_U

ClientSampleId :





BG3Q6DL

Tgt Ion:106 Resp: 3320

Ion Ratio Lower Upper

106 100

91 230.7 147.6 274.0

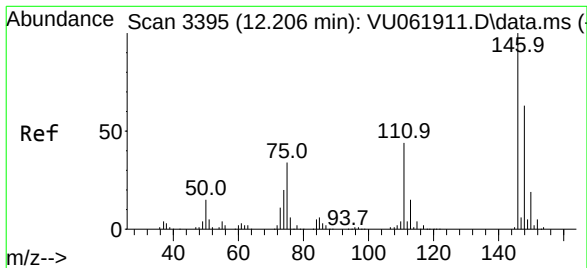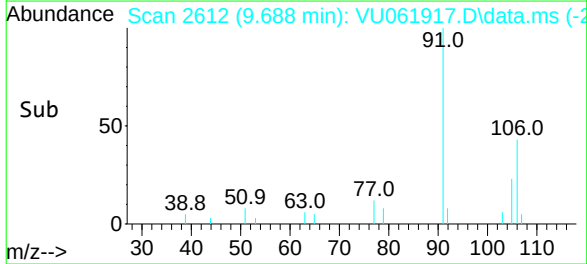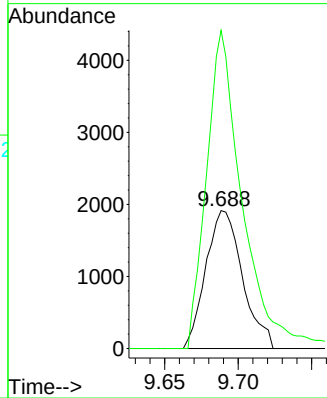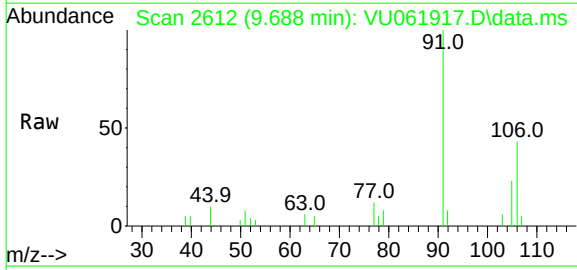

#67

1,2-Dichlorobenzene

Concen: 0.209 ug/L

RT: 12.209 min Scan# 3396

Delta R.T. 0.003 min

Lab File: VU061917.D

Acq: 21 Nov 2024 14:58

Tgt Ion:146 Resp: 3963

Ion Ratio Lower Upper

146 100

111 51.7 36.0 54.0

148 65.1 52.3 78.5

