

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112124\
 Data File : VU061937.D
 Acq On : 22 Nov 2024 00:01
 Operator : MD/SY
 Sample : P4903-15
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BG434

Quant Time: Nov 22 04:11:42 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR112024WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 22 00:07:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.241	114	136546	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	129632	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	56848	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	37323	5.572	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	111.400%
7) Chloroethane-d5	1.907	69	29385	4.959	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.200%
11) 1,1-Dichloroethene-d2	2.560	65	16930	6.327	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	126.600%#
20) 2-Butanone-d5	4.611	46	85126	40.473	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	80.940%
24) Chloroform-d	5.052	84	75968	4.649	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.000%
26) 1,2-Dichloroethane-d4	5.692	65	39093	4.649	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.000%
32) Benzene-d6	5.717	84	149916	5.936	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	118.800%
36) 1,2-Dichloropropane-d6	6.679	67	47321	5.514	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	110.200%
41) Toluene-d8	7.891	98	130901	6.214	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	124.200%
43) trans-1,3-Dichloroprop...	8.174	79	15526	4.887	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	97.800%
46) 2-Hexanone-d5	8.624	63	54724	37.737	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	75.480%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	34922	4.072	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	81.400%
66) 1,2-Dichlorobenzene-d4	12.187	152	44438	5.287	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.800%
Target Compounds					Qvalue	
13) Acetone	2.618	43	26349	18.145	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112124\
Data File : VU061937.D
Acq On : 22 Nov 2024 00:01
Operator : MD/SY
Sample : P4903-15
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG434


Quant Time: Nov 22 04:11:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR112024WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 22 00:07:48 2024
Response via : Initial Calibration

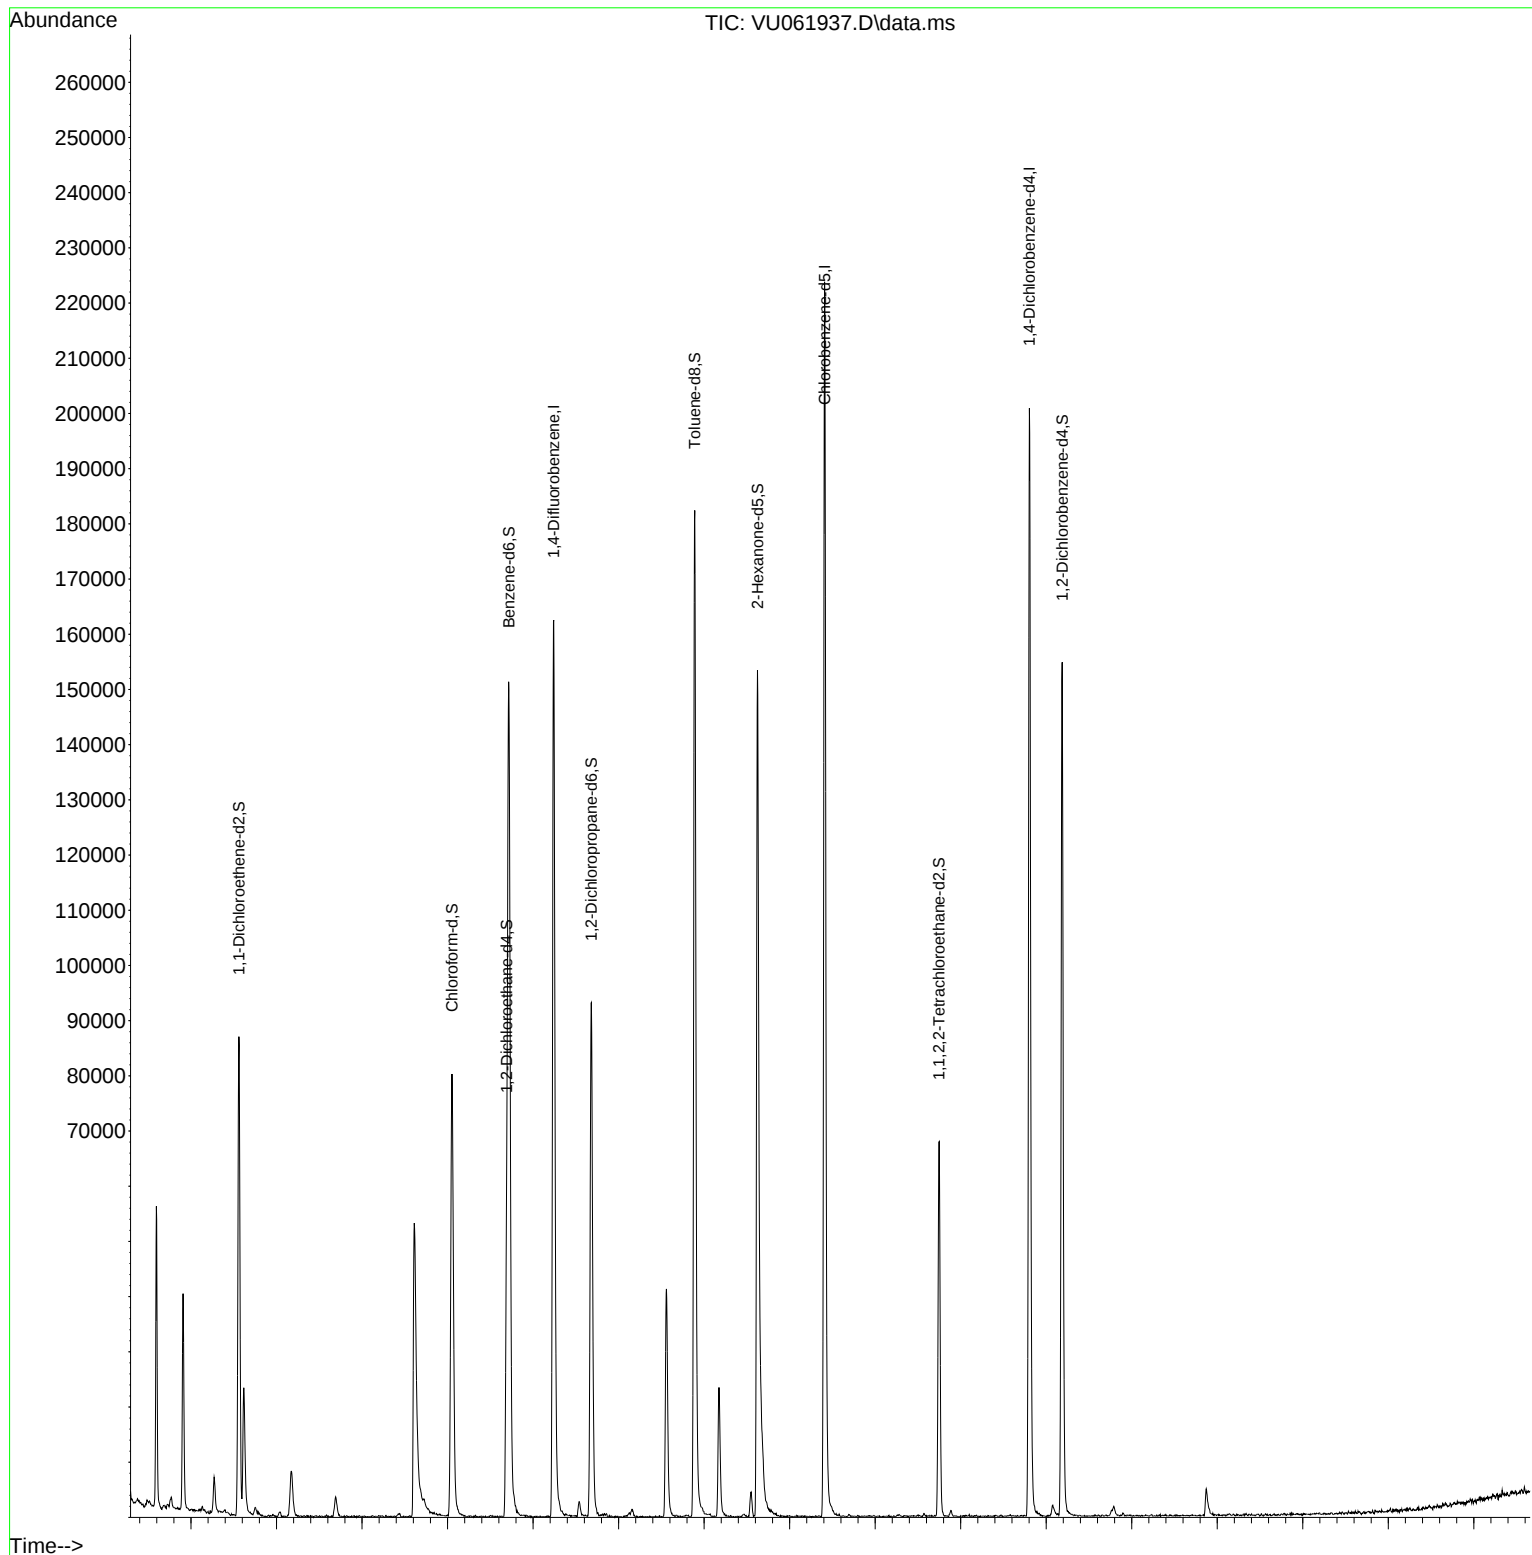

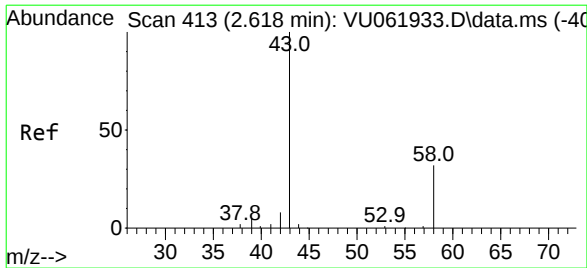

#13
 Acetone
 Concen: 18.145 ug/L
 RT: 2.618 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: VU061937.D
 Acq: 22 Nov 2024 00:01

Instrument :
 MSVOA_U
 ClientSampleId :
 BG434

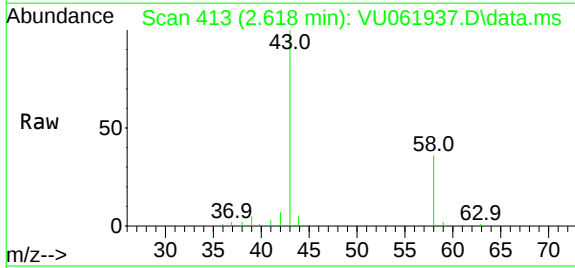

Tgt Ion: 43 Resp: 26349
 Ion Ratio Lower Upper
 43 100
 58 36.0 0.0 64.0

