

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112124\
 Data File : VU061938.D
 Acq On : 22 Nov 2024 00:25
 Operator : MD/SY
 Sample : P4903-16
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BG435

Quant Time: Nov 22 04:13:47 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR112024WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 22 00:07:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	139611	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	134117	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	57729	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	37559	5.485	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	109.600%
7) Chloroethane-d5	1.907	69	28955	4.780	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.600%
11) 1,1-Dichloroethene-d2	2.560	65	17360	6.345	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	127.000%#
20) 2-Butanone-d5	4.612	46	87046	40.478	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	80.960%
24) Chloroform-d	5.052	84	76421	4.574	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.400%
26) 1,2-Dichloroethane-d4	5.692	65	39561	4.601	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.000%
32) Benzene-d6	5.718	84	151583	5.801	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	116.000%
36) 1,2-Dichloropropane-d6	6.682	67	48862	5.503	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	110.000%
41) Toluene-d8	7.891	98	134333	6.164	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	123.200%
43) trans-1,3-Dichloroprop...	8.174	79	15881	4.831	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	96.600%
46) 2-Hexanone-d5	8.624	63	56541	37.686	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	75.380%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	36944	4.164	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	83.200%
66) 1,2-Dichlorobenzene-d4	12.187	152	44127	5.169	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.400%
Target Compounds						
13) Acetone	2.618	43	24879	16.756	ug/L	Qvalue 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112124\
Data File : VU061938.D
Acq On : 22 Nov 2024 00:25
Operator : MD/SY
Sample : P4903-16
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG435

Quant Time: Nov 22 04:13:47 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR112024WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 22 00:07:48 2024
Response via : Initial Calibration

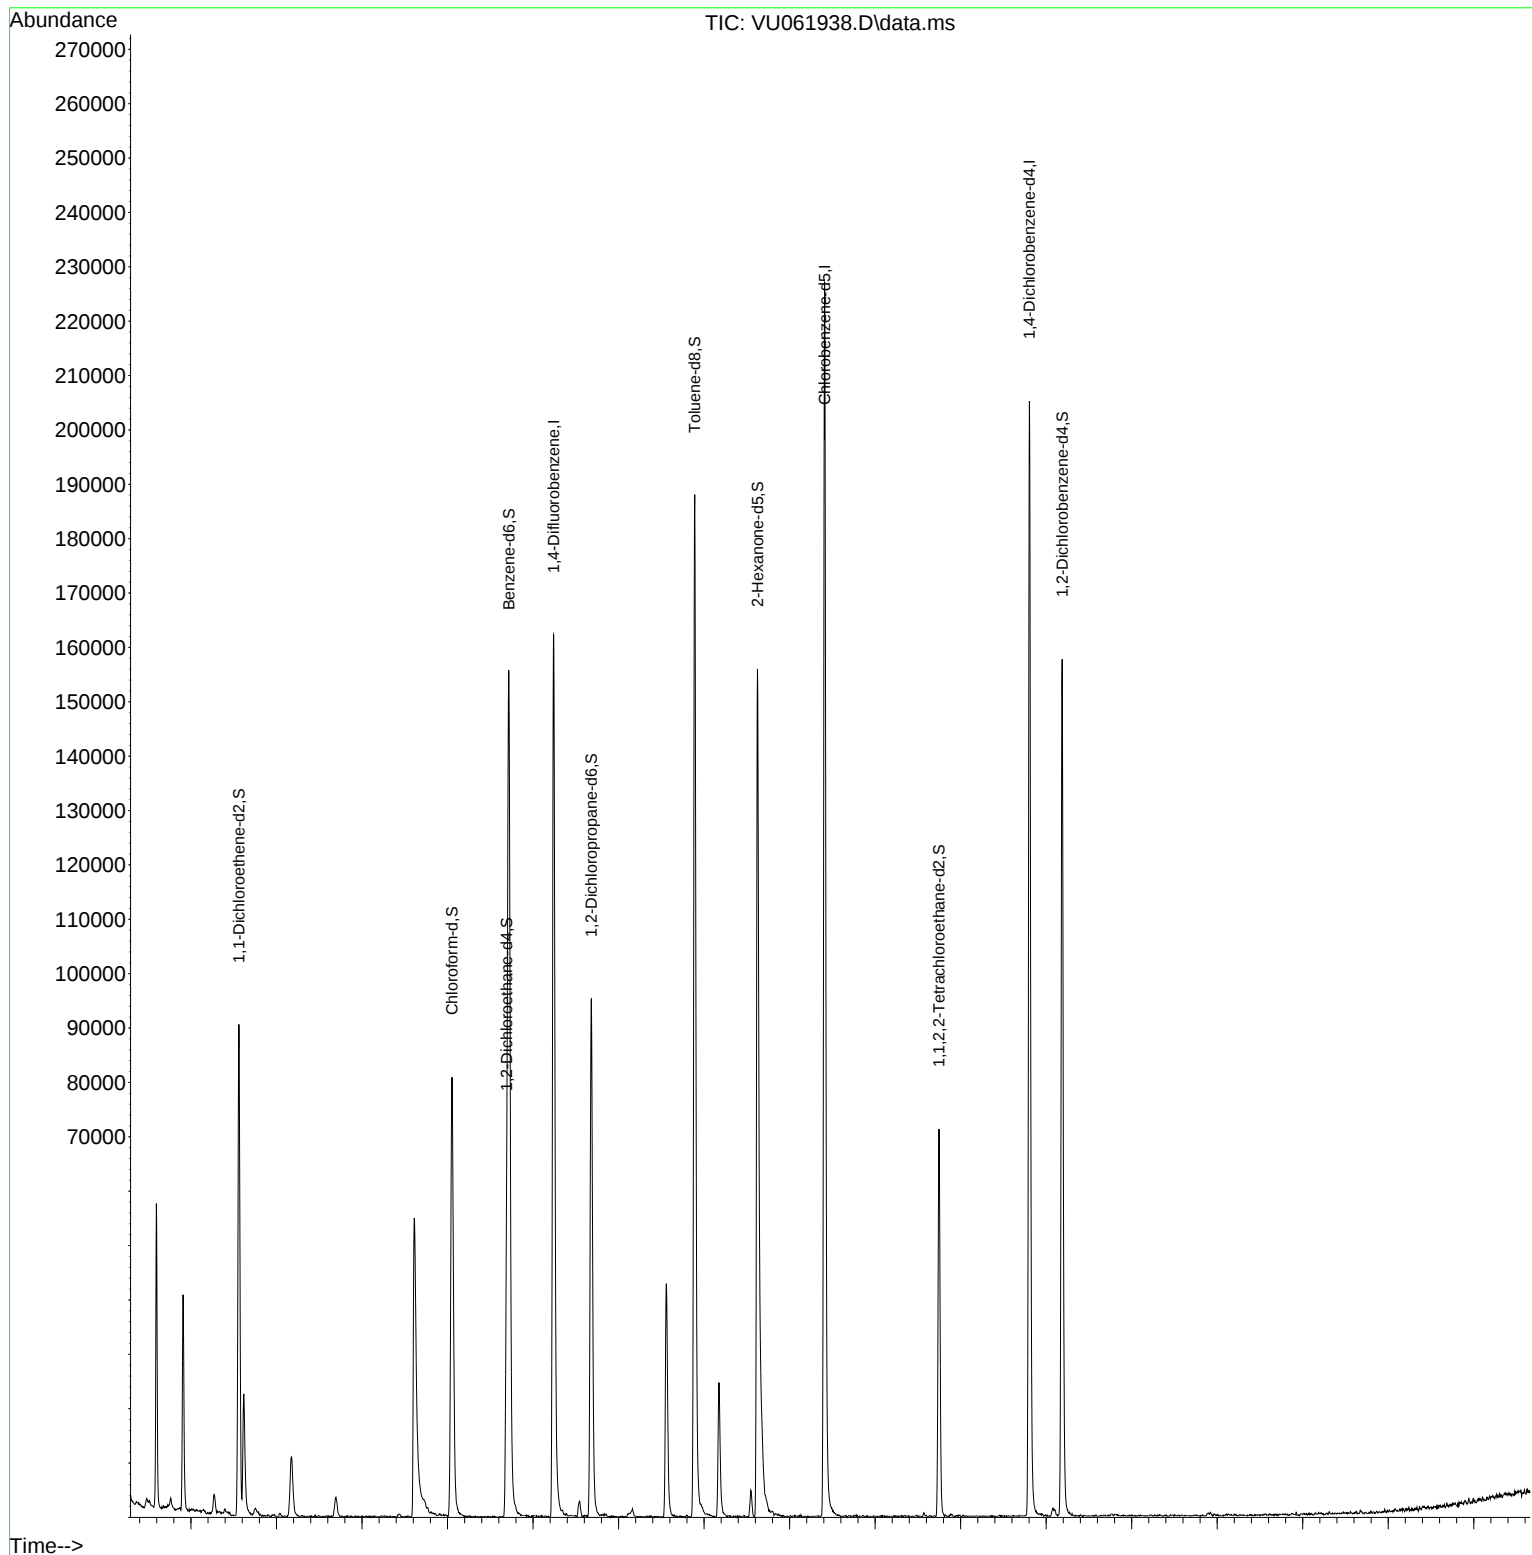

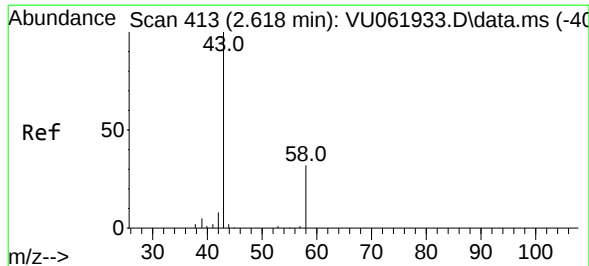

#13

Acetone

Concen: 16.756 ug/L

RT: 2.618 min Scan# 41

Delta R.T. 0.000 min

Lab File: VU061938.D


Acq: 22 Nov 2024 00:25

Instrument :

MSVOA_U

ClientSampleId :

BG435

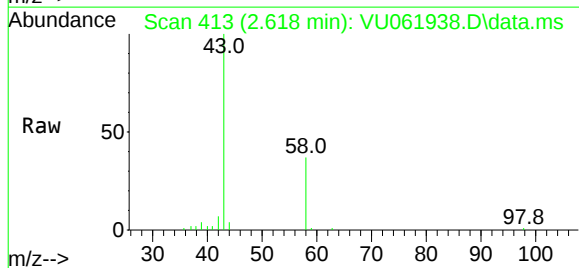

Tgt Ion: 43 Resp: 24879

Ion Ratio Lower Upper

43 100

58 39.0 0.0 64.0

