
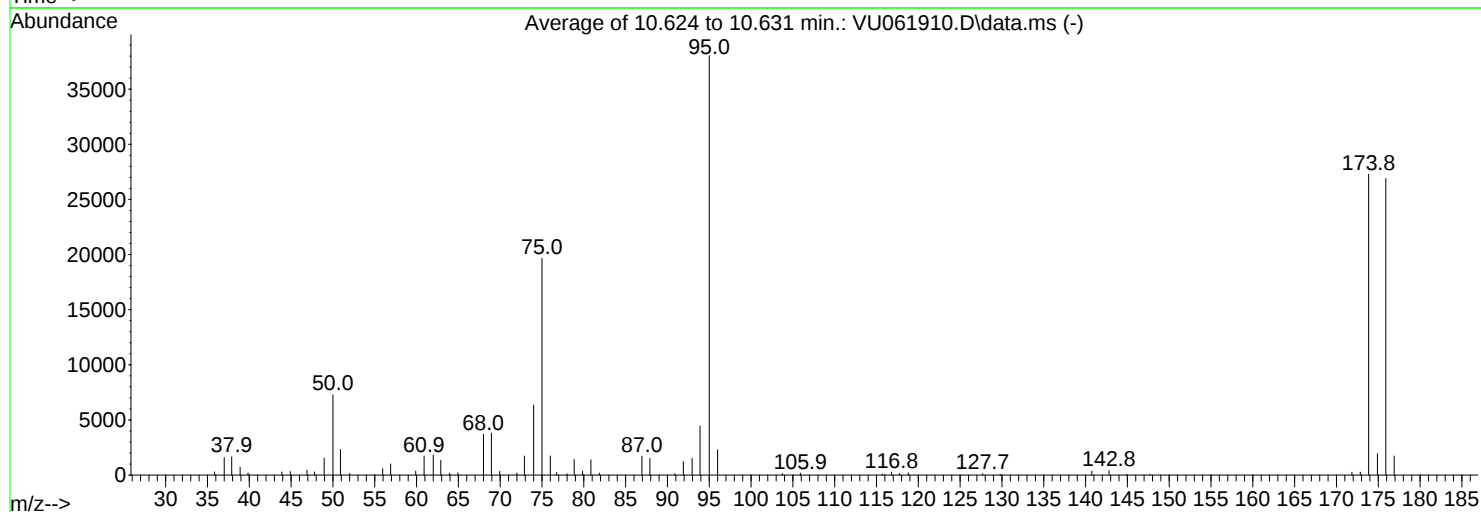


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112124\
Data File : VU061910.D
Acq On : 21 Nov 2024 10:47
Operator : MD/SY
Sample : BFB033
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB033

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR112024WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Mon Nov 25 01:25:39 2024

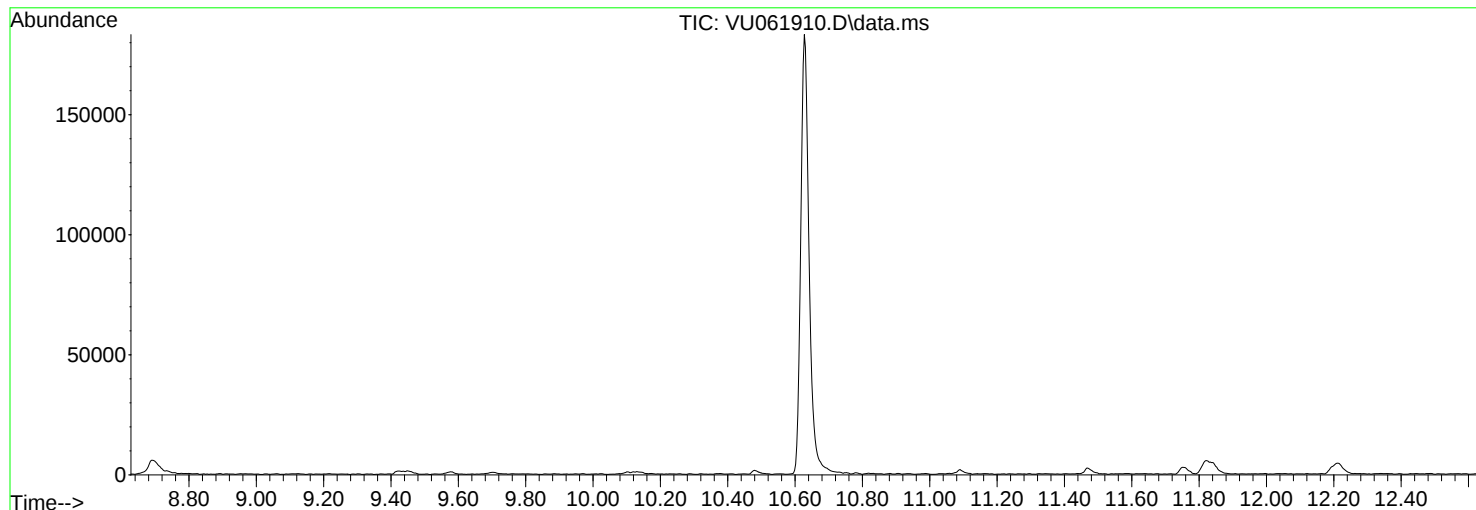

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	7282	PASS
75	95	30	80	51.7	19664	PASS
95	95	100	100	100.0	38032	PASS
96	95	5	9	6.0	2299	PASS
173	174	0.00	2	1.0	266	PASS
174	95	50	120	71.8	27288	PASS
175	174	5	9	7.1	1951	PASS
176	174	95	101	98.6	26907	PASS
177	176	5	9	6.4	1730	PASS

m/z	Abundance
43.90	398.0

Instrument :
MSVOA_U
ClientSampleId :
BFB033

m/z	Abundance
35.90	274.0
37.00	1574.0
37.90	1658.0
38.90	740.0
39.90	179.0
43.90	680.0
44.90	335.0
46.90	418.0
47.80	293.0
49.00	1483.0
50.00	7294.0
50.90	2311.0
52.00	160.0
55.00	110.0
55.90	540.0
56.90	995.0
59.90	352.0
60.90	1801.0
62.00	1833.0
62.90	1323.0
64.00	152.0
65.00	202.0
68.00	3599.0
68.90	3603.0
69.90	304.0
72.00	159.0
72.90	1703.0
74.00	6019.0
75.00	19104.0
76.00	1709.0
76.80	238.0
78.00	113.0
78.80	1367.0
79.90	332.0
80.80	1383.0
81.80	160.0
87.00	1771.0
87.90	1481.0
90.90	122.0
91.90	1179.0
93.00	1532.0
93.90	4146.0
95.00	37040.0
96.00	2222.0
103.70	138.0
105.90	181.0
116.00	109.0
116.80	269.0
117.80	166.0
118.80	233.0
127.70	126.0
140.70	314.0
142.80	331.0
171.80	220.0
172.90	282.0
173.80	25544.0
174.90	1946.0
175.90	25496.0
176.90	1652.0

Instrument :
MSVOA_U
ClientSampleId :
BFB033

m/z	Abundance
35.80	302.0
37.00	1626.0
37.90	1724.0
38.90	713.0
39.80	181.0
43.90	738.0
44.90	345.0
46.90	467.0
47.80	311.0
48.90	1609.0
50.00	7554.0
50.90	2414.0
52.00	153.0
56.00	587.0
56.90	1045.0
59.90	374.0
60.90	1777.0
62.00	1914.0
62.90	1381.0
63.90	151.0
65.00	197.0
68.00	3778.0
68.90	3931.0
70.00	351.0
72.00	184.0
72.90	1797.0
74.00	6542.0
75.00	20288.0
76.00	1796.0
76.80	260.0
78.00	117.0
78.90	1473.0
79.90	355.0
80.90	1431.0
81.90	176.0
86.90	1788.0
87.90	1584.0
90.90	128.0
91.90	1295.0
92.90	1567.0
93.90	4624.0
95.00	39360.0
96.00	2326.0
103.70	138.0
105.90	180.0
115.70	116.0
116.80	280.0
117.80	154.0
118.80	216.0
127.70	143.0
129.80	114.0
140.80	355.0
142.80	402.0
144.90	101.0
147.70	111.0
171.80	255.0
172.90	279.0
173.90	28144.0
174.90	1995.0
175.90	27864.0
176.90	1773.0

Instrument :
MSVOA_U
ClientSampleId :
BFB033

m/z	Abundance
35.90	281.0
37.00	1567.0
37.90	1592.0
38.90	673.0
39.80	209.0
43.90	652.0
44.90	296.0
46.90	461.0
47.80	249.0
48.90	1514.0
50.00	6999.0
50.90	2223.0
52.00	123.0
56.00	604.0
56.90	989.0
59.90	342.0
60.90	1593.0
62.00	1737.0
62.90	1328.0
63.90	153.0
64.90	198.0
68.00	3737.0
69.00	3910.0
70.00	360.0
72.00	219.0
72.90	1692.0
74.00	6513.0
75.00	19600.0
76.00	1719.0
76.70	216.0
78.00	121.0
78.90	1404.0
79.80	387.0
80.90	1349.0
81.90	215.0
86.90	1594.0
87.90	1499.0
90.90	136.0
91.90	1234.0
92.90	1474.0
93.90	4609.0
95.00	37696.0
96.00	2350.0
103.80	149.0
105.90	182.0
115.70	160.0
116.80	275.0
117.70	119.0
118.80	190.0
127.70	130.0
129.80	116.0
140.80	399.0
142.80	454.0
144.90	106.0
147.70	116.0
171.90	282.0
172.80	236.0
173.90	28176.0
174.90	1912.0
175.90	27360.0
176.90	1765.0

Instrument :
MSVOA_U
ClientSampleId :
BFB033