

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
 Data File : VU063771.D
 Acq On : 21 Nov 2025 16:10
 Operator : MD/SY
 Sample : Q3688-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Quant Time: Nov 21 22:32:26 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Nov 21 22:28:08 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.219	114	329913	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.393	117	315330	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.788	152	154810	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.583	65	116413	40.862	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	81.720%
7) Chloroethane-d5	1.891	69	96591	44.008	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	88.020%
11) 1,1-Dichloroethene-d2	2.541	63	163990	33.208	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	66.420%
21) 2-Butanone-d5	4.595	46	141725	87.261	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	87.260%
24) Chloroform-d	5.029	84	212552	44.467	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.940%
26) 1,2-Dichloroethane-d4	5.669	65	149839	47.672	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.340%
32) Benzene-d6	5.695	84	427162	46.215	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.440%
36) 1,2-Dichloropropane-d6	6.663	67	127579	47.018	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	94.040%
41) Toluene-d8	7.872	98	391994	44.667	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.340%
43) trans-1,3-Dichloroprop...	8.155	79	46308	41.298	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	82.600%
47) 2-Hexanone-d5	8.611	63	88263	89.466	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	89.470%
56) 1,1,2,2-Tetrachloroeth...	10.730	84	188573	47.522	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	95.040%
66) 1,2-Dichlorobenzene-d4	12.167	152	142729	48.839	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.680%
Target Compounds						
					Qvalue	
69) 1,3,5-Trichlorobenzene	13.820	180	4235	1.197	ug/L	97
70) 1,2,4-trichlorobenzene	13.820	180	4235	1.435	ug/L	97
71) Naphthalene	14.068	128	18369	2.339	ug/L	98
72) 1,2,3-Trichlorobenzene	14.306	180	4445	1.589	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
Data File : VU063771.D
Acq On : 21 Nov 2025 16:10
Operator : MD/SY
Sample : Q3688-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Time: Nov 21 22:32:26 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 21 22:28:08 2025
Response via : Initial Calibration




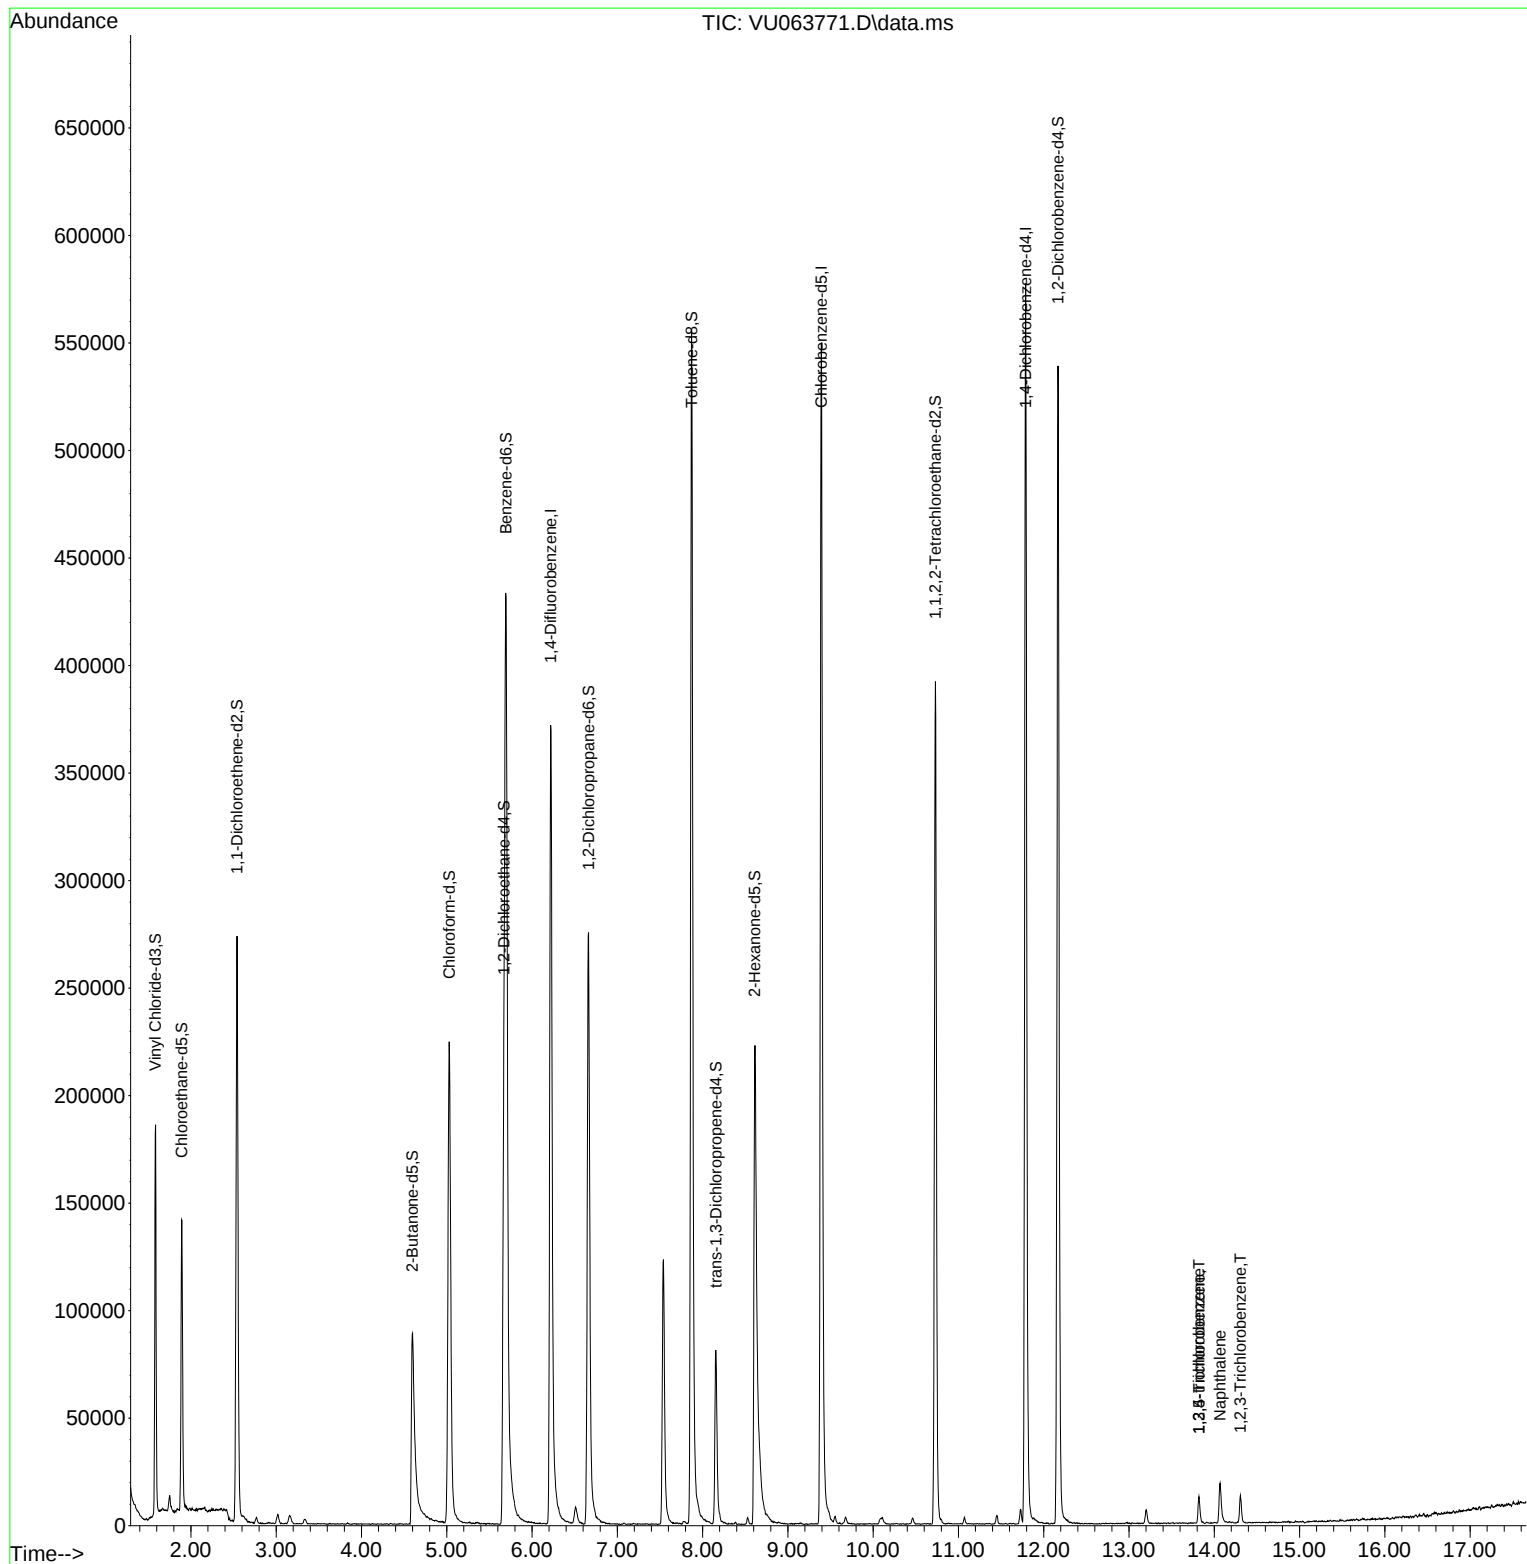


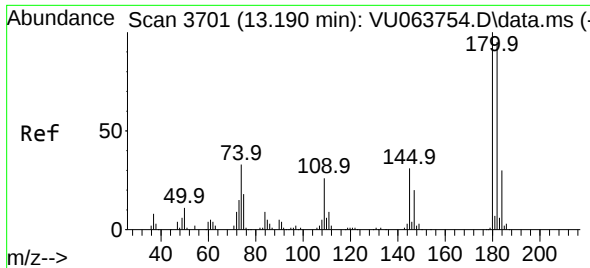

#69
 1,3,5-Trichlorobenzene
 Concen: 1.197 ug/L
 RT: 13.820 min Scan# 3897
 Delta R.T. 0.630 min
 Lab File: VU063771.D
 Acq: 21 Nov 2025 16:10




Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001


Tgt Ion:	180	Resp:	4235
Ion Ratio	Lower	Upper	
180	100		
182	91.4	76.4	114.6
184	29.7	24.4	36.6
145	30.5	25.8	38.6

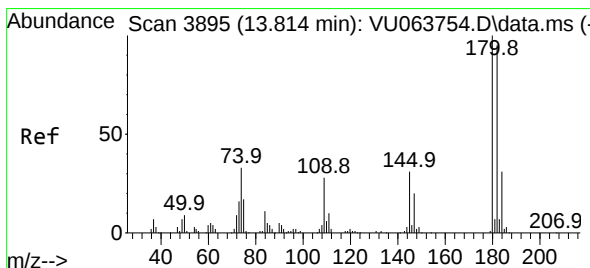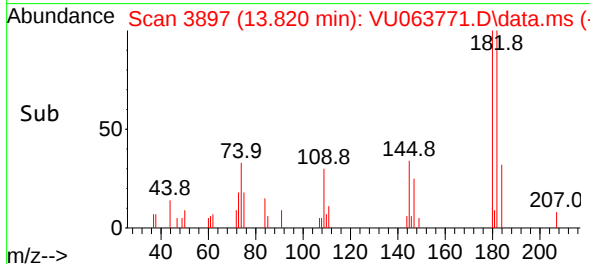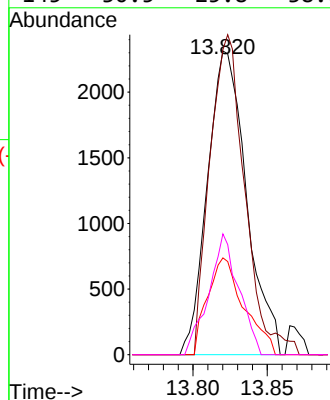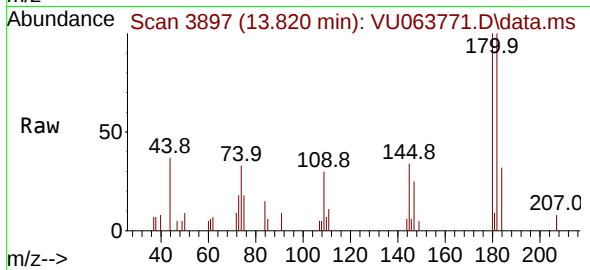

#70
 1,2,4-trichlorobenzene
 Concen: 1.435 ug/L
 RT: 13.820 min Scan# 3897
 Delta R.T. 0.006 min
 Lab File: VU063771.D
 Acq: 21 Nov 2025 16:10

Tgt Ion:	180	Resp:	4235
Ion Ratio	Lower	Upper	
180	100		
182	91.4	75.8	113.8
145	30.5	25.7	38.5


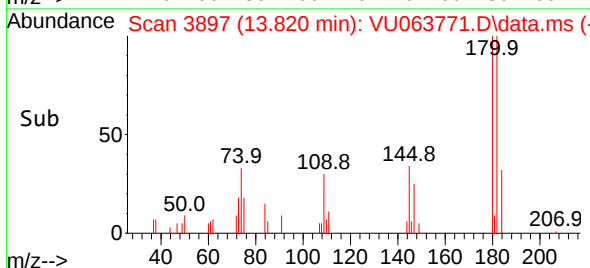
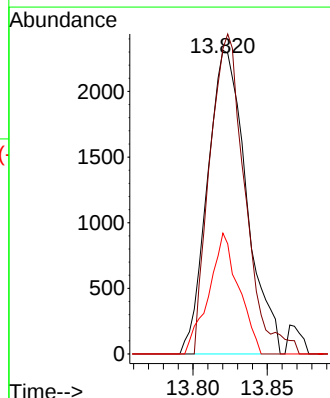
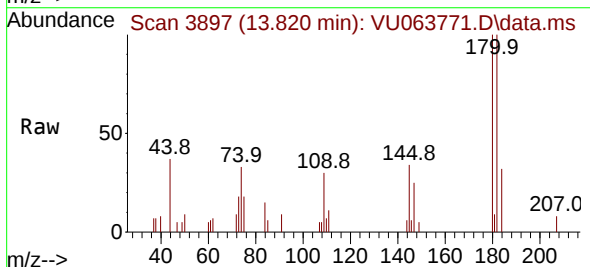


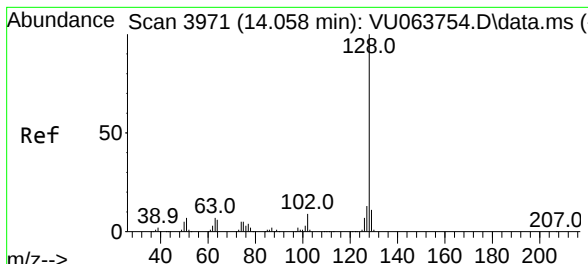

#71
Naphthalene
Concen: 2.339 ug/L
RT: 14.068 min Scan# 3971
Delta R.T. 0.010 min
Lab File: VU063771.D
Acq: 21 Nov 2025 16:10

Instrument : MSVOA_U
ClientSampleId : VHBLK001

Tgt Ion:	128	Resp:	18369
Ion Ratio	Lower	Upper	
128	100		
127	12.7	10.3	15.5
129	9.8	8.7	13.1

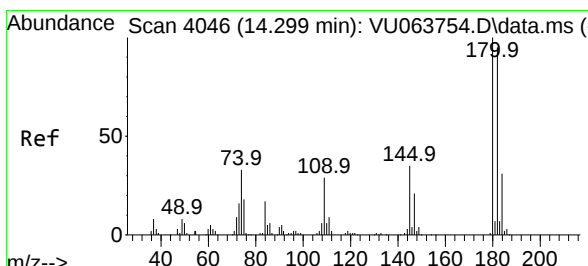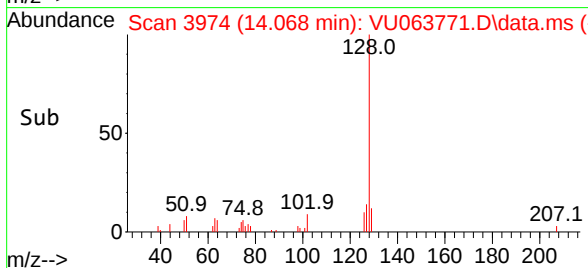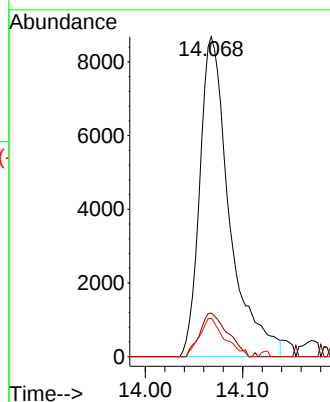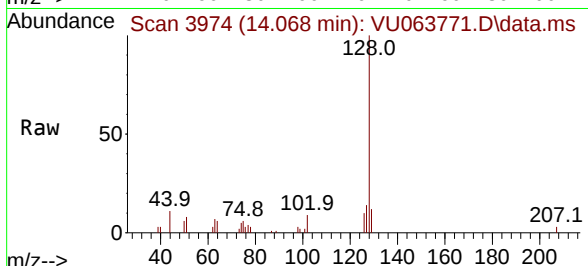

#72
1,2,3-Trichlorobenzene
Concen: 1.589 ug/L
RT: 14.306 min Scan# 4048
Delta R.T. 0.006 min
Lab File: VU063771.D
Acq: 21 Nov 2025 16:10

Tgt Ion:	180	Resp:	4445
Ion Ratio	Lower	Upper	
180	100		
182	100.5	76.9	115.3
145	30.3	26.6	39.8

