

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
 Data File : VU063756.D
 Acq On : 21 Nov 2025 09:36
 Operator : MD/SY
 Sample : VU1121WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK130

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M

Title : VOC Analysis

Signal : TIC: VU063756.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.583	84	91	105	rBV	173580	192944	15.52%	2.053%
2	1.894	180	188	202	rVB	131235	169977	13.67%	1.809%
3	2.480	368	370	374	rBV4	765	546	0.04%	0.006%
4	2.541	377	389	405	rBV	265087	438645	35.28%	4.668%
5	2.734	446	449	451	rBV2	467	274	0.02%	0.003%
6	2.769	452	460	467	rVB4	2398	3747	0.30%	0.040%
7	2.814	471	474	479	rVB	334	273	0.02%	0.003%
8	2.939	510	513	515	rBV2	442	276	0.02%	0.003%
9	3.013	528	536	549	rBV5	3071	5828	0.47%	0.062%
10	3.158	570	581	593	rBV3	3266	7229	0.58%	0.077%
11	3.206	593	596	601	rVV3	432	326	0.03%	0.003%
12	3.235	601	605	610	rVB	254	271	0.02%	0.003%
13	3.296	617	624	627	rVB2	313	354	0.03%	0.004%
14	3.341	627	638	640	rBV4	2251	3895	0.31%	0.041%
15	3.518	690	693	697	rBV2	313	252	0.02%	0.003%
16	3.576	708	711	716	rBV2	332	271	0.02%	0.003%
17	3.814	780	785	787	rBV2	293	239	0.02%	0.003%
18	3.827	787	789	792	rVV	413	273	0.02%	0.003%
19	3.846	792	795	799	rVV	357	314	0.03%	0.003%
20	3.997	837	842	848	rBV2	325	412	0.03%	0.004%
21	4.139	883	886	890	rVB2	333	259	0.02%	0.003%
22	4.164	890	894	902	rBV	598	901	0.07%	0.010%
23	4.325	935	944	948	rBV2	333	433	0.03%	0.005%
24	4.528	1002	1007	1010	rBV	317	294	0.02%	0.003%
25	4.599	1019	1029	1062	rBV	85680	248826	20.01%	2.648%
26	5.029	1147	1163	1198	rBV	209349	487575	39.22%	5.189%
27	5.351	1255	1263	1276	rVB5	1397	3006	0.24%	0.032%
28	5.489	1295	1306	1308	rBV3	854	989	0.08%	0.011%
29	5.560	1322	1328	1331	rBV2	242	259	0.02%	0.003%
30	5.695	1349	1370	1422	rBV2	415162	1243219	100.00%	13.230%
31	6.161	1513	1515	1521	rVB2	307	244	0.02%	0.003%
32	6.219	1521	1533	1574	rBV	343389	714454	57.47%	7.603%
33	6.515	1613	1625	1637	rBV10	6640	14662	1.18%	0.156%
34	6.660	1656	1670	1698	rBV	254252	534318	42.98%	5.686%
35	6.872	1733	1736	1741	rVB3	538	443	0.04%	0.005%
36	6.920	1748	1751	1754	rBV2	413	306	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
 Data File : VU063756.D
 Acq On : 21 Nov 2025 09:36
 Operator : MD/SY
 Sample : VU1121WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK130

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

37	7.078	1794	1800	1803	rBV3	618	738	0.06%	0.008%
38	7.158	1817	1825	1827	rBV	234	256	0.02%	0.003%
39	7.296	1862	1868	1872	rBV	262	246	0.02%	0.003%
40	7.541	1931	1944	1973	rBV	122100	232241	18.68%	2.471%
41	7.692	1987	1991	1995	rBV3	439	362	0.03%	0.004%
42	7.772	2010	2016	2018	rBV3	1969	1686	0.14%	0.018%
43	7.872	2034	2047	2067	rBV	536982	987282	79.41%	10.506%
44	8.155	2124	2135	2156	rBV	76962	140254	11.28%	1.493%
45	8.306	2180	2182	2188	rVB2	360	308	0.02%	0.003%
46	8.386	2197	2207	2210	rBV6	1111	1497	0.12%	0.016%
47	8.441	2222	2224	2232	rVB2	306	313	0.03%	0.003%
48	8.531	2244	2252	2262	rBV6	2835	4273	0.34%	0.045%
49	8.614	2267	2278	2322	rBV2	208335	550197	44.26%	5.855%
50	8.888	2355	2363	2364	rBV3	757	767	0.06%	0.008%
51	8.994	2394	2396	2401	rVB	466	308	0.02%	0.003%
52	9.020	2401	2404	2405	rBV	361	227	0.02%	0.002%
53	9.142	2438	2442	2443	rBV3	512	321	0.03%	0.003%
54	9.203	2456	2461	2465	rVB2	629	499	0.04%	0.005%
55	9.241	2465	2473	2477	rBV2	532	550	0.04%	0.006%
56	9.338	2499	2503	2507	rVB2	289	251	0.02%	0.003%
57	9.393	2507	2520	2563	rBV	510730	929945	74.80%	9.896%
58	9.547	2563	2568	2581	rVV3	3913	6546	0.53%	0.070%
59	9.614	2585	2589	2591	rBV4	347	275	0.02%	0.003%
60	9.676	2600	2608	2617	rBV6	2655	4344	0.35%	0.046%
61	9.746	2626	2630	2632	rBV2	344	225	0.02%	0.002%
62	9.942	2689	2691	2697	rVB2	332	301	0.02%	0.003%
63	9.981	2699	2703	2708	rVB	239	239	0.02%	0.003%
64	10.020	2712	2715	2720	rBV2	253	285	0.02%	0.003%
65	10.087	2726	2736	2740	rBV3	2798	5130	0.41%	0.055%
66	10.254	2780	2788	2789	rBV2	271	318	0.03%	0.003%
67	10.274	2791	2794	2799	rVB2	649	524	0.04%	0.006%
68	10.302	2799	2803	2804	rBV2	363	227	0.02%	0.002%
69	10.335	2809	2813	2822	rBV2	441	635	0.05%	0.007%
70	10.460	2845	2852	2860	rBV2	3582	5130	0.41%	0.055%
71	10.618	2894	2901	2915	rBV3	2585	4511	0.36%	0.048%
72	10.730	2923	2936	2955	rBV	368371	608017	48.91%	6.470%
73	10.875	2977	2981	2985	rBV4	462	544	0.04%	0.006%
74	11.068	3030	3041	3056	rBV4	2762	5456	0.44%	0.058%
75	11.331	3121	3123	3129	rVB2	363	320	0.03%	0.003%
76	11.450	3152	3160	3171	rVB	3587	5164	0.42%	0.055%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
 Data File : VU063756.D
 Acq On : 21 Nov 2025 09:36
 Operator : MD/SY
 Sample : VU1121WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK130

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

77	11.537	3183	3187	3190	rVB	369	274	0.02%	0.003%
78	11.556	3190	3193	3200	rVB2	247	255	0.02%	0.003%
79	11.624	3210	3214	3217	rBV3	340	258	0.02%	0.003%
80	11.663	3223	3226	3229	rBV	388	301	0.02%	0.003%
81	11.727	3238	3246	3253	rBV6	4915	7987	0.64%	0.085%
82	11.788	3253	3265	3290	rVV	514168	885630	71.24%	9.425%
83	12.045	3340	3345	3347	rBV3	238	268	0.02%	0.003%
84	12.058	3347	3349	3354	rVB2	343	293	0.02%	0.003%
85	12.167	3370	3383	3408	rBV	507460	864362	69.53%	9.198%
86	12.499	3483	3486	3492	rVB	372	324	0.03%	0.003%
87	12.743	3559	3562	3564	rBV2	462	275	0.02%	0.003%
88	12.810	3580	3583	3585	rBV2	363	241	0.02%	0.003%
89	12.942	3621	3624	3626	rBV	376	240	0.02%	0.003%
90	12.984	3635	3637	3639	rBV3	637	366	0.03%	0.004%
91	13.061	3655	3661	3668	rBV3	442	614	0.05%	0.007%
92	13.199	3697	3704	3713	rBV6	4178	6993	0.56%	0.074%
93	13.402	3764	3767	3771	rBV2	231	262	0.02%	0.003%
94	13.476	3787	3790	3794	rBV3	281	255	0.02%	0.003%
95	13.820	3888	3897	3907	rBV4	8407	13313	1.07%	0.142%
96	14.071	3966	3975	3992	rBV2	10888	20830	1.68%	0.222%
97	14.306	4040	4048	4059	rVV5	8729	14188	1.14%	0.151%
98	14.862	4218	4221	4224	rBV2	455	373	0.03%	0.004%
99	15.170	4312	4317	4321	rBV3	775	763	0.06%	0.008%
100	15.341	4365	4370	4373	rBV4	1037	967	0.08%	0.010%




Sum of corrected areas: 9396878

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
Data File : VU063756.D
Acq On : 21 Nov 2025 09:36
Operator : MD/SY
Sample : VU1121WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK130

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

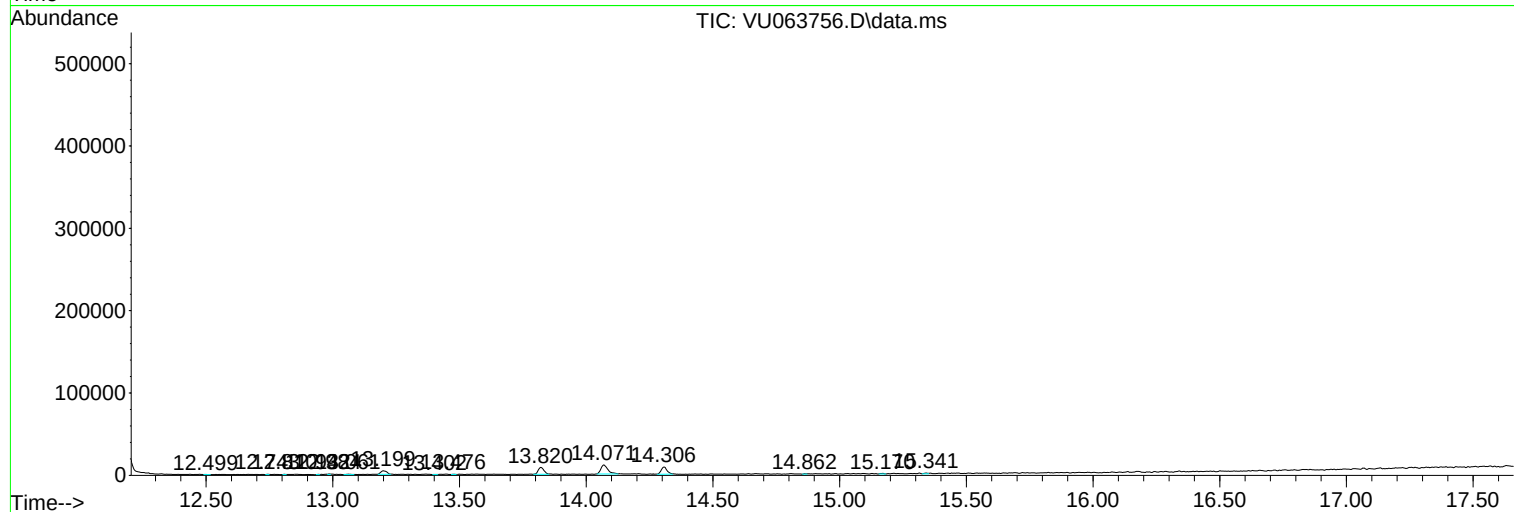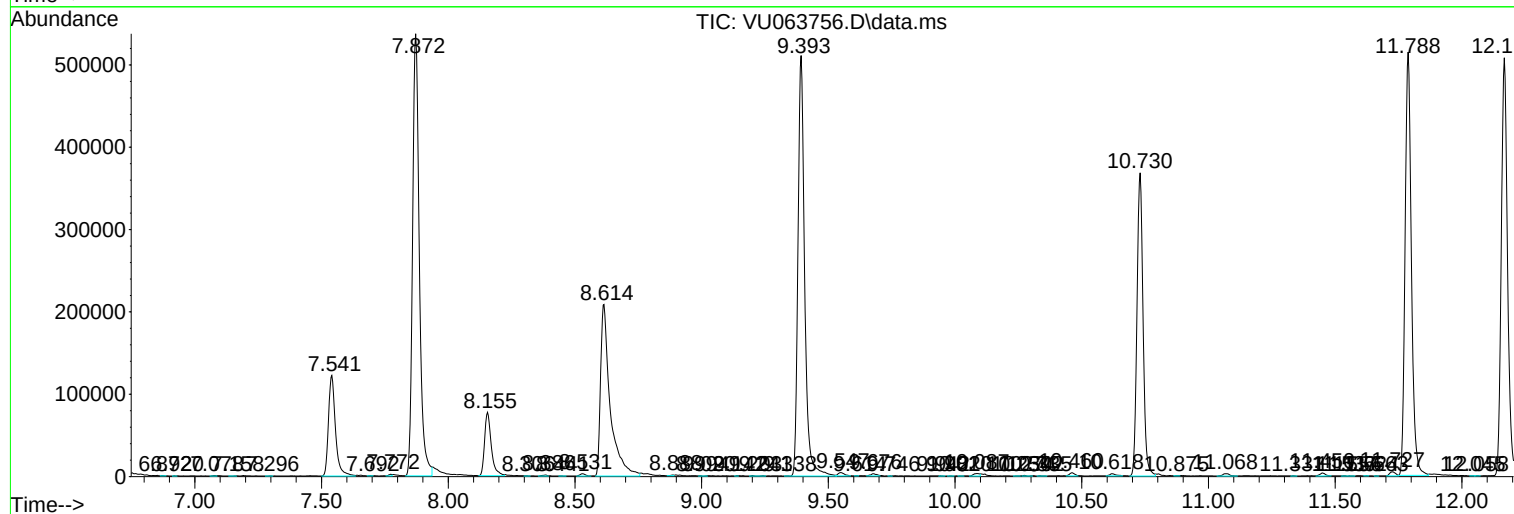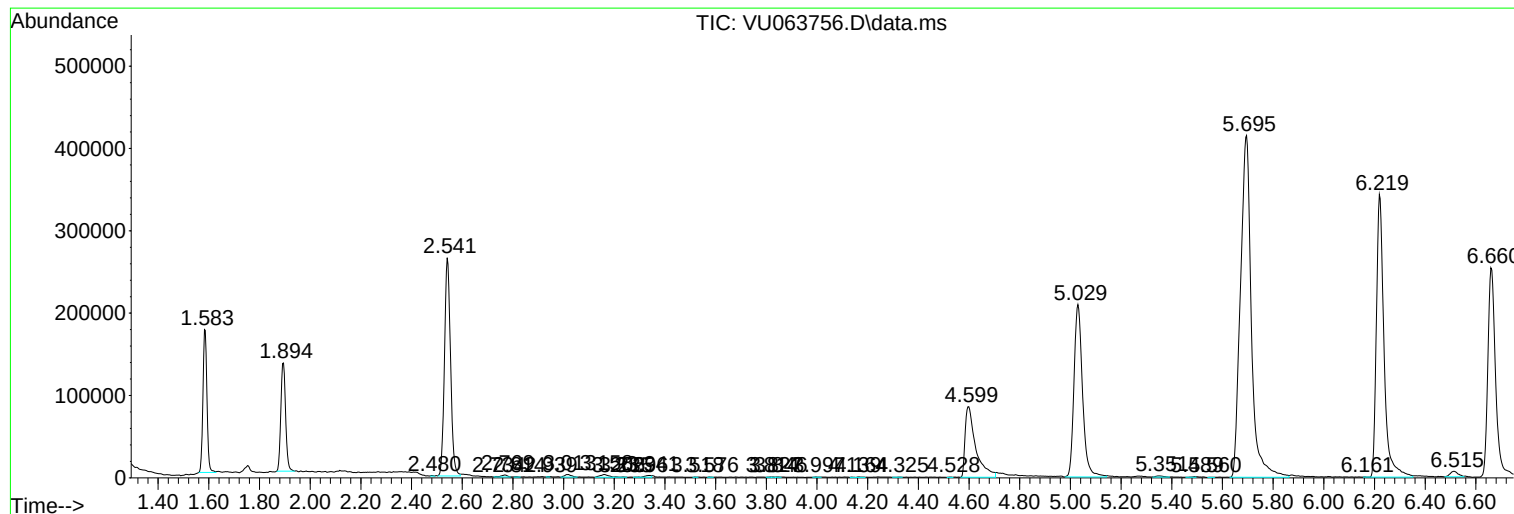

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
Data File : VU063756.D
Acq On : 21 Nov 2025 09:36
Operator : MD/SY
Sample : VU1121WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK130

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
Data File : VU063756.D
Acq On : 21 Nov 2025 09:36
Operator : MD/SY
Sample : VU1121WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK130

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc