

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
 Data File : VU063758.D
 Acq On : 21 Nov 2025 10:30
 Operator : MD/SY
 Sample : Q3688-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 TBGW-20251119

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M

Title : VOC Analysis

Signal : TIC: VU063758.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.586	84	92	103	rBV	178697	198364	15.99%	2.088%
2	1.894	180	188	205	rVB	136144	176882	14.26%	1.862%
3	2.541	377	389	403	rBV	268707	444300	35.82%	4.678%
4	2.747	443	453	472	rBV4	7727	19491	1.57%	0.205%
5	3.023	528	539	547	rBV3	3052	5312	0.43%	0.056%
6	3.158	566	581	600	rBV	20780	48056	3.87%	0.506%
7	3.335	629	636	641	rVV4	1326	1746	0.14%	0.018%
8	3.409	655	659	664	rVB2	270	264	0.02%	0.003%
9	3.602	715	719	724	rVB2	223	216	0.02%	0.002%
10	3.656	731	736	738	rBV2	244	231	0.02%	0.002%
11	3.701	743	750	753	rBV2	274	284	0.02%	0.003%
12	3.779	770	774	779	rVB2	338	318	0.03%	0.003%
13	3.814	779	785	790	rBV2	215	237	0.02%	0.002%
14	3.853	792	797	801	rVB3	344	370	0.03%	0.004%
15	3.894	807	810	815	rVB2	331	224	0.02%	0.002%
16	4.000	839	843	846	rBV	361	325	0.03%	0.003%
17	4.065	859	863	866	rVV2	365	265	0.02%	0.003%
18	4.107	872	876	882	rBV2	200	242	0.02%	0.003%
19	4.364	953	956	963	rVB2	359	348	0.03%	0.004%
20	4.418	967	973	977	rBV	252	314	0.03%	0.003%
21	4.599	1015	1029	1063	rBV	86492	254413	20.51%	2.678%
22	4.943	1134	1136	1140	rVB3	370	202	0.02%	0.002%
23	5.029	1148	1163	1190	rBV	210168	485282	39.13%	5.109%
24	5.319	1251	1253	1256	rVB2	599	385	0.03%	0.004%
25	5.351	1256	1263	1271	rBV4	936	1630	0.13%	0.017%
26	5.435	1285	1289	1293	rVB	394	314	0.03%	0.003%
27	5.486	1302	1305	1309	rVB	466	292	0.02%	0.003%
28	5.541	1320	1322	1325	rVV	350	207	0.02%	0.002%
29	5.695	1348	1370	1421	rBV2	420485	1240245	100.00%	13.057%
30	5.962	1451	1453	1455	rVB	712	320	0.03%	0.003%
31	5.981	1455	1459	1462	rBV3	289	263	0.02%	0.003%
32	6.065	1482	1485	1489	rVB2	346	294	0.02%	0.003%
33	6.177	1515	1520	1522	rBV3	402	386	0.03%	0.004%
34	6.219	1522	1533	1567	rBV	367582	754524	60.84%	7.944%
35	6.512	1614	1624	1643	rVB8	5905	13223	1.07%	0.139%
36	6.660	1657	1670	1703	rBV	255710	535406	43.17%	5.637%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
 Data File : VU063758.D
 Acq On : 21 Nov 2025 10:30
 Operator : MD/SY
 Sample : Q3688-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 TBGW-20251119

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

37	6.917	1746	1750	1751	rBV3	463	293	0.02%	0.003%
38	7.058	1790	1794	1800	rBV2	306	275	0.02%	0.003%
39	7.184	1828	1833	1836	rBV3	363	307	0.02%	0.003%
40	7.206	1836	1840	1842	rBV2	335	254	0.02%	0.003%
41	7.344	1878	1883	1886	rVB	309	292	0.02%	0.003%
42	7.383	1890	1895	1898	rVV2	216	207	0.02%	0.002%
43	7.541	1932	1944	1963	rBV	122038	227428	18.34%	2.394%
44	7.788	2016	2021	2024	rBV3	799	778	0.06%	0.008%
45	7.872	2034	2047	2073	rBV	535887	1001516	80.75%	10.544%
46	8.155	2124	2135	2159	rBV	76679	139555	11.25%	1.469%
47	8.405	2211	2213	2219	rVB	259	201	0.02%	0.002%
48	8.528	2246	2251	2261	rBV5	1226	1680	0.14%	0.018%
49	8.614	2267	2278	2327	rBV2	200258	543332	43.81%	5.720%
50	8.840	2346	2348	2351	rBV2	341	229	0.02%	0.002%
51	8.936	2375	2378	2380	rBV3	554	408	0.03%	0.004%
52	8.965	2385	2387	2390	rVV3	427	287	0.02%	0.003%
53	9.032	2402	2408	2413	rVB	466	595	0.05%	0.006%
54	9.094	2422	2427	2428	rBV2	224	211	0.02%	0.002%
55	9.142	2436	2442	2444	rBV3	693	672	0.05%	0.007%
56	9.219	2462	2466	2469	rVV	266	218	0.02%	0.002%
57	9.251	2473	2476	2480	rBV2	370	310	0.02%	0.003%
58	9.393	2502	2520	2561	rBV	524020	968104	78.06%	10.192%
59	9.663	2598	2604	2605	rBV	1009	670	0.05%	0.007%
60	9.759	2630	2634	2637	rBV2	250	199	0.02%	0.002%
61	9.811	2648	2650	2657	rVB2	393	289	0.02%	0.003%
62	9.846	2657	2661	2664	rBV2	264	209	0.02%	0.002%
63	9.926	2682	2686	2688	rBV	289	231	0.02%	0.002%
64	10.077	2728	2733	2734	rBV2	885	617	0.05%	0.006%
65	10.415	2835	2838	2842	rVB2	297	245	0.02%	0.003%
66	10.463	2846	2853	2858	rBV2	1554	1565	0.13%	0.016%
67	10.618	2896	2901	2904	rBV3	1151	1139	0.09%	0.012%
68	10.685	2918	2922	2923	rBV2	440	263	0.02%	0.003%
69	10.730	2923	2936	2954	rBV	360989	601642	48.51%	6.334%
70	11.032	3025	3030	3032	rBV	378	305	0.02%	0.003%
71	11.065	3035	3040	3049	rVV3	1181	1849	0.15%	0.019%
72	11.129	3054	3060	3063	rBV2	234	276	0.02%	0.003%
73	11.257	3096	3100	3106	rBV	330	425	0.03%	0.004%
74	11.335	3121	3124	3127	rBV2	269	262	0.02%	0.003%
75	11.380	3132	3138	3140	rBV	376	347	0.03%	0.004%
76	11.454	3154	3161	3169	rVB2	1486	2170	0.17%	0.023%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
 Data File : VU063758.D
 Acq On : 21 Nov 2025 10:30
 Operator : MD/SY
 Sample : Q3688-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 TBGW-20251119

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

77	11.618	3209	3212	3215	rVB2	409	253	0.02%	0.003%
78	11.724	3239	3245	3252	rBV4	2830	3944	0.32%	0.042%
79	11.788	3252	3265	3290	rBV	544605	921967	74.34%	9.706%
80	11.981	3323	3325	3330	rVB2	441	332	0.03%	0.003%
81	12.052	3344	3347	3351	rVV	461	303	0.02%	0.003%
82	12.109	3361	3365	3370	rVB3	730	519	0.04%	0.005%
83	12.167	3370	3383	3406	rBV	507502	861057	69.43%	9.065%
84	12.383	3447	3450	3456	rVB3	299	297	0.02%	0.003%
85	12.434	3464	3466	3468	rBV	462	245	0.02%	0.003%
86	12.534	3495	3497	3504	rVB3	378	390	0.03%	0.004%
87	12.569	3504	3508	3510	rBV	379	266	0.02%	0.003%
88	12.634	3525	3528	3530	rBV2	337	249	0.02%	0.003%
89	13.058	3657	3660	3663	rBV2	304	272	0.02%	0.003%
90	13.203	3699	3705	3711	rBV3	2446	3128	0.25%	0.033%
91	13.788	3884	3887	3890	rBV2	388	283	0.02%	0.003%
92	13.823	3891	3898	3907	rVV3	3837	5595	0.45%	0.059%
93	13.942	3933	3935	3939	rBV3	337	258	0.02%	0.003%
94	14.000	3951	3953	3956	rBV	433	269	0.02%	0.003%
95	14.074	3968	3976	3995	rBV2	4668	9214	0.74%	0.097%
96	14.306	4043	4048	4049	rBV3	3170	2523	0.20%	0.027%
97	14.476	4096	4101	4107	rBV3	396	508	0.04%	0.005%
98	14.862	4217	4221	4223	rBV	621	444	0.04%	0.005%
99	15.270	4346	4348	4352	rBV3	571	299	0.02%	0.003%
100	15.508	4418	4422	4424	rBV3	1085	859	0.07%	0.009%




Sum of corrected areas: 9498504

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
Data File : VU063758.D
Acq On : 21 Nov 2025 10:30
Operator : MD/SY
Sample : Q3688-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TBGW-20251119

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

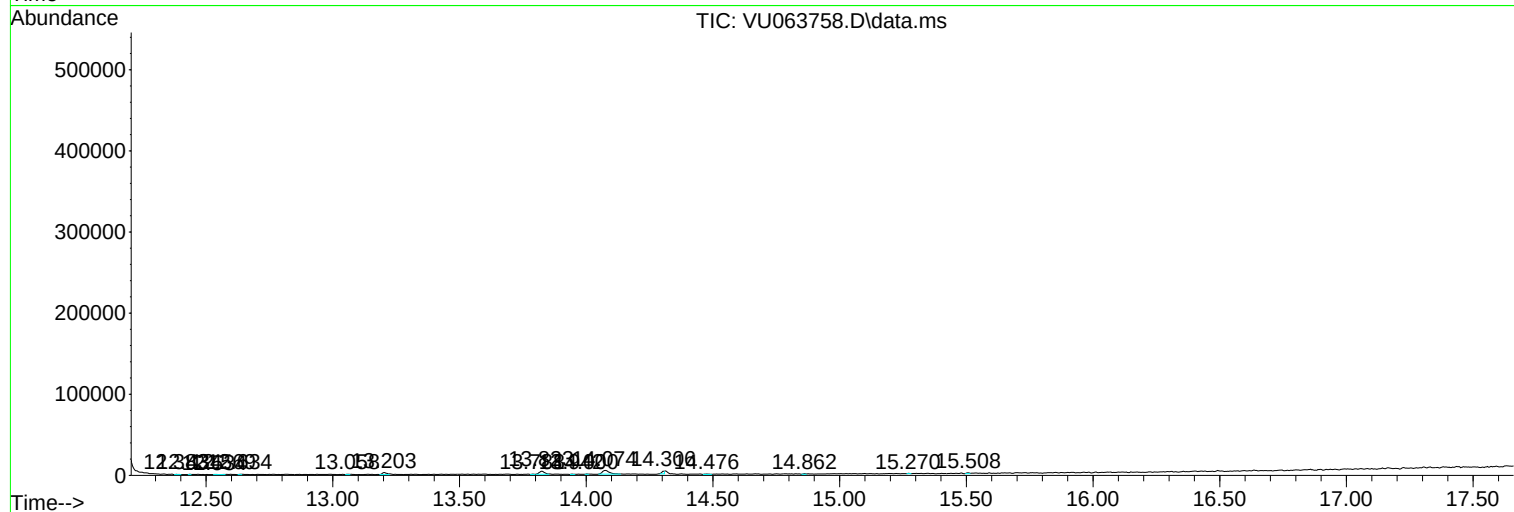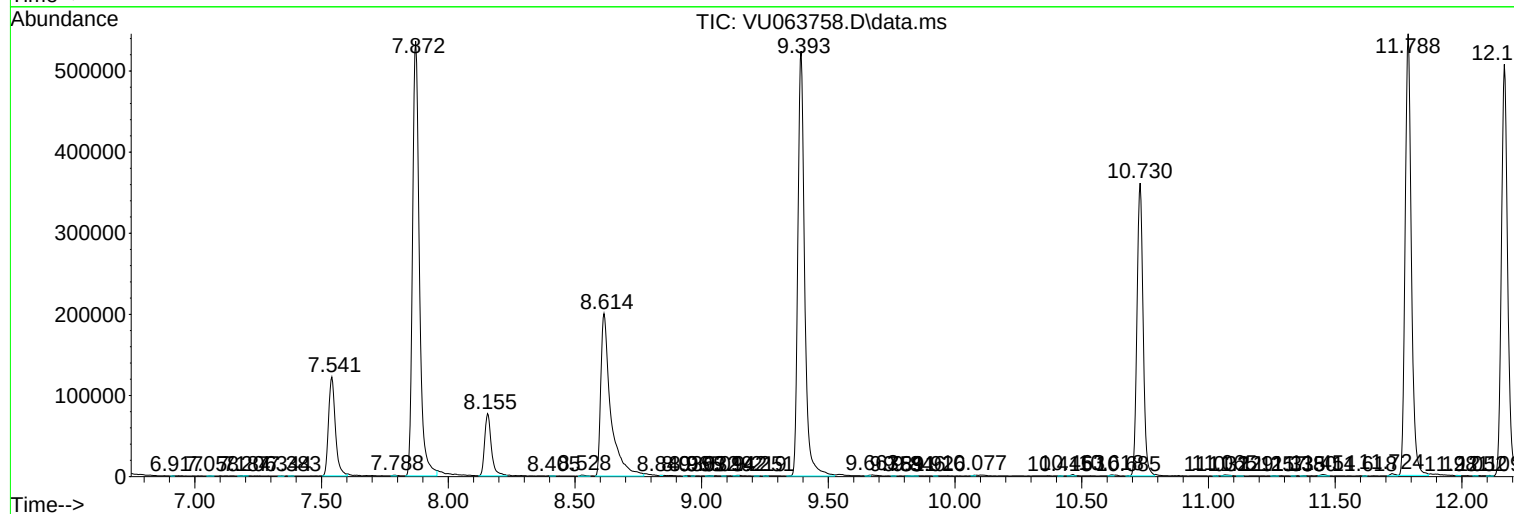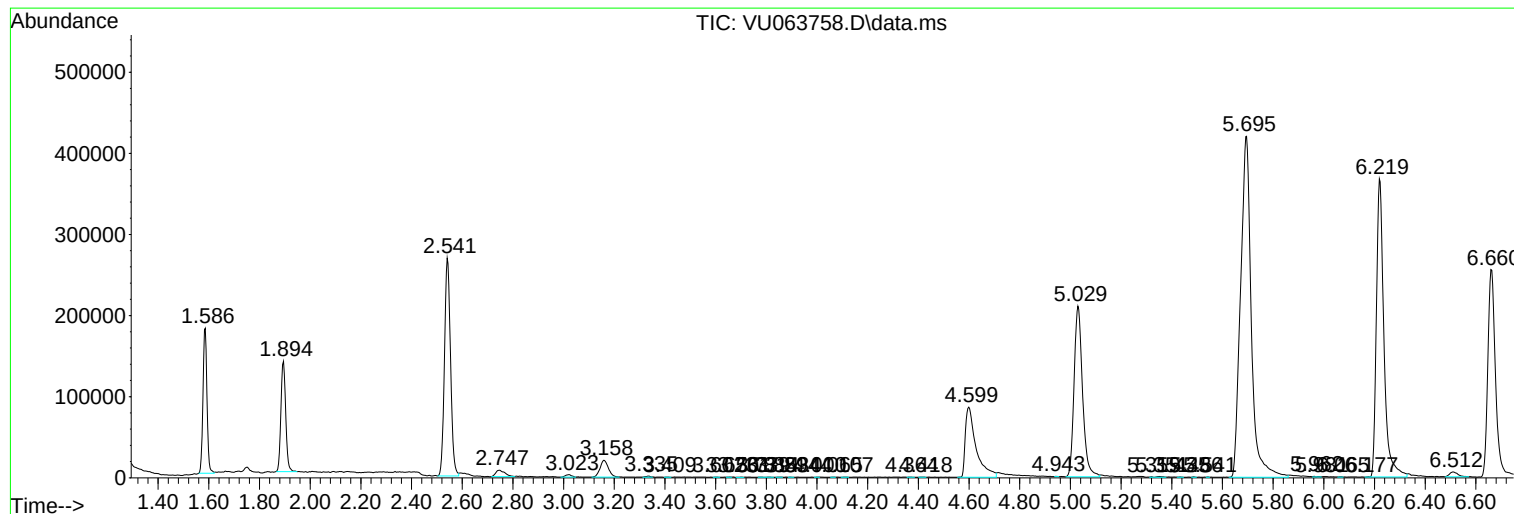

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
Data File : VU063758.D
Acq On : 21 Nov 2025 10:30
Operator : MD/SY
Sample : Q3688-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TBGW-20251119

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
Data File : VU063758.D
Acq On : 21 Nov 2025 10:30
Operator : MD/SY
Sample : Q3688-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TBGW-20251119

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc