

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
 Data File : VU063761.D
 Acq On : 21 Nov 2025 11:42
 Operator : MD/SY
 Sample : Q3688-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 TBGW-20251120

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

Signal : TIC: VU063761.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.583	84	91	104	rBV	197210	214564	15.64%	2.098%
2	1.891	179	187	199	rBV	148820	193413	14.10%	1.891%
3	2.541	377	389	407	rBV	295632	489092	35.65%	4.783%
4	2.750	442	454	467	rBV4	4731	12483	0.91%	0.122%
5	2.814	471	474	478	rVB2	596	456	0.03%	0.004%
6	2.927	507	509	516	rVB3	560	435	0.03%	0.004%
7	2.959	516	519	525	rBV2	417	438	0.03%	0.004%
8	3.020	530	538	549	rVV7	2940	5061	0.37%	0.049%
9	3.113	563	567	568	rBV	394	258	0.02%	0.003%
10	3.158	568	581	597	rVB	9682	21681	1.58%	0.212%
11	3.290	617	622	623	rBV2	270	244	0.02%	0.002%
12	3.332	631	635	637	rBV	755	579	0.04%	0.006%
13	3.438	664	668	673	rVV3	261	289	0.02%	0.003%
14	3.570	704	709	713	rVB2	347	296	0.02%	0.003%
15	3.727	754	758	765	rVB2	327	392	0.03%	0.004%
16	3.792	775	778	786	rVB2	354	441	0.03%	0.004%
17	3.830	786	790	792	rBV	348	252	0.02%	0.002%
18	3.930	817	821	824	rBV2	353	327	0.02%	0.003%
19	4.235	909	916	920	rVB2	373	400	0.03%	0.004%
20	4.264	920	925	931	rBV2	296	404	0.03%	0.004%
21	4.338	944	948	954	rBV2	344	347	0.03%	0.003%
22	4.377	954	960	963	rBV	399	398	0.03%	0.004%
23	4.534	1007	1009	1016	rVB2	361	298	0.02%	0.003%
24	4.595	1016	1028	1070	rBV	91568	271874	19.82%	2.659%
25	5.030	1147	1163	1195	rBV	232792	542868	39.57%	5.309%
26	5.341	1255	1260	1264	rBV4	689	834	0.06%	0.008%
27	5.695	1347	1370	1422	rBV2	469569	1371861	100.00%	13.415%
28	6.219	1521	1533	1572	rBV	380078	789314	57.54%	7.719%
29	6.512	1612	1624	1643	rVB5	7165	15909	1.16%	0.156%
30	6.660	1656	1670	1702	rBV	286380	596429	43.48%	5.832%
31	6.837	1722	1725	1731	rVB6	648	710	0.05%	0.007%
32	7.046	1785	1790	1796	rBV2	204	333	0.02%	0.003%
33	7.110	1805	1810	1815	rBV2	291	359	0.03%	0.004%
34	7.181	1829	1832	1838	rVB4	498	473	0.03%	0.005%
35	7.213	1838	1842	1845	rBV3	468	379	0.03%	0.004%
36	7.435	1907	1911	1915	rVB2	311	255	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
 Data File : VU063761.D
 Acq On : 21 Nov 2025 11:42
 Operator : MD/SY
 Sample : Q3688-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 TBGW-20251120

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

37	7.541	1931	1944	1977	rBV2	136230	254528	18.55%	2.489%
38	7.714	1993	1998	2002	rBV4	769	727	0.05%	0.007%
39	7.775	2014	2017	2020	rBV	441	283	0.02%	0.003%
40	7.798	2020	2024	2033	rVB4	677	1030	0.08%	0.010%
41	7.872	2033	2047	2077	rBV	598747	1108577	80.81%	10.841%
42	8.155	2123	2135	2156	rBV	85259	154748	11.28%	1.513%
43	8.328	2187	2189	2193	rVB3	428	246	0.02%	0.002%
44	8.483	2233	2237	2239	rBV	366	279	0.02%	0.003%
45	8.528	2245	2251	2255	rBV4	1206	1194	0.09%	0.012%
46	8.615	2263	2278	2327	rBV2	225426	591475	43.11%	5.784%
47	8.843	2346	2349	2352	rBV3	376	310	0.02%	0.003%
48	8.869	2355	2357	2361	rVB3	544	292	0.02%	0.003%
49	8.936	2375	2378	2383	rBV3	340	279	0.02%	0.003%
50	8.955	2383	2384	2390	rVB3	468	339	0.02%	0.003%
51	8.988	2390	2394	2397	rBV	303	250	0.02%	0.002%
52	9.007	2397	2400	2404	rBV4	323	260	0.02%	0.003%
53	9.090	2420	2426	2428	rBV2	478	434	0.03%	0.004%
54	9.139	2436	2441	2447	rBV4	585	717	0.05%	0.007%
55	9.206	2459	2462	2465	rBV	280	256	0.02%	0.003%
56	9.229	2467	2469	2474	rVV2	415	286	0.02%	0.003%
57	9.393	2507	2520	2544	rBV	547300	982173	71.59%	9.605%
58	9.669	2602	2606	2608	rBV2	983	670	0.05%	0.007%
59	9.730	2622	2625	2628	rBV2	393	282	0.02%	0.003%
60	9.846	2658	2661	2665	rVV2	344	250	0.02%	0.002%
61	10.081	2728	2734	2737	rBV3	931	937	0.07%	0.009%
62	10.203	2769	2772	2779	rVB2	266	310	0.02%	0.003%
63	10.235	2779	2782	2788	rVB	492	396	0.03%	0.004%
64	10.415	2833	2838	2844	rVB2	452	534	0.04%	0.005%
65	10.460	2844	2852	2854	rBV3	939	968	0.07%	0.009%
66	10.528	2870	2873	2879	rVB2	343	355	0.03%	0.003%
67	10.566	2879	2885	2888	rBV2	422	475	0.03%	0.005%
68	10.730	2924	2936	2961	rBV	393696	650177	47.39%	6.358%
69	10.881	2979	2983	2993	rVB3	751	1285	0.09%	0.013%
70	11.068	3037	3041	3044	rBV3	824	815	0.06%	0.008%
71	11.277	3099	3106	3112	rVB2	266	383	0.03%	0.004%
72	11.454	3155	3161	3169	rVB2	1082	1420	0.10%	0.014%
73	11.679	3225	3231	3235	rBV2	362	429	0.03%	0.004%
74	11.727	3240	3246	3252	rBV3	2031	2751	0.20%	0.027%
75	11.788	3252	3265	3292	rBV	571831	962993	70.20%	9.417%
76	11.971	3317	3322	3326	rBV5	335	419	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
 Data File : VU063761.D
 Acq On : 21 Nov 2025 11:42
 Operator : MD/SY
 Sample : Q3688-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 TBGW-20251120

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

77	12.032	3339	3341	3345	rVB3	452	290	0.02%	0.003%
78	12.065	3345	3351	3353	rBV3	312	342	0.02%	0.003%
79	12.168	3369	3383	3404	rBV	567401	951799	69.38%	9.308%
80	12.370	3444	3446	3451	rBV2	393	299	0.02%	0.003%
81	12.557	3501	3504	3508	rBV3	328	250	0.02%	0.002%
82	12.582	3508	3512	3517	rBV2	523	350	0.03%	0.003%
83	12.849	3592	3595	3598	rBV2	414	318	0.02%	0.003%
84	13.071	3660	3664	3670	rVB3	370	350	0.03%	0.003%
85	13.119	3675	3679	3683	rBV2	407	330	0.02%	0.003%
86	13.180	3694	3698	3700	rBV2	335	301	0.02%	0.003%
87	13.193	3700	3702	3703	rBV	550	261	0.02%	0.003%
88	13.296	3731	3734	3741	rBV3	329	460	0.03%	0.004%
89	13.402	3764	3767	3771	rVB2	428	351	0.03%	0.003%
90	13.563	3813	3817	3820	rBV3	404	335	0.02%	0.003%
91	13.827	3894	3899	3908	rVB5	2322	2893	0.21%	0.028%
92	14.084	3972	3979	3984	rVV4	2119	2772	0.20%	0.027%
93	14.309	4044	4049	4059	rVB7	2018	3100	0.23%	0.030%
94	14.499	4104	4108	4109	rBV2	428	335	0.02%	0.003%
95	14.759	4187	4189	4194	rVB3	436	275	0.02%	0.003%
96	15.055	4279	4281	4283	rBV	574	377	0.03%	0.004%
97	15.110	4295	4298	4303	rVB3	642	551	0.04%	0.005%
98	15.180	4317	4320	4321	rBV2	489	289	0.02%	0.003%
99	15.228	4333	4335	4337	rBV	442	290	0.02%	0.003%
100	15.267	4345	4347	4351	rBV2	602	545	0.04%	0.005%




Sum of corrected areas: 10226141

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
Data File : VU063761.D
Acq On : 21 Nov 2025 11:42
Operator : MD/SY
Sample : Q3688-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TBGW-20251120

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

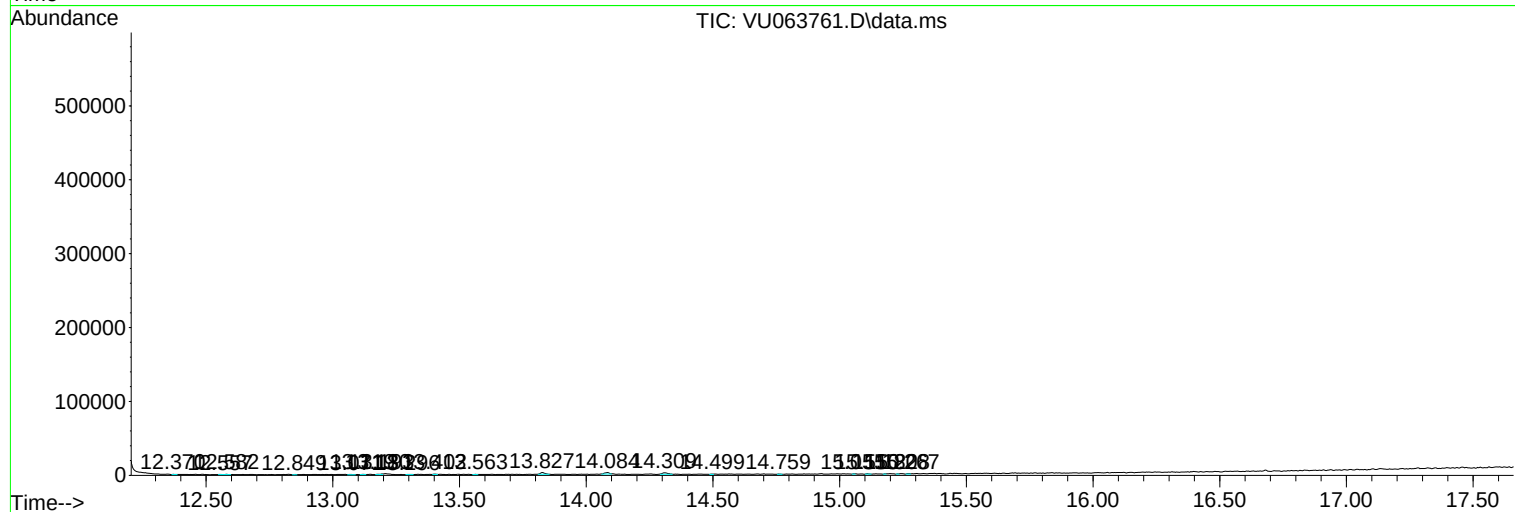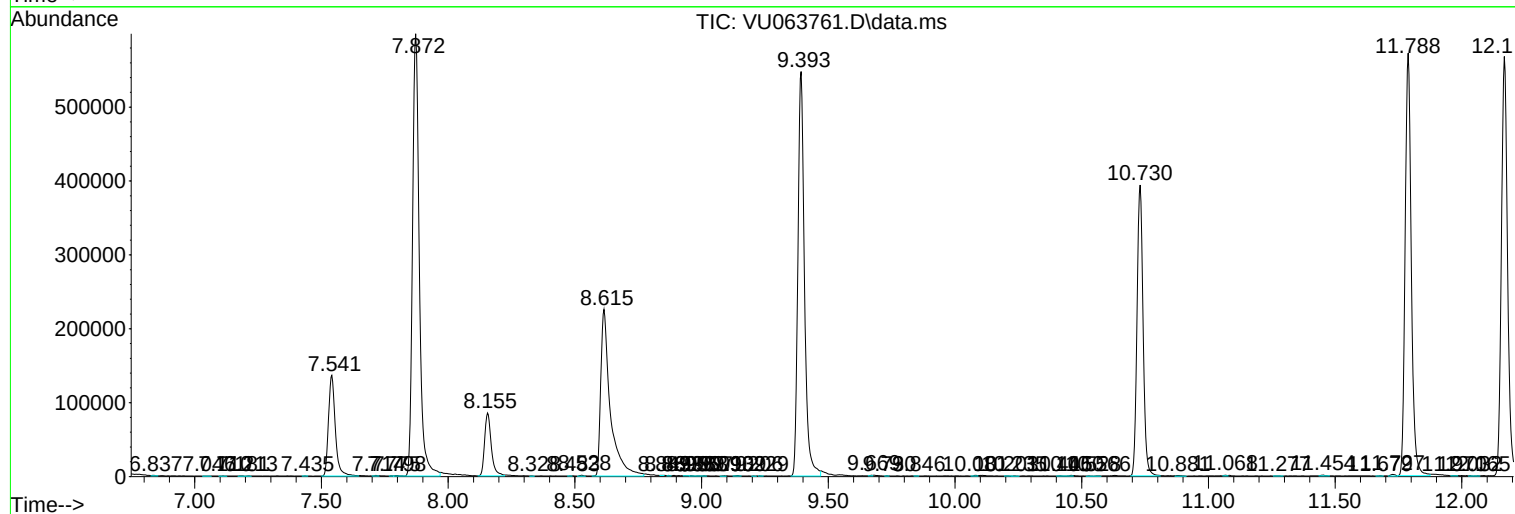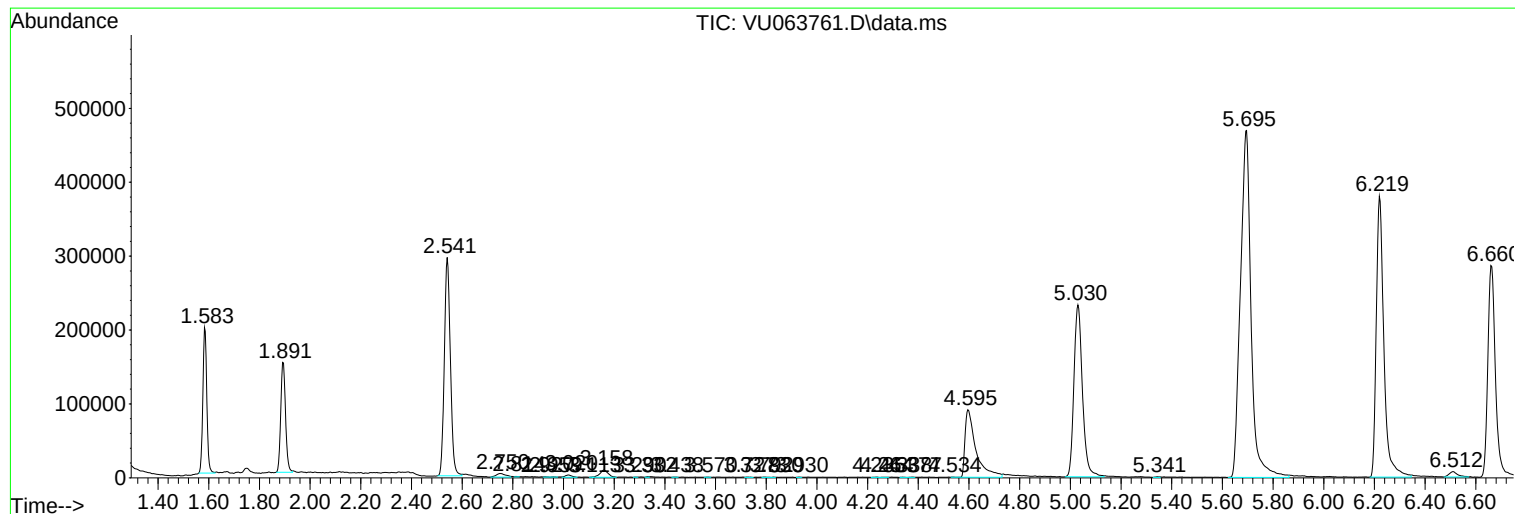

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
Data File : VU063761.D
Acq On : 21 Nov 2025 11:42
Operator : MD/SY
Sample : Q3688-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TBGW-20251120

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
Data File : VU063761.D
Acq On : 21 Nov 2025 11:42
Operator : MD/SY
Sample : Q3688-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TBGW-20251120

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc