

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
 Data File : VU063762.D
 Acq On : 21 Nov 2025 12:06
 Operator : MD/SY
 Sample : Q3688-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 FDGW-20251120

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

Signal : TIC: VU063762.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.583	84	91	105	rBV	190964	211206	15.58%	2.047%
2	1.895	179	188	201	rBV	143453	187788	13.86%	1.820%
3	2.541	378	389	407	rBV	287000	474213	34.99%	4.596%
4	2.747	443	453	468	rBV	10785	25689	1.90%	0.249%
5	2.885	492	496	501	rVV3	519	392	0.03%	0.004%
6	2.907	501	503	507	rVB2	503	253	0.02%	0.002%
7	2.985	525	527	529	rBV2	535	314	0.02%	0.003%
8	3.017	530	537	547	rVB5	2845	4835	0.36%	0.047%
9	3.158	566	581	604	rBV	26463	60757	4.48%	0.589%
10	3.329	629	634	635	rBV2	1369	1003	0.07%	0.010%
11	3.788	772	777	779	rBV2	314	231	0.02%	0.002%
12	3.814	781	785	787	rBV	411	335	0.02%	0.003%
13	3.882	801	806	808	rBV	364	341	0.03%	0.003%
14	3.972	830	834	836	rBV2	279	258	0.02%	0.003%
15	4.033	848	853	858	rVV2	196	241	0.02%	0.002%
16	4.165	892	894	899	rVB2	308	231	0.02%	0.002%
17	4.406	964	969	974	rVB	243	252	0.02%	0.002%
18	4.486	992	994	997	rVV2	310	219	0.02%	0.002%
19	4.505	997	1000	1003	rVB	351	230	0.02%	0.002%
20	4.595	1017	1028	1061	rBV2	90705	270297	19.94%	2.620%
21	5.030	1147	1163	1188	rBV	231484	531864	39.24%	5.155%
22	5.210	1216	1219	1224	rVB2	617	474	0.03%	0.005%
23	5.303	1244	1248	1251	rVB4	428	320	0.02%	0.003%
24	5.354	1261	1264	1268	rVB2	485	328	0.02%	0.003%
25	5.399	1275	1278	1283	rVB2	541	456	0.03%	0.004%
26	5.428	1283	1287	1292	rBV3	440	379	0.03%	0.004%
27	5.531	1316	1319	1324	rVB2	335	214	0.02%	0.002%
28	5.605	1336	1342	1344	rBV2	261	265	0.02%	0.003%
29	5.692	1349	1369	1417	rBV2	458120	1355364	100.00%	13.136%
30	6.026	1471	1473	1474	rBV	718	235	0.02%	0.002%
31	6.113	1497	1500	1503	rBV	261	227	0.02%	0.002%
32	6.219	1521	1533	1583	rBV	393030	821059	60.58%	7.958%
33	6.505	1613	1622	1623	rBV4	4812	5099	0.38%	0.049%
34	6.660	1656	1670	1703	rBV	283107	590518	43.57%	5.723%
35	6.837	1722	1725	1732	rVB5	1180	1203	0.09%	0.012%
36	6.869	1732	1735	1738	rVB2	446	285	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
 Data File : VU063762.D
 Acq On : 21 Nov 2025 12:06
 Operator : MD/SY
 Sample : Q3688-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 FDGW-20251120

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

37	7.081	1798	1801	1806	rVB2	501	401	0.03%	0.004%
38	7.184	1828	1833	1837	rBV4	583	522	0.04%	0.005%
39	7.306	1867	1871	1873	rBV2	397	278	0.02%	0.003%
40	7.380	1888	1894	1897	rBV2	225	251	0.02%	0.002%
41	7.480	1917	1925	1928	rBV2	480	499	0.04%	0.005%
42	7.541	1932	1944	1974	rBV	131610	248985	18.37%	2.413%
43	7.730	2001	2003	2008	rVB2	416	277	0.02%	0.003%
44	7.798	2022	2024	2030	rVB3	684	413	0.03%	0.004%
45	7.872	2034	2047	2078	rBV	584914	1103442	81.41%	10.695%
46	8.155	2124	2135	2158	rBV	81833	151698	11.19%	1.470%
47	8.322	2185	2187	2194	rVB2	323	319	0.02%	0.003%
48	8.435	2216	2222	2230	rBV2	791	1097	0.08%	0.011%
49	8.480	2230	2236	2238	rBV	406	431	0.03%	0.004%
50	8.534	2247	2253	2257	rVB3	1031	1006	0.07%	0.010%
51	8.615	2266	2278	2317	rBV2	216250	581058	42.87%	5.632%
52	8.894	2361	2365	2366	rBV2	389	263	0.02%	0.003%
53	9.023	2402	2405	2408	rVV3	347	221	0.02%	0.002%
54	9.074	2417	2421	2425	rBV3	330	391	0.03%	0.004%
55	9.097	2425	2428	2431	rVB	307	221	0.02%	0.002%
56	9.393	2507	2520	2561	rBV	572987	1040224	76.75%	10.082%
57	9.672	2603	2607	2608	rBV	774	490	0.04%	0.005%
58	9.727	2621	2624	2627	rVB2	461	312	0.02%	0.003%
59	9.746	2627	2630	2637	rVB	224	229	0.02%	0.002%
60	9.779	2637	2640	2646	rBV2	308	321	0.02%	0.003%
61	9.923	2682	2685	2694	rVB2	238	248	0.02%	0.002%
62	9.997	2700	2708	2713	rBV2	356	554	0.04%	0.005%
63	10.020	2713	2715	2722	rVB2	217	256	0.02%	0.002%
64	10.074	2728	2732	2734	rBV	667	515	0.04%	0.005%
65	10.409	2832	2836	2840	rBV2	352	347	0.03%	0.003%
66	10.463	2848	2853	2863	rVB2	856	1356	0.10%	0.013%
67	10.512	2864	2868	2871	rBV	298	277	0.02%	0.003%
68	10.624	2900	2903	2911	rVB3	768	921	0.07%	0.009%
69	10.682	2917	2921	2924	rBV2	405	263	0.02%	0.003%
70	10.730	2924	2936	2955	rBV	398187	655176	48.34%	6.350%
71	10.894	2985	2987	2994	rBV2	270	237	0.02%	0.002%
72	10.987	3012	3016	3024	rBV2	416	600	0.04%	0.006%
73	11.023	3024	3027	3031	rVV	319	216	0.02%	0.002%
74	11.071	3032	3042	3049	rVV4	1008	1637	0.12%	0.016%
75	11.193	3078	3080	3089	rVB2	446	518	0.04%	0.005%
76	11.238	3089	3094	3096	rBV	233	239	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
 Data File : VU063762.D
 Acq On : 21 Nov 2025 12:06
 Operator : MD/SY
 Sample : Q3688-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 FDGW-20251120

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

77	11.303	3112	3114	3119	rVB2	273	214	0.02%	0.002%
78	11.447	3155	3159	3162	rBV2	958	880	0.06%	0.009%
79	11.730	3240	3247	3253	rBV2	2392	2957	0.22%	0.029%
80	11.788	3253	3265	3289	rBV	595448	1007383	74.33%	9.764%
81	12.010	3332	3334	3336	rVB	530	214	0.02%	0.002%
82	12.061	3348	3350	3355	rVB3	345	263	0.02%	0.003%
83	12.097	3356	3361	3364	rBV4	607	560	0.04%	0.005%
84	12.167	3370	3383	3406	rBV	555606	947301	69.89%	9.181%
85	12.492	3481	3484	3487	rBV	293	223	0.02%	0.002%
86	12.512	3487	3490	3493	rVB2	392	227	0.02%	0.002%
87	13.061	3658	3661	3665	rVB3	552	447	0.03%	0.004%
88	13.119	3676	3679	3682	rVV2	269	216	0.02%	0.002%
89	13.200	3700	3704	3705	rBV2	772	554	0.04%	0.005%
90	13.508	3797	3800	3806	rBV3	399	500	0.04%	0.005%
91	13.627	3834	3837	3842	rVB2	434	334	0.02%	0.003%
92	13.740	3870	3872	3875	rBV2	492	326	0.02%	0.003%
93	13.827	3893	3899	3904	rBV7	1737	2491	0.18%	0.024%
94	13.894	3917	3920	3925	rBV2	588	598	0.04%	0.006%
95	14.081	3972	3978	3980	rBV5	1397	1270	0.09%	0.012%
96	14.309	4043	4049	4060	rVB4	1793	3019	0.22%	0.029%
97	15.032	4269	4274	4276	rBV4	821	754	0.06%	0.007%
98	15.222	4329	4333	4336	rBV3	925	813	0.06%	0.008%
99	15.293	4353	4355	4365	rVB3	1004	1045	0.08%	0.010%
100	15.338	4365	4369	4373	rBV4	958	874	0.06%	0.008%




Sum of corrected areas: 10317547

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
Data File : VU063762.D
Acq On : 21 Nov 2025 12:06
Operator : MD/SY
Sample : Q3688-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
FDGW-20251120

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

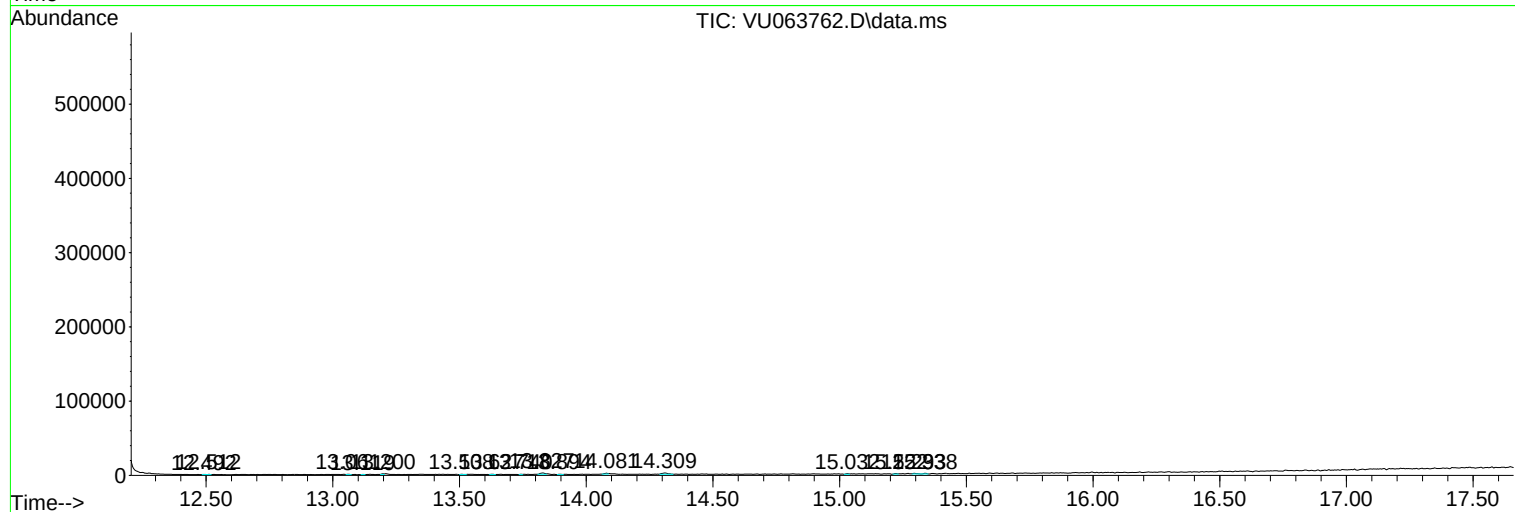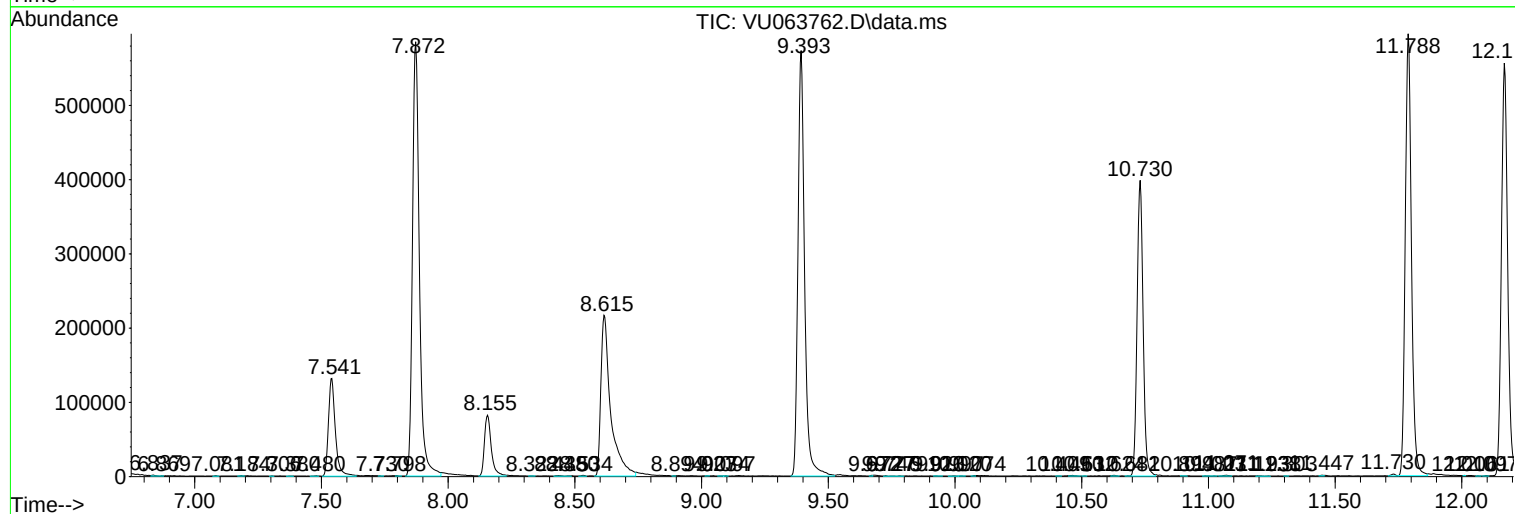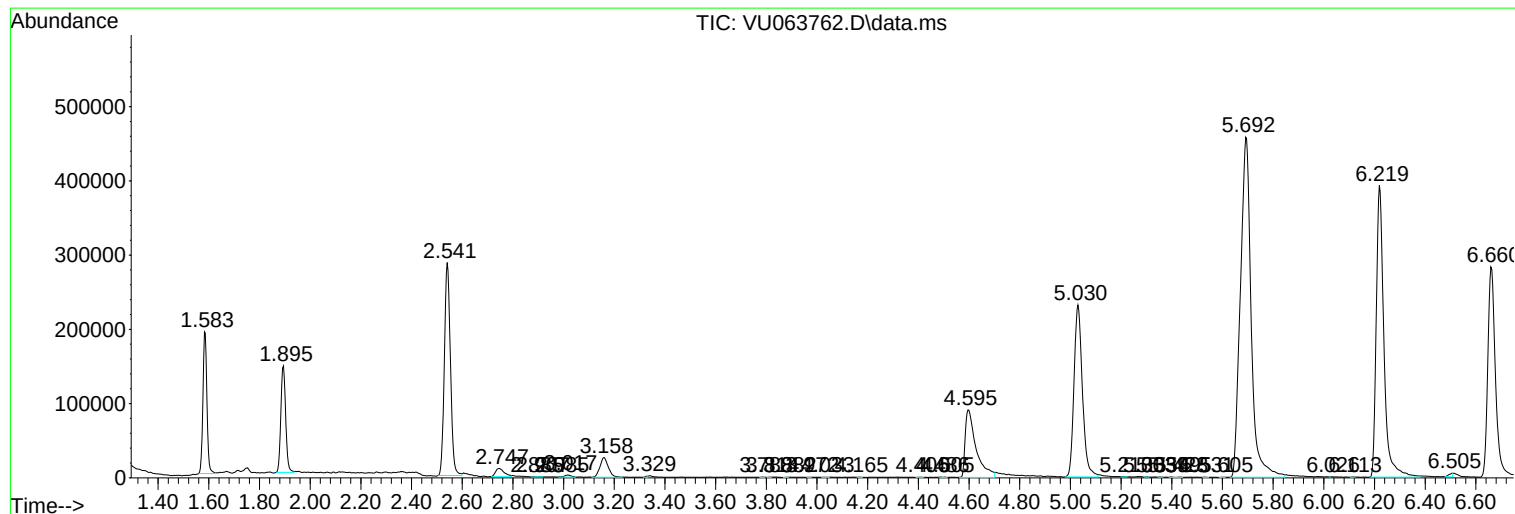

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
Data File : VU063762.D
Acq On : 21 Nov 2025 12:06
Operator : MD/SY
Sample : Q3688-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
FDGW-20251120

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
Data File : VU063762.D
Acq On : 21 Nov 2025 12:06
Operator : MD/SY
Sample : Q3688-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
FDGW-20251120

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------