

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
 Data File : VU063763.D
 Acq On : 21 Nov 2025 12:31
 Operator : MD/SY
 Sample : Q3688-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 M-31S

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M

Title : VOC Analysis

Signal : TIC: VU063763.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.586	84	92	106	rBV	200914	216456	15.76%	2.059%
2	1.894	179	188	200	rBV	145650	189934	13.83%	1.807%
3	2.541	377	389	406	rBV	292211	484482	35.28%	4.609%
4	2.746	444	453	471	rBV2	6704	15708	1.14%	0.149%
5	3.017	530	537	549	rVB4	2909	5617	0.41%	0.053%
6	3.107	560	565	567	rBV2	322	272	0.02%	0.003%
7	3.158	567	581	602	rBV2	14514	33544	2.44%	0.319%
8	3.258	607	612	613	rBV	302	242	0.02%	0.002%
9	3.290	617	622	626	rVB2	313	294	0.02%	0.003%
10	3.328	631	634	635	rBV2	802	514	0.04%	0.005%
11	3.637	725	730	734	rBV2	219	245	0.02%	0.002%
12	3.840	788	793	796	rBV2	449	400	0.03%	0.004%
13	3.984	834	838	841	rBV	299	238	0.02%	0.002%
14	4.029	848	852	855	rBV2	232	229	0.02%	0.002%
15	4.087	867	870	874	rBV2	255	296	0.02%	0.003%
16	4.152	884	890	896	rBV2	288	375	0.03%	0.004%
17	4.184	896	900	907	rBV	281	319	0.02%	0.003%
18	4.254	918	922	926	rBV2	318	259	0.02%	0.002%
19	4.370	953	958	963	rBV2	184	227	0.02%	0.002%
20	4.418	970	973	978	rVB2	305	274	0.02%	0.003%
21	4.460	978	986	992	rBV	275	417	0.03%	0.004%
22	4.499	995	998	1004	rVB2	262	233	0.02%	0.002%
23	4.598	1018	1029	1061	rBV2	90239	264332	19.25%	2.515%
24	4.955	1137	1140	1144	rVB2	643	440	0.03%	0.004%
25	5.029	1146	1163	1202	rVV	235152	551174	40.14%	5.243%
26	5.261	1232	1235	1237	rBV	421	237	0.02%	0.002%
27	5.360	1264	1266	1276	rVB4	939	1010	0.07%	0.010%
28	5.473	1296	1301	1303	rBV2	341	258	0.02%	0.002%
29	5.695	1348	1370	1410	rBV2	472073	1373156	100.00%	13.062%
30	6.058	1481	1483	1488	rVB3	446	311	0.02%	0.003%
31	6.081	1488	1490	1495	rBV3	284	242	0.02%	0.002%
32	6.164	1514	1516	1521	rVB	349	299	0.02%	0.003%
33	6.219	1521	1533	1568	rBV	406999	850319	61.92%	8.089%
34	6.508	1613	1623	1641	rVB5	6899	16275	1.19%	0.155%
35	6.659	1655	1670	1704	rBV	286567	604079	43.99%	5.746%
36	6.901	1742	1745	1748	rVB	538	396	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
 Data File : VU063763.D
 Acq On : 21 Nov 2025 12:31
 Operator : MD/SY
 Sample : Q3688-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 M-31S

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

37	6.971	1763	1767	1770	rBV2	457	412	0.03%	0.004%
38	7.110	1807	1810	1812	rBV	368	221	0.02%	0.002%
39	7.254	1849	1855	1856	rBV2	293	255	0.02%	0.002%
40	7.280	1860	1863	1868	rVB	337	255	0.02%	0.002%
41	7.315	1868	1874	1878	rBV2	364	344	0.03%	0.003%
42	7.354	1882	1886	1888	rBV	398	288	0.02%	0.003%
43	7.473	1919	1923	1928	rBV	338	353	0.03%	0.003%
44	7.540	1932	1944	1970	rBV	133389	254149	18.51%	2.418%
45	7.733	2002	2004	2008	rVB2	559	352	0.03%	0.003%
46	7.762	2008	2013	2015	rBV3	334	221	0.02%	0.002%
47	7.782	2015	2019	2021	rBV2	335	223	0.02%	0.002%
48	7.872	2034	2047	2079	rBV	605785	1118265	81.44%	10.638%
49	8.155	2125	2135	2164	rBV2	82891	153570	11.18%	1.461%
50	8.531	2244	2252	2263	rVB6	4192	6270	0.46%	0.060%
51	8.614	2266	2278	2320	rBV3	221892	586999	42.75%	5.584%
52	8.827	2342	2344	2349	rVB4	836	628	0.05%	0.006%
53	8.856	2349	2353	2361	rVB4	895	1035	0.08%	0.010%
54	8.897	2362	2366	2367	rBV2	296	236	0.02%	0.002%
55	9.116	2429	2434	2437	rVB2	303	232	0.02%	0.002%
56	9.142	2437	2442	2445	rBV3	792	826	0.06%	0.008%
57	9.257	2474	2478	2481	rBV	314	296	0.02%	0.003%
58	9.392	2508	2520	2563	rBV	602148	1086771	79.14%	10.338%
59	9.621	2588	2591	2593	rBV3	458	270	0.02%	0.003%
60	9.675	2602	2608	2610	rBV2	951	962	0.07%	0.009%
61	9.769	2631	2637	2638	rBV	304	261	0.02%	0.002%
62	9.798	2642	2646	2648	rVV2	289	276	0.02%	0.003%
63	10.036	2715	2720	2725	rBV2	444	353	0.03%	0.003%
64	10.081	2726	2734	2735	rBV2	879	759	0.06%	0.007%
65	10.203	2769	2772	2775	rBV2	291	246	0.02%	0.002%
66	10.283	2793	2797	2801	rBV2	305	236	0.02%	0.002%
67	10.444	2840	2847	2848	rBV	237	235	0.02%	0.002%
68	10.460	2848	2852	2854	rBV4	677	467	0.03%	0.004%
69	10.624	2898	2903	2911	rVB5	914	1166	0.08%	0.011%
70	10.730	2923	2936	2957	rBV	393257	659886	48.06%	6.277%
71	10.888	2983	2985	2990	rVB3	723	395	0.03%	0.004%
72	10.917	2990	2994	2998	rBV3	413	412	0.03%	0.004%
73	11.068	3035	3041	3046	rBV2	832	1142	0.08%	0.011%
74	11.164	3067	3071	3076	rBV	346	349	0.03%	0.003%
75	11.280	3103	3107	3112	rVB2	312	295	0.02%	0.003%
76	11.309	3112	3116	3118	rBV	253	228	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
 Data File : VU063763.D
 Acq On : 21 Nov 2025 12:31
 Operator : MD/SY
 Sample : Q3688-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 M-31S

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

77	11.360	3130	3132	3135	rBV2	387	247	0.02%	0.002%
78	11.453	3156	3161	3168	rVB2	1010	1347	0.10%	0.013%
79	11.730	3239	3247	3252	rBV6	1830	2382	0.17%	0.023%
80	11.788	3252	3265	3293	rBV	618062	1045729	76.16%	9.948%
81	12.087	3356	3358	3363	rVB3	348	258	0.02%	0.002%
82	12.167	3363	3383	3408	rBV	561373	958495	69.80%	9.118%
83	12.357	3439	3442	3445	rBV2	611	342	0.02%	0.003%
84	12.418	3455	3461	3467	rBV2	644	936	0.07%	0.009%
85	12.450	3467	3471	3474	rBV3	493	390	0.03%	0.004%
86	12.781	3571	3574	3577	rBV2	390	267	0.02%	0.003%
87	12.807	3578	3582	3587	rBV	540	587	0.04%	0.006%
88	12.855	3592	3597	3599	rBV2	411	385	0.03%	0.004%
89	12.981	3633	3636	3640	rVB3	528	430	0.03%	0.004%
90	13.138	3679	3685	3686	rBV	525	433	0.03%	0.004%
91	13.325	3740	3743	3746	rBV2	427	351	0.03%	0.003%
92	13.367	3753	3756	3759	rBV	338	255	0.02%	0.002%
93	13.408	3766	3769	3775	rBV3	452	530	0.04%	0.005%
94	13.498	3794	3797	3800	rBV2	410	323	0.02%	0.003%
95	13.592	3821	3826	3829	rBV3	446	396	0.03%	0.004%
96	13.826	3894	3899	3901	rBV4	1260	1127	0.08%	0.011%
97	14.215	4017	4020	4024	rBV2	307	235	0.02%	0.002%
98	14.315	4043	4051	4055	rBV4	1654	2220	0.16%	0.021%
99	15.084	4286	4290	4293	rBV3	684	617	0.04%	0.006%
100	15.447	4400	4403	4406	rBV3	880	686	0.05%	0.007%


Sum of corrected areas: 10512210

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
Data File : VU063763.D
Acq On : 21 Nov 2025 12:31
Operator : MD/SY
Sample : Q3688-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
M-31S

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

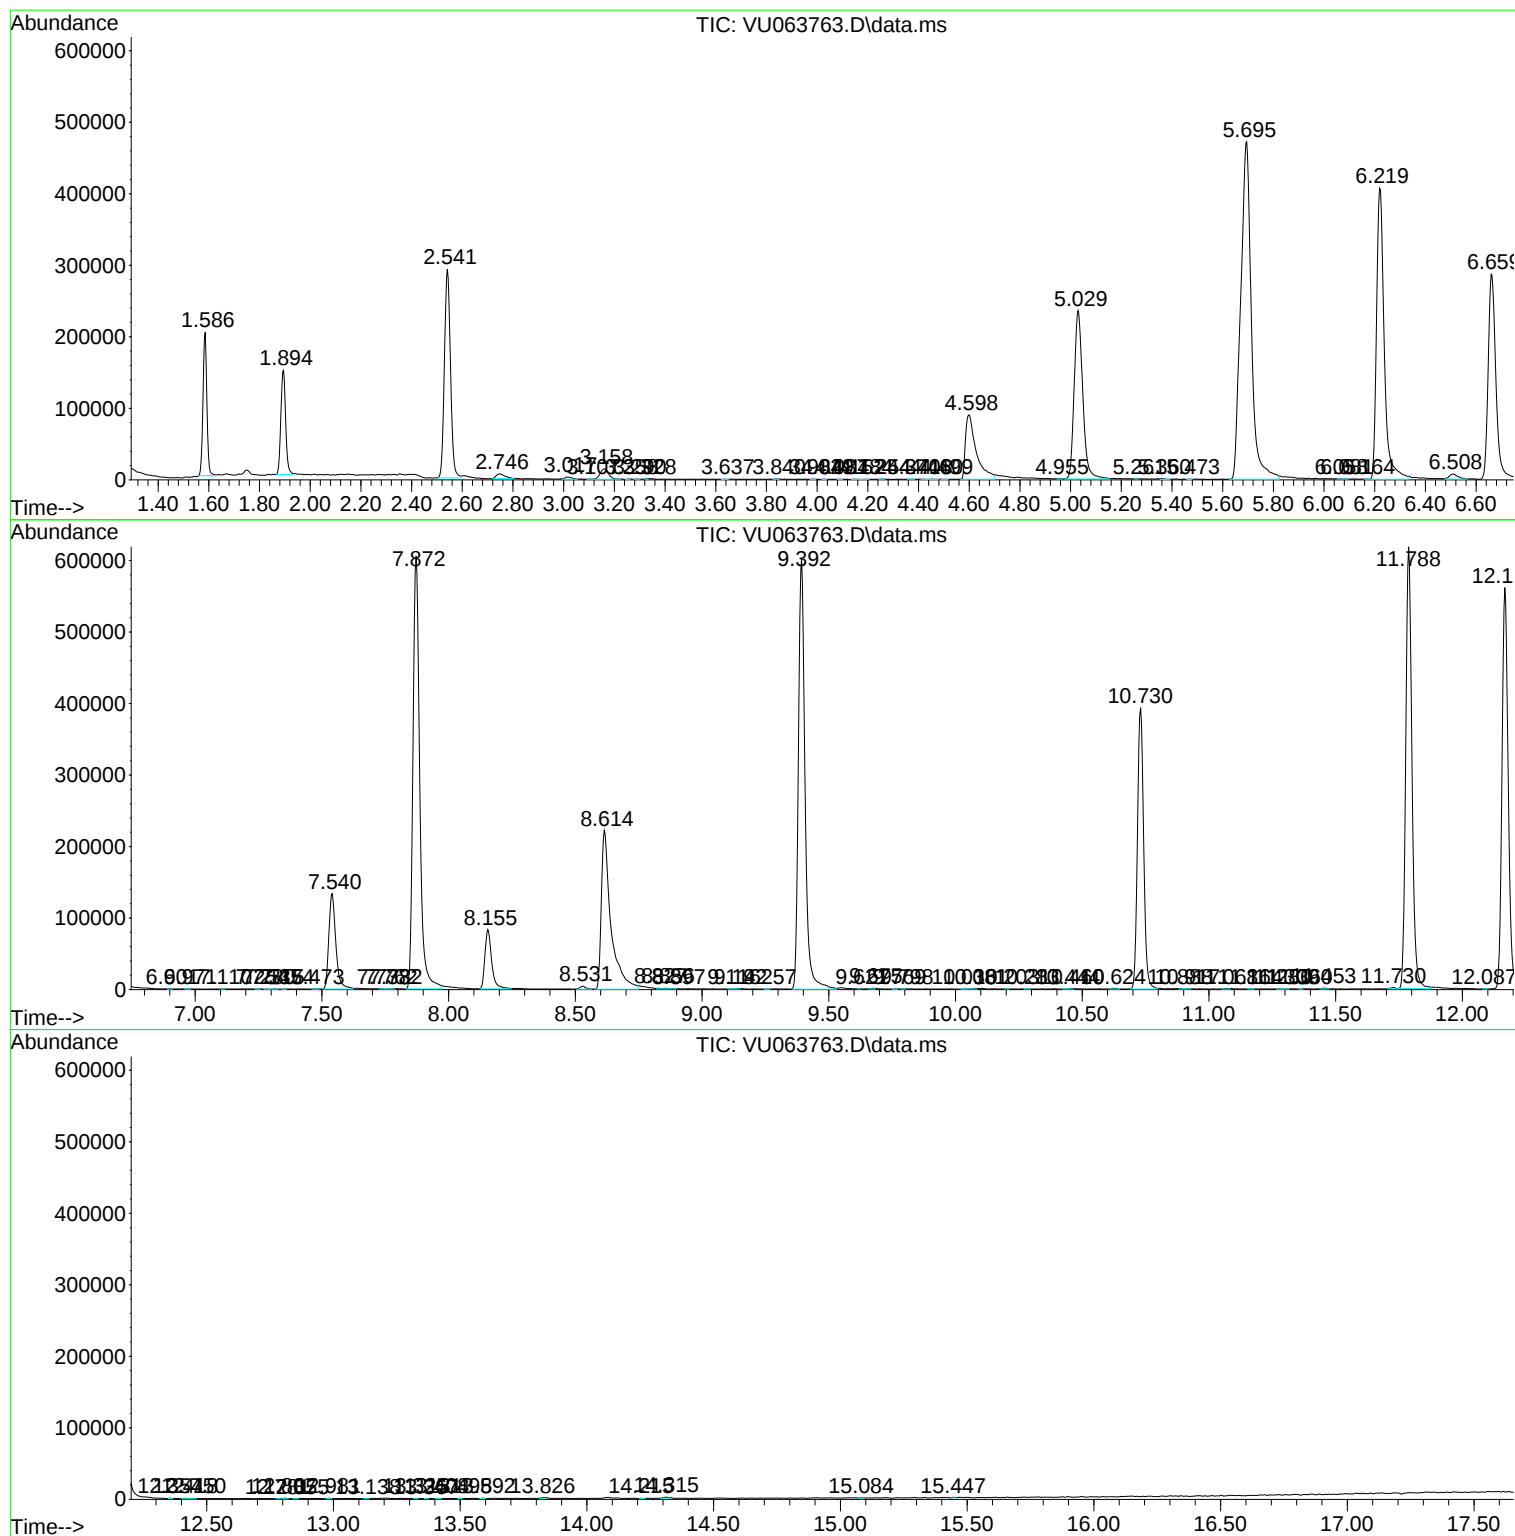

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
Data File : VU063763.D
Acq On : 21 Nov 2025 12:31
Operator : MD/SY
Sample : Q3688-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
M-31S

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
Data File : VU063763.D
Acq On : 21 Nov 2025 12:31
Operator : MD/SY
Sample : Q3688-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
M-31S

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc