

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
 Data File : VU063765.D
 Acq On : 21 Nov 2025 13:20
 Operator : MD/SY
 Sample : Q3688-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 M-32S

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

Signal : TIC: VU063765.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.583	84	91	105	rBV	192412	213292	15.60%	2.049%
2	1.894	179	188	203	rBV	145196	190208	13.91%	1.827%
3	2.541	377	389	406	rBV	287945	474913	34.74%	4.562%
4	2.743	442	452	477	rBV	15684	40472	2.96%	0.389%
5	2.904	497	502	506	rBV3	591	776	0.06%	0.007%
6	2.946	512	515	520	rVB2	599	441	0.03%	0.004%
7	3.020	529	538	545	rBV6	2573	4335	0.32%	0.042%
8	3.081	553	557	563	rVB4	311	420	0.03%	0.004%
9	3.161	563	582	602	rBV	33950	81282	5.95%	0.781%
10	3.261	608	613	615	rBV2	389	398	0.03%	0.004%
11	3.332	631	635	638	rBV2	377	439	0.03%	0.004%
12	3.383	647	651	655	rBV	404	333	0.02%	0.003%
13	3.422	660	663	667	rVB3	463	338	0.02%	0.003%
14	3.454	667	673	676	rBV2	279	302	0.02%	0.003%
15	3.605	717	720	725	rBV2	225	270	0.02%	0.003%
16	4.136	882	885	887	rBV	367	269	0.02%	0.003%
17	4.226	909	913	918	rBV2	412	482	0.04%	0.005%
18	4.293	929	934	937	rBV2	338	315	0.02%	0.003%
19	4.521	1002	1005	1008	rVB	365	258	0.02%	0.002%
20	4.544	1008	1012	1017	rBV2	323	294	0.02%	0.003%
21	4.599	1017	1029	1059	rBV	93342	276452	20.22%	2.656%
22	5.029	1148	1163	1201	rBV	232872	537495	39.32%	5.163%
23	5.261	1231	1235	1236	rBV2	599	406	0.03%	0.004%
24	5.383	1271	1273	1281	rVB2	347	334	0.02%	0.003%
25	5.447	1289	1293	1297	rVV2	416	316	0.02%	0.003%
26	5.611	1341	1344	1346	rBV	499	309	0.02%	0.003%
27	5.695	1346	1370	1415	rBV2	465820	1367073	100.00%	13.132%
28	5.968	1452	1455	1459	rVB3	695	522	0.04%	0.005%
29	6.007	1465	1467	1476	rVB3	845	747	0.05%	0.007%
30	6.219	1521	1533	1571	rBV	385106	811368	59.35%	7.794%
31	6.508	1612	1623	1639	rBV6	5910	12892	0.94%	0.124%
32	6.660	1657	1670	1699	rBV	281617	591352	43.26%	5.680%
33	6.894	1740	1743	1745	rBV	449	275	0.02%	0.003%
34	6.971	1764	1767	1772	rVB2	621	451	0.03%	0.004%
35	6.997	1772	1775	1780	rBV	269	304	0.02%	0.003%
36	7.084	1794	1802	1807	rVV2	354	348	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
 Data File : VU063765.D
 Acq On : 21 Nov 2025 13:20
 Operator : MD/SY
 Sample : Q3688-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 M-32S

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

37	7.197	1832	1837	1842	rVB3	374	370	0.03%	0.004%
38	7.264	1855	1858	1864	rVB2	247	291	0.02%	0.003%
39	7.438	1908	1912	1919	rVB	376	369	0.03%	0.004%
40	7.541	1932	1944	1973	rVV	130873	250159	18.30%	2.403%
41	7.679	1985	1987	1993	rVB4	504	457	0.03%	0.004%
42	7.737	2001	2005	2008	rBV3	516	409	0.03%	0.004%
43	7.872	2030	2047	2087	rBV	591762	1115241	81.58%	10.713%
44	8.155	2124	2135	2154	rBV	81143	147971	10.82%	1.421%
45	8.338	2188	2192	2195	rBV	385	371	0.03%	0.004%
46	8.357	2195	2198	2203	rVB2	516	355	0.03%	0.003%
47	8.438	2217	2223	2226	rBV2	283	350	0.03%	0.003%
48	8.531	2244	2252	2259	rVB4	838	1074	0.08%	0.010%
49	8.566	2259	2263	2265	rBV	401	285	0.02%	0.003%
50	8.614	2267	2278	2314	rBV2	225125	585223	42.81%	5.621%
51	8.840	2346	2348	2351	rVB2	555	258	0.02%	0.002%
52	8.926	2373	2375	2379	rVB	450	287	0.02%	0.003%
53	9.158	2437	2447	2452	rVB5	603	919	0.07%	0.009%
54	9.393	2507	2520	2562	rBV	579321	1045122	76.45%	10.039%
55	9.544	2565	2567	2571	rBV3	618	390	0.03%	0.004%
56	9.682	2602	2610	2611	rBV3	768	948	0.07%	0.009%
57	9.749	2629	2631	2636	rVB3	392	304	0.02%	0.003%
58	9.788	2636	2643	2645	rBV	328	313	0.02%	0.003%
59	9.830	2653	2656	2663	rVB2	353	323	0.02%	0.003%
60	9.971	2694	2700	2703	rBV2	286	284	0.02%	0.003%
61	10.045	2718	2723	2725	rBV2	293	247	0.02%	0.002%
62	10.074	2725	2732	2733	rBV3	481	346	0.03%	0.003%
63	10.116	2741	2745	2749	rVB4	630	530	0.04%	0.005%
64	10.190	2762	2768	2773	rBV	184	282	0.02%	0.003%
65	10.290	2795	2799	2802	rBV	343	251	0.02%	0.002%
66	10.457	2846	2851	2862	rBV4	1147	1809	0.13%	0.017%
67	10.569	2880	2886	2888	rBV2	292	290	0.02%	0.003%
68	10.618	2898	2901	2902	rBV	561	340	0.02%	0.003%
69	10.730	2923	2936	2954	rBV	412058	666744	48.77%	6.405%
70	10.862	2973	2977	2979	rBV	498	379	0.03%	0.004%
71	10.894	2984	2987	2992	rVV3	414	375	0.03%	0.004%
72	11.061	3036	3039	3040	rBV	467	294	0.02%	0.003%
73	11.180	3072	3076	3082	rVB2	409	384	0.03%	0.004%
74	11.415	3145	3149	3152	rBV2	338	276	0.02%	0.003%
75	11.450	3154	3160	3169	rVB2	903	1330	0.10%	0.013%
76	11.573	3191	3198	3202	rBV2	292	394	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
 Data File : VU063765.D
 Acq On : 21 Nov 2025 13:20
 Operator : MD/SY
 Sample : Q3688-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 M-32S

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

77	11.659	3221	3225	3229	rVB2	308	263	0.02%	0.003%
78	11.704	3232	3239	3241	rBV2	353	375	0.03%	0.004%
79	11.733	3241	3248	3253	rBV5	1327	1670	0.12%	0.016%
80	11.788	3253	3265	3289	rBV	591695	1001671	73.27%	9.622%
81	12.167	3367	3383	3418	rVV	556809	958259	70.10%	9.205%
82	12.463	3468	3475	3477	rBV	350	390	0.03%	0.004%
83	12.531	3493	3496	3500	rVB4	421	317	0.02%	0.003%
84	12.653	3531	3534	3539	rBV2	354	323	0.02%	0.003%
85	12.849	3589	3595	3598	rBV	561	513	0.04%	0.005%
86	12.881	3598	3605	3609	rVV3	262	429	0.03%	0.004%
87	13.016	3644	3647	3651	rVB	352	287	0.02%	0.003%
88	13.042	3651	3655	3658	rBV	483	318	0.02%	0.003%
89	13.199	3699	3704	3707	rBV	608	625	0.05%	0.006%
90	13.328	3741	3744	3750	rVB	429	382	0.03%	0.004%
91	13.367	3750	3756	3763	rBV4	596	680	0.05%	0.007%
92	13.479	3788	3791	3794	rBV2	470	312	0.02%	0.003%
93	13.569	3816	3819	3824	rVB	377	279	0.02%	0.003%
94	13.627	3832	3837	3838	rBV3	400	371	0.03%	0.004%
95	13.772	3878	3882	3887	rBV3	461	389	0.03%	0.004%
96	13.826	3894	3899	3907	rBV6	1584	2171	0.16%	0.021%
97	14.000	3951	3953	3959	rVB2	587	485	0.04%	0.005%
98	14.077	3971	3977	3979	rBV3	1200	1154	0.08%	0.011%
99	14.312	4044	4050	4057	rVB3	1371	1768	0.13%	0.017%
100	14.704	4170	4172	4175	rBV3	432	280	0.02%	0.003%




Sum of corrected areas: 10410536

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
Data File : VU063765.D
Acq On : 21 Nov 2025 13:20
Operator : MD/SY
Sample : Q3688-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
M-32S

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

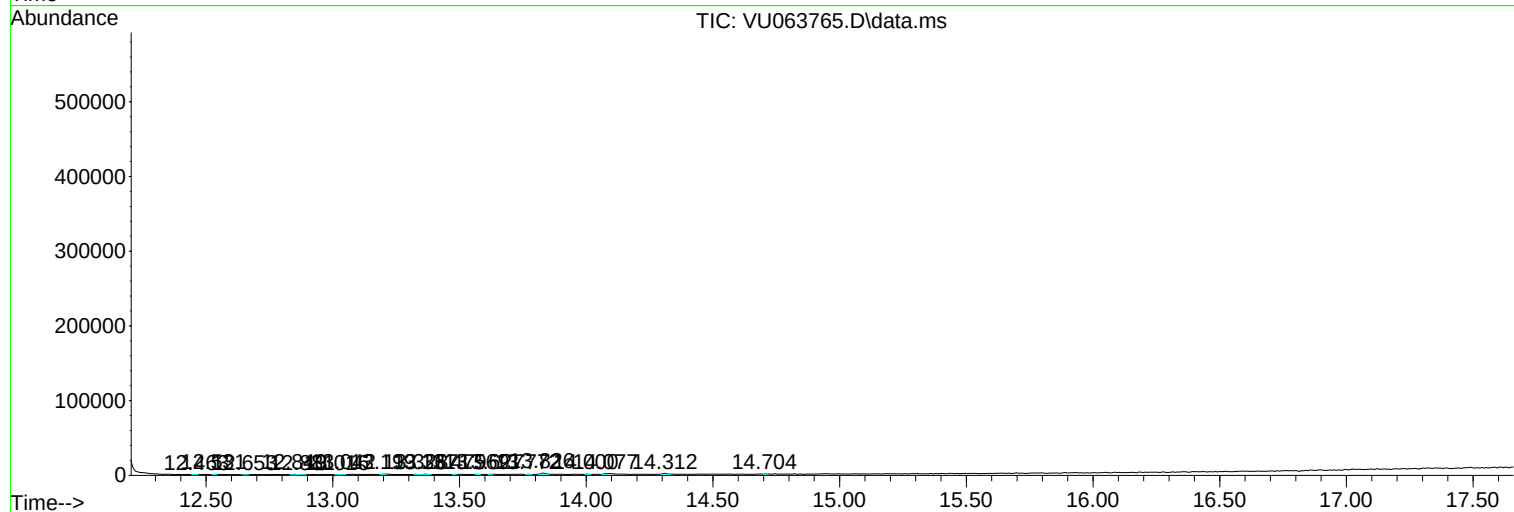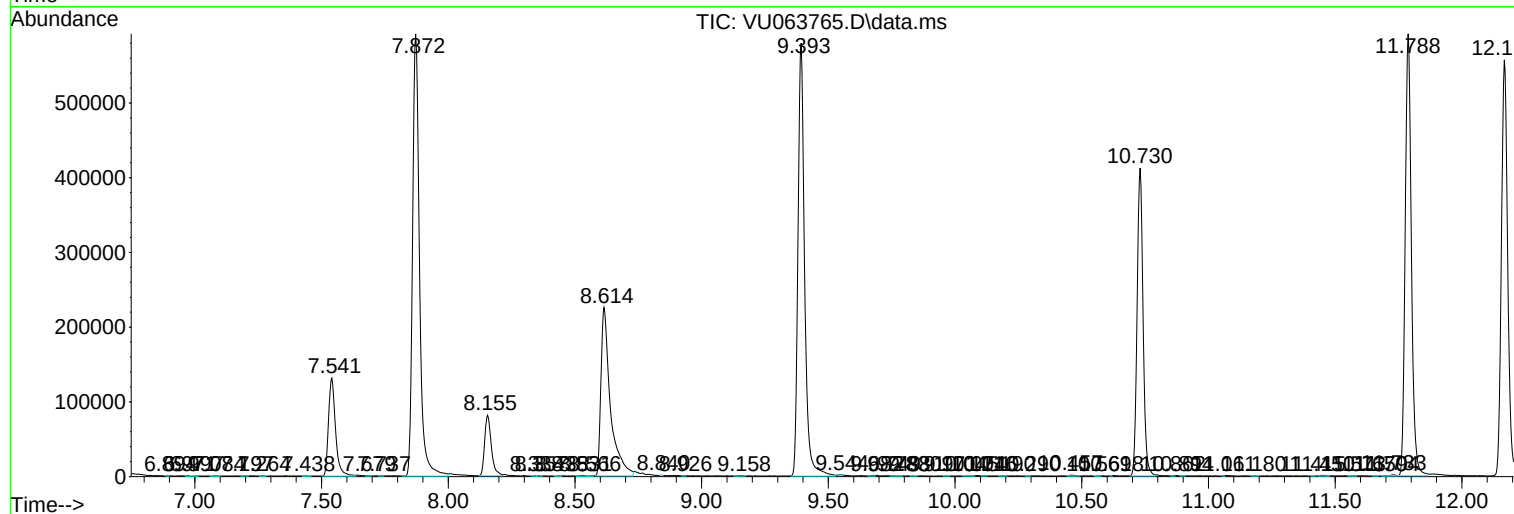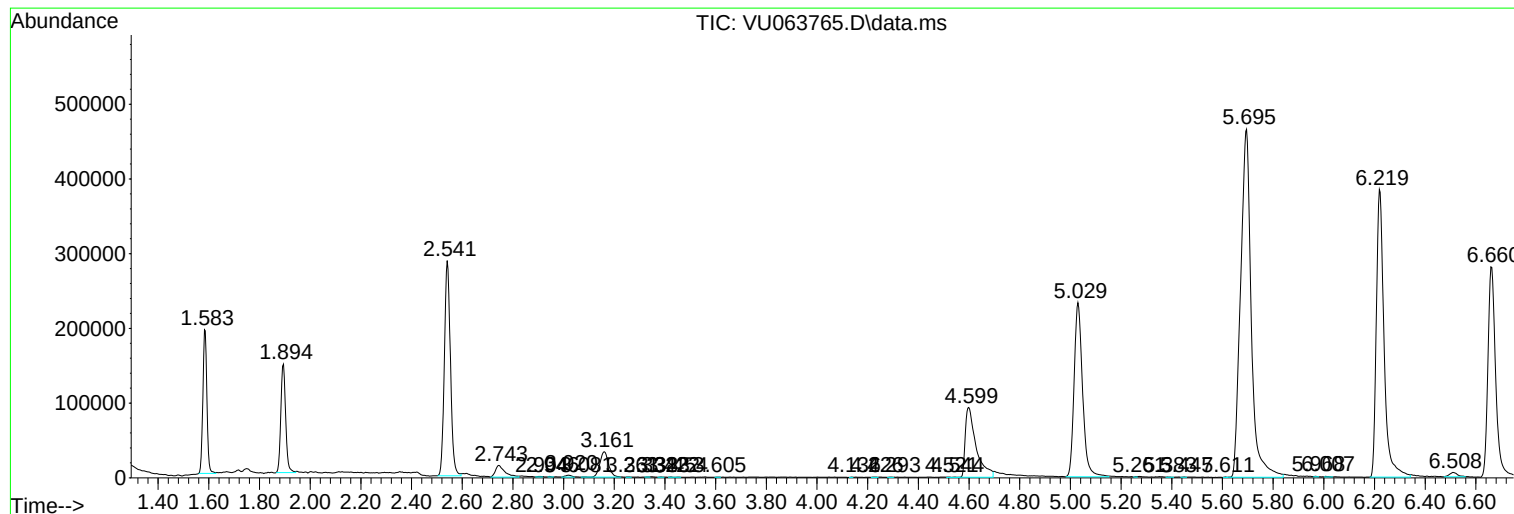

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
Data File : VU063765.D
Acq On : 21 Nov 2025 13:20
Operator : MD/SY
Sample : Q3688-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
M-32S

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
Data File : VU063765.D
Acq On : 21 Nov 2025 13:20
Operator : MD/SY
Sample : Q3688-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
M-32S

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc