

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
 Data File : VU063766.D
 Acq On : 21 Nov 2025 13:44
 Operator : MD/SY
 Sample : Q3688-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 M-30S

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

Signal : TIC: VU063766.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.583	84	91	104	rBV	188067	204392	15.17%	2.016%
2	1.891	179	187	199	rBV	143266	187080	13.88%	1.845%
3	2.470	364	367	368	rBV	805	400	0.03%	0.004%
4	2.541	377	389	405	rBV	286080	471630	35.00%	4.652%
5	2.750	444	454	457	rBV3	3026	4275	0.32%	0.042%
6	3.013	530	536	549	rVB4	2490	4490	0.33%	0.044%
7	3.091	558	560	563	rBV2	447	247	0.02%	0.002%
8	3.158	569	581	603	rVB	6150	14871	1.10%	0.147%
9	3.284	614	620	623	rBV2	466	375	0.03%	0.004%
10	3.338	628	637	646	rBV6	1732	3125	0.23%	0.031%
11	3.406	652	658	660	rBV2	458	305	0.02%	0.003%
12	3.570	699	709	712	rVB2	192	261	0.02%	0.003%
13	3.647	729	733	735	rBV2	236	209	0.02%	0.002%
14	3.769	768	771	778	rVB2	242	276	0.02%	0.003%
15	3.804	778	782	788	rBV	382	397	0.03%	0.004%
16	3.911	810	815	817	rBV2	298	262	0.02%	0.003%
17	4.052	855	859	864	rVB	225	205	0.02%	0.002%
18	4.087	864	870	873	rVB2	333	343	0.03%	0.003%
19	4.222	908	912	916	rVB2	295	245	0.02%	0.002%
20	4.251	916	921	923	rBV	247	249	0.02%	0.002%
21	4.447	977	982	988	rBV2	303	369	0.03%	0.004%
22	4.599	1014	1029	1065	rBV	87492	257201	19.09%	2.537%
23	5.029	1147	1163	1204	rBV2	228917	535780	39.76%	5.285%
24	5.235	1224	1227	1230	rBV3	341	244	0.02%	0.002%
25	5.283	1241	1242	1246	rVB2	365	200	0.01%	0.002%
26	5.306	1246	1249	1251	rVB2	344	219	0.02%	0.002%
27	5.332	1253	1257	1260	rVB3	619	423	0.03%	0.004%
28	5.348	1260	1262	1265	rBV2	565	467	0.03%	0.005%
29	5.457	1293	1296	1301	rVB3	298	241	0.02%	0.002%
30	5.502	1307	1310	1315	rBV2	392	405	0.03%	0.004%
31	5.557	1322	1327	1330	rBV	229	202	0.01%	0.002%
32	5.611	1341	1344	1349	rVB	294	268	0.02%	0.003%
33	5.692	1349	1369	1412	rBV2	457480	1347657	100.00%	13.292%
34	6.097	1493	1495	1500	rBV2	525	413	0.03%	0.004%
35	6.219	1520	1533	1574	rBV	374657	788596	58.52%	7.778%
36	6.467	1607	1610	1612	rVB2	554	288	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
 Data File : VU063766.D
 Acq On : 21 Nov 2025 13:44
 Operator : MD/SY
 Sample : Q3688-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 M-30S

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

37	6.509	1612	1623	1636	rBV7	6056	13501	1.00%	0.133%
38	6.660	1656	1670	1701	rBV	279570	586425	43.51%	5.784%
39	6.917	1747	1750	1753	rVB3	462	250	0.02%	0.002%
40	7.039	1785	1788	1795	rBV2	253	300	0.02%	0.003%
41	7.074	1795	1799	1802	rBV	230	211	0.02%	0.002%
42	7.119	1808	1813	1818	rBV	366	373	0.03%	0.004%
43	7.171	1821	1829	1831	rBV	226	201	0.01%	0.002%
44	7.190	1831	1835	1839	rBV2	475	466	0.03%	0.005%
45	7.357	1884	1887	1891	rVV2	286	204	0.02%	0.002%
46	7.499	1924	1931	1932	rBV2	258	225	0.02%	0.002%
47	7.541	1932	1944	1977	rBV	129321	248070	18.41%	2.447%
48	7.766	2009	2014	2016	rBV3	395	311	0.02%	0.003%
49	7.872	2034	2047	2088	rBV	584643	1107133	82.15%	10.920%
50	8.155	2125	2135	2155	rBV	84563	151889	11.27%	1.498%
51	8.380	2200	2205	2208	rBV3	360	259	0.02%	0.003%
52	8.470	2229	2233	2238	rVB2	304	267	0.02%	0.003%
53	8.531	2247	2252	2255	rVB3	1077	734	0.05%	0.007%
54	8.615	2265	2278	2331	rBV3	219800	589468	43.74%	5.814%
55	8.942	2378	2380	2383	rVB	702	398	0.03%	0.004%
56	8.978	2387	2391	2396	rBV3	295	239	0.02%	0.002%
57	9.026	2404	2406	2413	rVB2	397	278	0.02%	0.003%
58	9.058	2413	2416	2417	rBV	540	209	0.02%	0.002%
59	9.148	2436	2444	2447	rBV3	469	471	0.03%	0.005%
60	9.184	2451	2455	2458	rBV2	373	313	0.02%	0.003%
61	9.261	2476	2479	2484	rBV2	382	293	0.02%	0.003%
62	9.309	2491	2494	2499	rVB	345	258	0.02%	0.003%
63	9.393	2507	2520	2558	rBV	555278	1015606	75.36%	10.017%
64	9.631	2590	2594	2598	rBV3	506	509	0.04%	0.005%
65	9.660	2599	2603	2605	rBV3	501	414	0.03%	0.004%
66	9.782	2638	2641	2646	rVV	200	207	0.02%	0.002%
67	9.807	2646	2649	2655	rVB2	209	223	0.02%	0.002%
68	9.955	2691	2695	2700	rVB2	371	382	0.03%	0.004%
69	10.074	2728	2732	2733	rBV	464	332	0.02%	0.003%
70	10.209	2771	2774	2777	rBV	296	206	0.02%	0.002%
71	10.344	2812	2816	2819	rBV	345	264	0.02%	0.003%
72	10.463	2846	2853	2859	rVB5	1156	1781	0.13%	0.018%
73	10.492	2859	2862	2863	rBV	327	218	0.02%	0.002%
74	10.618	2897	2901	2903	rBV2	448	358	0.03%	0.004%
75	10.634	2904	2906	2912	rVB2	526	371	0.03%	0.004%
76	10.730	2924	2936	2956	rBV	393351	648311	48.11%	6.395%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
 Data File : VU063766.D
 Acq On : 21 Nov 2025 13:44
 Operator : MD/SY
 Sample : Q3688-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 M-30S

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

77	11.068	3038	3041	3045	rVV3	793	748	0.06%	0.007%
78	11.087	3045	3047	3051	rVB	613	397	0.03%	0.004%
79	11.299	3106	3113	3116	rBV2	219	287	0.02%	0.003%
80	11.444	3154	3158	3161	rBV3	493	531	0.04%	0.005%
81	11.531	3182	3185	3188	rVB	467	271	0.02%	0.003%
82	11.730	3239	3247	3252	rBV4	1489	2116	0.16%	0.021%
83	11.788	3252	3265	3288	rBV	575021	978787	72.63%	9.654%
84	12.167	3368	3383	3410	rBV	553862	948200	70.36%	9.352%
85	12.322	3429	3431	3437	rVB3	488	349	0.03%	0.003%
86	12.907	3610	3613	3616	rBV2	317	226	0.02%	0.002%
87	12.994	3637	3640	3643	rBV2	539	398	0.03%	0.004%
88	13.013	3643	3646	3649	rVV2	345	275	0.02%	0.003%
89	13.106	3673	3675	3681	rVB2	520	489	0.04%	0.005%
90	13.196	3698	3703	3706	rBV2	667	633	0.05%	0.006%
91	13.241	3713	3717	3718	rBV	382	225	0.02%	0.002%
92	13.322	3739	3742	3745	rBV2	411	278	0.02%	0.003%
93	13.830	3895	3900	3907	rVB5	1418	1697	0.13%	0.017%
94	13.884	3914	3917	3923	rVB3	399	362	0.03%	0.004%
95	13.917	3923	3927	3930	rBV2	604	545	0.04%	0.005%
96	14.142	3995	3997	4000	rBV3	384	223	0.02%	0.002%
97	14.306	4044	4048	4057	rVB5	1034	1366	0.10%	0.013%
98	14.788	4196	4198	4203	rVB3	659	352	0.03%	0.003%
99	15.518	4423	4425	4427	rBV2	579	291	0.02%	0.003%
100	15.753	4496	4498	4507	rBV6	993	983	0.07%	0.010%




Sum of corrected areas: 10138567

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
Data File : VU063766.D
Acq On : 21 Nov 2025 13:44
Operator : MD/SY
Sample : Q3688-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
M-30S

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

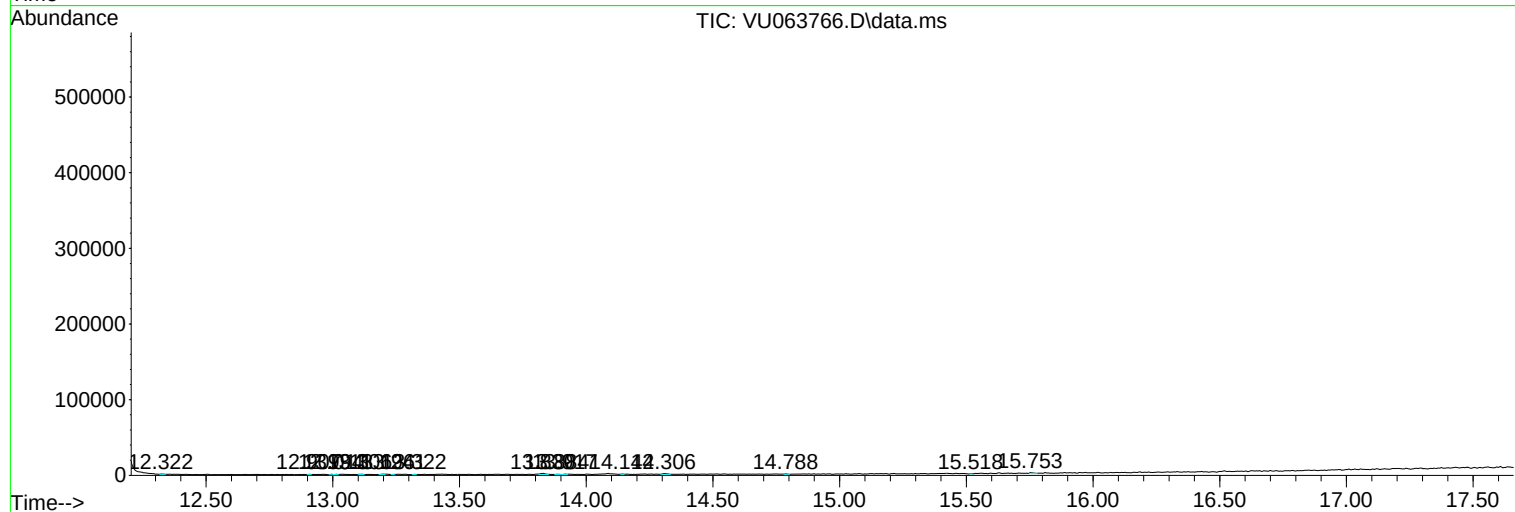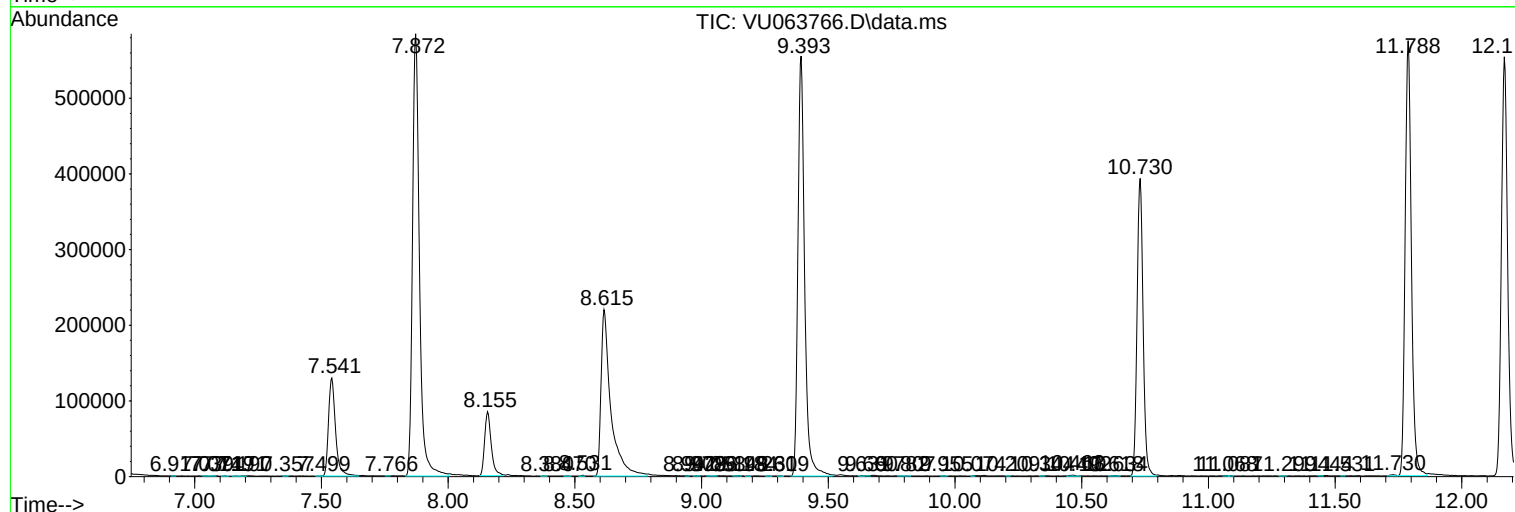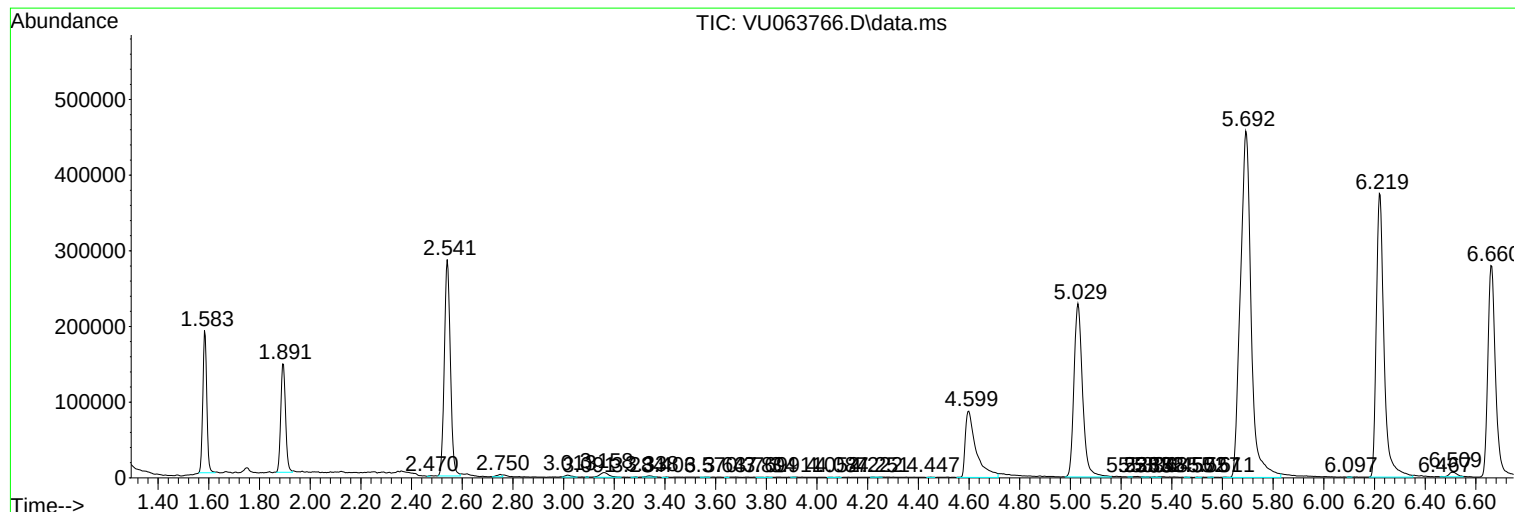

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
Data File : VU063766.D
Acq On : 21 Nov 2025 13:44
Operator : MD/SY
Sample : Q3688-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
M-30S

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
Data File : VU063766.D
Acq On : 21 Nov 2025 13:44
Operator : MD/SY
Sample : Q3688-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
M-30S

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc