

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
 Data File : VU063771.D
 Acq On : 21 Nov 2025 16:10
 Operator : MD/SY
 Sample : Q3688-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

Signal : TIC: VU063771.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.586	84	92	103	rBV	181167	196413	15.11%	1.958%
2	1.891	179	187	200	rBV	135277	177766	13.68%	1.772%
3	2.454	360	362	366	rVB2	1401	780	0.06%	0.008%
4	2.541	377	389	407	rBV	271877	447300	34.42%	4.459%
5	2.769	451	460	469	rBV	2877	4605	0.35%	0.046%
6	2.837	477	481	484	rBV	413	262	0.02%	0.003%
7	2.907	499	503	506	rBV2	573	415	0.03%	0.004%
8	3.020	528	538	548	rVB3	4383	7949	0.61%	0.079%
9	3.158	570	581	596	rBV3	3817	8671	0.67%	0.086%
10	3.332	624	635	647	rVB8	2203	4577	0.35%	0.046%
11	3.386	647	652	659	rBV2	193	273	0.02%	0.003%
12	3.486	679	683	687	rBV2	329	335	0.03%	0.003%
13	3.631	723	728	731	rBV2	393	369	0.03%	0.004%
14	3.837	784	792	795	rBV4	640	699	0.05%	0.007%
15	4.091	867	871	874	rVB2	329	273	0.02%	0.003%
16	4.190	899	902	908	rBV2	255	271	0.02%	0.003%
17	4.296	931	935	942	rVB	421	471	0.04%	0.005%
18	4.338	942	948	952	rBV2	485	645	0.05%	0.006%
19	4.451	980	983	987	rBV2	378	321	0.02%	0.003%
20	4.599	1020	1029	1070	rBV	88741	266645	20.52%	2.658%
21	5.029	1147	1163	1193	rBV	223735	514961	39.63%	5.133%
22	5.271	1237	1238	1242	rVB4	559	262	0.02%	0.003%
23	5.341	1256	1260	1261	rBV3	546	383	0.03%	0.004%
24	5.409	1278	1281	1284	rBV2	366	291	0.02%	0.003%
25	5.438	1288	1290	1296	rVB2	354	342	0.03%	0.003%
26	5.483	1299	1304	1307	rBV2	430	384	0.03%	0.004%
27	5.692	1347	1369	1411	rBV2	433109	1299554	100.00%	12.954%
28	6.026	1470	1473	1479	rVB4	571	448	0.03%	0.004%
29	6.094	1491	1494	1498	rVB3	565	366	0.03%	0.004%
30	6.219	1521	1533	1569	rBV	371231	777493	59.83%	7.750%
31	6.512	1613	1624	1639	rVV	7452	16790	1.29%	0.167%
32	6.586	1645	1647	1652	rVB2	640	461	0.04%	0.005%
33	6.663	1656	1671	1699	rBV	275018	576077	44.33%	5.742%
34	7.000	1773	1776	1780	rVB	402	285	0.02%	0.003%
35	7.081	1794	1801	1810	rVB2	664	901	0.07%	0.009%
36	7.187	1830	1834	1839	rBV3	447	477	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
 Data File : VU063771.D
 Acq On : 21 Nov 2025 16:10
 Operator : MD/SY
 Sample : Q3688-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

37	7.348	1880	1884	1890	rVB2	346	370	0.03%	0.004%
38	7.541	1931	1944	1975	rBV2	123016	237814	18.30%	2.370%
39	7.779	2012	2018	2019	rBV3	1152	1043	0.08%	0.010%
40	7.872	2034	2047	2081	rBV	555305	1048759	80.70%	10.454%
41	8.155	2122	2135	2156	rBV	80792	148753	11.45%	1.483%
42	8.383	2202	2206	2207	rBV2	710	435	0.03%	0.004%
43	8.428	2214	2220	2225	rBV2	245	297	0.02%	0.003%
44	8.528	2244	2251	2259	rBV3	3053	4065	0.31%	0.041%
45	8.615	2267	2278	2317	rBV2	222671	584439	44.97%	5.826%
46	8.888	2359	2363	2364	rBV2	431	280	0.02%	0.003%
47	8.987	2391	2394	2397	rVB2	304	239	0.02%	0.002%
48	9.020	2397	2404	2407	rBV2	251	280	0.02%	0.003%
49	9.042	2407	2411	2414	rVB2	415	286	0.02%	0.003%
50	9.145	2439	2443	2446	rBV3	373	312	0.02%	0.003%
51	9.216	2462	2465	2470	rVB2	300	268	0.02%	0.003%
52	9.264	2470	2480	2481	rBV2	239	288	0.02%	0.003%
53	9.277	2481	2484	2490	rVV2	337	312	0.02%	0.003%
54	9.393	2506	2520	2563	rBV	549365	1009457	77.68%	10.062%
55	9.557	2565	2571	2581	rVB4	3418	5020	0.39%	0.050%
56	9.611	2586	2588	2593	rVB	666	389	0.03%	0.004%
57	9.676	2597	2608	2618	rVV4	3157	5788	0.45%	0.058%
58	9.714	2618	2620	2625	rVV3	442	370	0.03%	0.004%
59	10.090	2727	2737	2740	rBV2	2597	4496	0.35%	0.045%
60	10.222	2773	2778	2782	rBV2	324	334	0.03%	0.003%
61	10.402	2829	2834	2838	rVV2	278	292	0.02%	0.003%
62	10.428	2838	2842	2845	rVV	314	343	0.03%	0.003%
63	10.463	2846	2853	2864	rVB3	2851	4583	0.35%	0.046%
64	10.573	2882	2887	2891	rBV2	272	267	0.02%	0.003%
65	10.602	2891	2896	2900	rVV2	287	350	0.03%	0.003%
66	10.640	2903	2908	2910	rBV3	284	252	0.02%	0.003%
67	10.730	2923	2936	2954	rBV	391842	649872	50.01%	6.478%
68	10.878	2978	2982	2984	rVV3	391	338	0.03%	0.003%
69	11.071	3034	3042	3052	rBV2	3166	4304	0.33%	0.043%
70	11.219	3084	3088	3093	rVB2	295	317	0.02%	0.003%
71	11.325	3116	3121	3126	rBV	312	439	0.03%	0.004%
72	11.450	3152	3160	3168	rVV2	3883	5751	0.44%	0.057%
73	11.640	3216	3219	3227	rVB2	436	503	0.04%	0.005%
74	11.730	3238	3247	3254	rBV3	6673	10007	0.77%	0.100%
75	11.788	3254	3265	3290	rVV	575917	977953	75.25%	9.748%
76	12.048	3344	3346	3349	rVB2	540	337	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
 Data File : VU063771.D
 Acq On : 21 Nov 2025 16:10
 Operator : MD/SY
 Sample : Q3688-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

77	12.090	3353	3359	3364	rBV2	458	535	0.04%	0.005%
78	12.167	3370	3383	3406	rBV	538317	920931	70.87%	9.180%
79	12.386	3446	3451	3452	rBV3	340	309	0.02%	0.003%
80	12.412	3456	3459	3464	rVB	410	377	0.03%	0.004%
81	12.444	3464	3469	3475	rVB3	336	346	0.03%	0.003%
82	12.685	3539	3544	3546	rBV	416	348	0.03%	0.003%
83	12.727	3554	3557	3560	rBV	391	259	0.02%	0.003%
84	12.955	3624	3628	3630	rBV2	383	272	0.02%	0.003%
85	13.007	3642	3644	3650	rVB2	634	469	0.04%	0.005%
86	13.039	3650	3654	3658	rBV3	690	721	0.06%	0.007%
87	13.203	3693	3705	3718	rBV5	6436	11286	0.87%	0.112%
88	13.344	3744	3749	3754	rBV3	584	578	0.04%	0.006%
89	13.405	3764	3768	3770	rBV2	324	269	0.02%	0.003%
90	13.454	3779	3783	3785	rBV2	339	315	0.02%	0.003%
91	13.495	3792	3796	3799	rBV2	306	313	0.02%	0.003%
92	13.515	3799	3802	3807	rVB2	653	510	0.04%	0.005%
93	13.550	3807	3813	3815	rBV2	358	423	0.03%	0.004%
94	13.701	3857	3860	3862	rBV2	445	289	0.02%	0.003%
95	13.820	3888	3897	3908	rBV6	12340	19429	1.50%	0.194%
96	13.913	3919	3926	3930	rBV3	688	914	0.07%	0.009%
97	14.068	3965	3974	3993	rBV	18325	34182	2.63%	0.341%
98	14.306	4039	4048	4064	rVB2	12648	19938	1.53%	0.199%
99	14.952	4246	4249	4251	rBV2	606	380	0.03%	0.004%
100	15.476	4409	4412	4415	rBV3	747	453	0.03%	0.005%




Sum of corrected areas: 10032363

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
Data File : VU063771.D
Acq On : 21 Nov 2025 16:10
Operator : MD/SY
Sample : Q3688-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

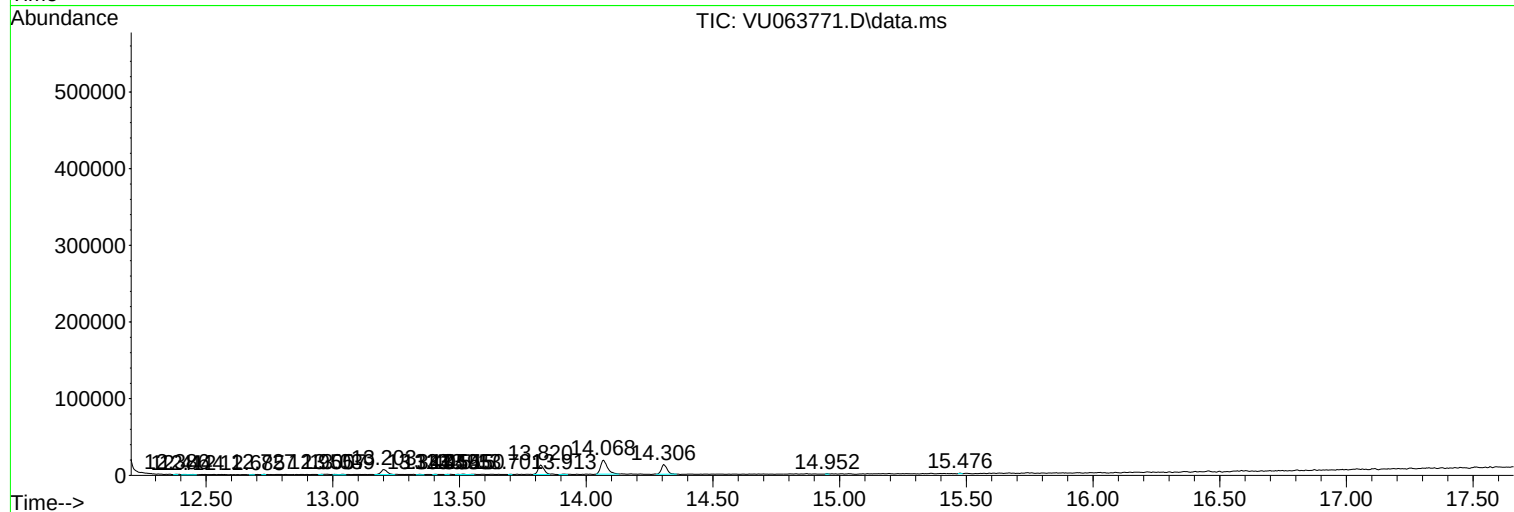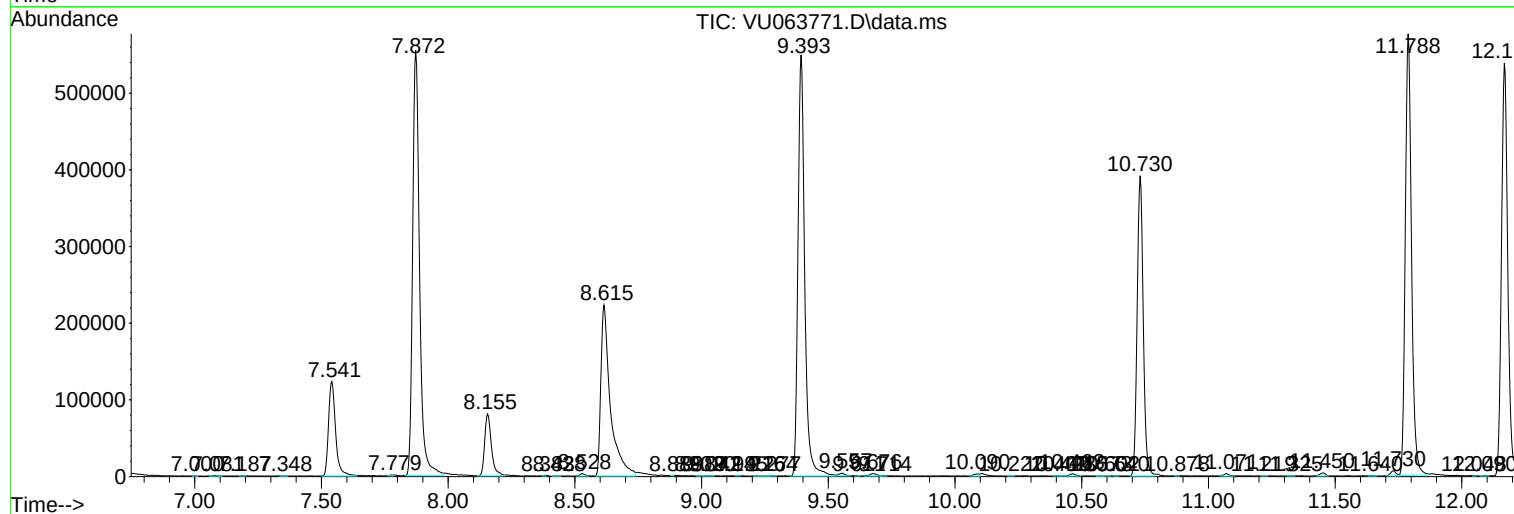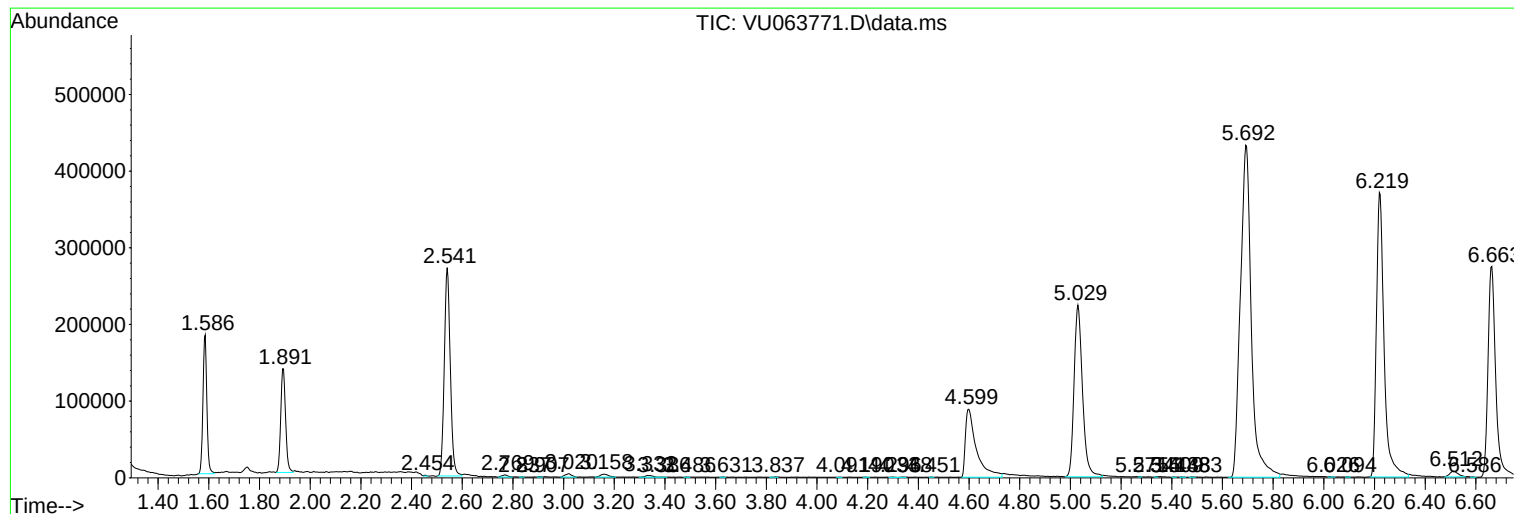

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
Data File : VU063771.D
Acq On : 21 Nov 2025 16:10
Operator : MD/SY
Sample : Q3688-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112125\
Data File : VU063771.D
Acq On : 21 Nov 2025 16:10
Operator : MD/SY
Sample : Q3688-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc