


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU112219\
Data File : VU035813.D
Acq On : 22 Nov 2019 08:36
Operator : JC/SP
Sample : BFB04
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB04

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR112119WMA.M
Title : TRACE VOA SOM01.0
Last Update : Wed Nov 27 17:39:33 2019

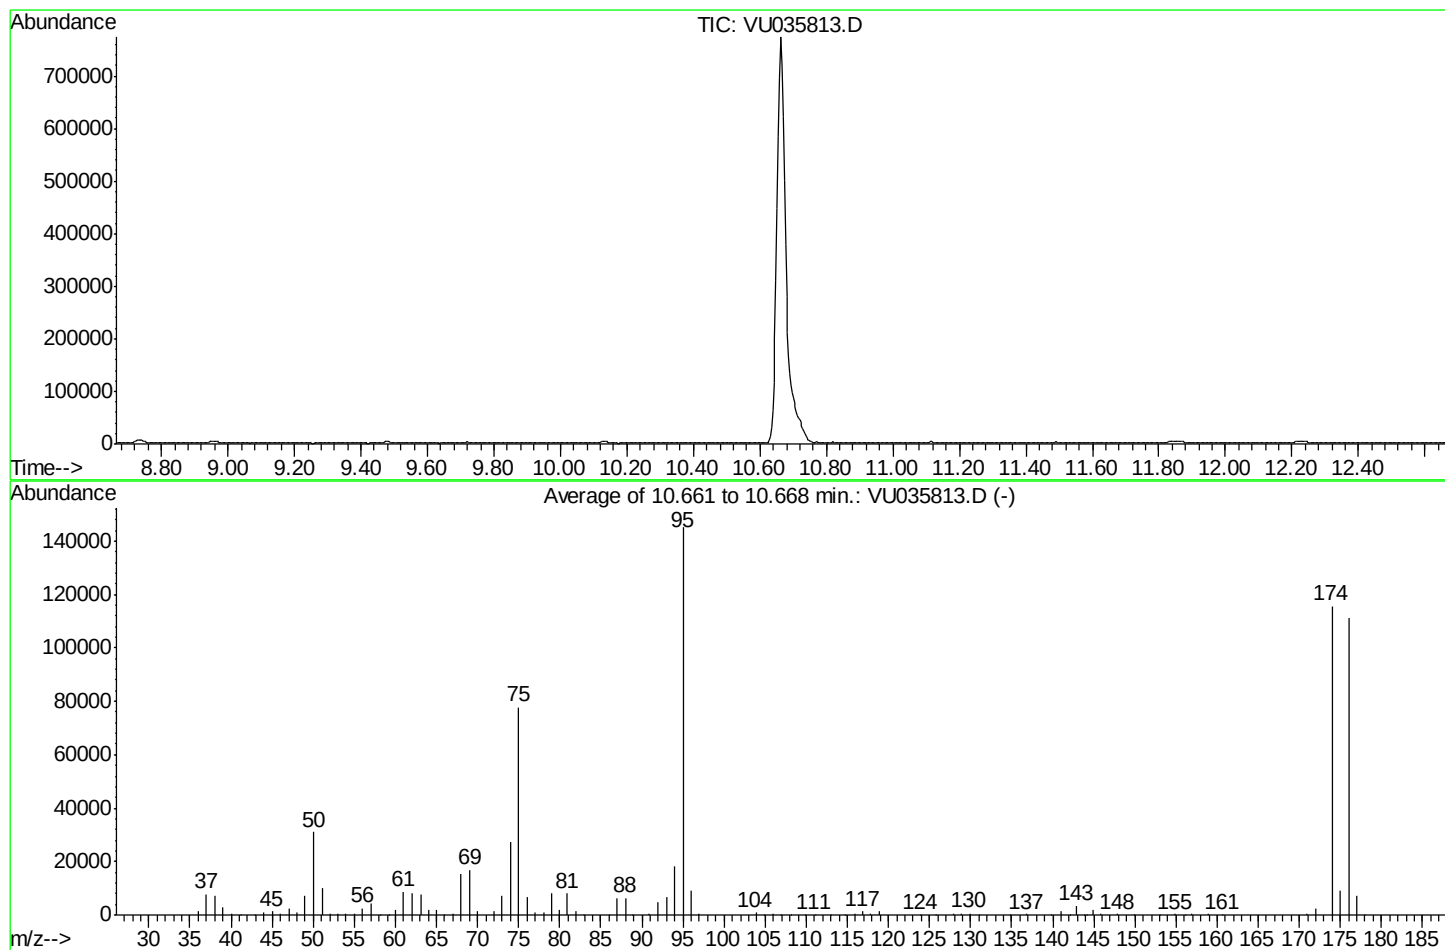

AutoFind: Scans 2899, 2900, 2901; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	30970	PASS
75	95	30	80	53.6	77778	PASS
95	95	100	100	100.0	145152	PASS
96	95	5	9	6.4	9287	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	79.7	115754	PASS
175	174	5	9	7.7	8912	PASS
176	174	95	101	96.2	111352	PASS
177	176	5	9	6.4	7120	PASS

m/z	Abundance
36.00	1437.0
37.00	8159.0
38.00	7860.0
39.10	3155.0
40.00	837.0
41.10	143.0
44.10	1986.0
45.00	1316.0
46.00	272.0
47.00	2109.0
48.00	931.0
49.00	7524.0
50.10	32208.0
51.10	10520.0
52.00	615.0
53.00	493.0
54.00	254.0
55.00	682.0
56.00	2643.0
57.00	4611.0
58.10	265.0
59.20	135.0
60.00	1748.0
61.00	8610.0
62.00	8492.0
63.10	8059.0
64.00	1874.0
65.00	1877.0
65.90	208.0
67.10	450.0
68.00	15508.0
69.10	16520.0
70.00	1394.0
72.00	1227.0
73.00	7386.0
74.00	28344.0
75.00	78664.0
76.10	6826.0
76.90	975.0
78.00	937.0
78.90	8350.0
80.00	2066.0
80.90	8354.0
82.00	1667.0
82.80	174.0
85.90	193.0
87.00	6291.0
88.00	6309.0
88.80	128.0
90.90	639.0
92.00	4704.0
93.00	6978.0
94.00	19264.0
95.00	148160.0
96.00	9659.0
97.00	319.0
103.90	930.0
104.90	201.0
106.00	685.0
107.00	104.0
108.10	184.0
111.00	175.0
114.80	134.0
115.90	745.0
116.90	1409.0
117.90	620.0
118.90	1442.0
123.90	205.0
125.70	109.0
128.00	626.0
128.80	253.0
129.90	672.0
131.00	133.0
134.80	229.0
136.80	302.0
139.80	125.0
141.00	1505.0
142.10	361.0
142.90	3247.0
143.80	205.0
144.90	2022.0
146.00	250.0
147.90	287.0
149.90	216.0
152.90	139.0
155.00	427.0
156.10	120.0
156.90	303.0
158.80	215.0
170.80	541.0
172.00	2130.0
174.00	114872.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

175.00	9123.0
176.00	112344.0
177.00	7229.0
177.90	183.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

m/z	Abundance
36.00	1421.0
37.00	8050.0
38.00	7414.0
39.00	3240.0
40.00	877.0
41.10	135.0
44.00	2003.0
45.00	1367.0
45.90	266.0
47.00	2332.0
48.00	1105.0
49.00	7413.0
50.10	31904.0
51.10	10289.0
52.00	524.0
53.10	398.0
54.00	263.0
55.00	626.0
56.00	2628.0
57.00	4514.0
58.10	275.0
60.00	1878.0
61.00	8967.0
62.00	8435.0
63.10	7883.0
64.00	2030.0
65.00	2104.0
66.00	215.0
67.10	517.0
68.00	15644.0
69.10	17416.0
70.00	1340.0
72.00	1377.0
73.00	7527.0
74.10	27512.0
75.00	79888.0
76.00	6928.0
77.00	937.0
78.00	792.0
78.90	8558.0
79.90	2225.0
80.90	8176.0
81.90	1716.0
82.90	157.0
85.90	237.0
87.00	6150.0
88.00	6514.0
90.90	707.0
92.00	4878.0
93.00	6885.0
94.00	18704.0
95.00	148800.0
96.00	9560.0
97.00	355.0
103.90	781.0
104.90	177.0
106.00	648.0
106.90	115.0
108.10	130.0
111.10	110.0
114.70	145.0
115.90	779.0
116.90	1425.0
117.80	648.0
118.90	1368.0
123.90	168.0
128.00	555.0
128.80	257.0
129.90	742.0
131.10	107.0
134.80	212.0
136.90	319.0
139.80	100.0
141.00	1484.0
142.00	282.0
143.00	3594.0
143.80	194.0
144.10	188.0
144.90	1856.0
145.90	250.0
147.90	306.0
149.90	184.0
152.90	171.0
154.90	401.0
156.90	305.0
158.80	275.0
160.70	114.0
170.90	643.0
172.00	2328.0
174.00	119080.0
175.00	9184.0
176.00	114928.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

177.007358.0

177.90211.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

m/z	Abundance
36.10	1320.0
37.00	7459.0
38.00	6587.0
39.00	3094.0
40.00	910.0
41.10	133.0
42.80	146.0
44.00	2067.0
45.00	1416.0
46.00	263.0
47.00	2199.0
48.00	1065.0
49.00	6745.0
50.10	28800.0
51.10	9235.0
52.00	390.0
53.10	247.0
54.00	255.0
55.10	497.0
56.00	2413.0
57.00	3942.0
58.10	220.0
60.00	1740.0
61.00	8349.0
62.00	7863.0
63.10	7549.0
64.00	1934.0
65.00	2053.0
66.00	175.0
67.00	481.0
68.00	14525.0
69.00	16496.0
70.00	1145.0
72.00	1258.0
73.00	6907.0
74.00	25432.0
75.00	74784.0
76.00	6729.0
76.90	903.0
78.00	680.0
79.00	7958.0
80.00	2211.0
80.90	7562.0
81.90	1686.0
82.90	146.0
86.00	237.0
87.00	5950.0
88.00	6025.0
90.90	634.0
92.00	4713.0
93.00	6411.0
94.00	16720.0
95.00	138496.0
96.00	8643.0
97.00	310.0
103.90	665.0
104.80	181.0
105.90	585.0
106.90	165.0
109.90	106.0
111.10	151.0
113.00	120.0
114.70	129.0
115.90	649.0
116.90	1308.0
117.80	599.0
119.00	1124.0
127.90	459.0
128.90	301.0
129.90	700.0
131.10	121.0
134.80	161.0
136.90	341.0
141.00	1506.0
143.00	3623.0
144.10	168.0
144.90	1581.0
145.80	278.0
147.90	354.0
150.00	156.0
153.00	122.0
154.80	388.0
156.90	231.0
158.90	317.0
160.70	123.0
170.90	749.0
172.00	2112.0
174.00	113312.0
174.90	8431.0
176.00	106784.0
177.00	6774.0
177.90	184.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

Scan 2884 (10.613 min): VU035813.D
BFB04

m/z	Abundance
39.20	102.0
40.00	521.0
44.00	1233.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04