

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112221\
 Data File : VU045938.D
 Acq On : 23 Nov 2021 01:23
 Operator : SY/MD
 Sample : M4775-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1


Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Nov 23 06:50:53 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U110521W.M
 Quant Title : SW846 8260
 QLast Update : Fri Nov 05 13:35:16 2021
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.378	168	114144	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.253	114	207903	50.000	ug/l	0.00
63) Chlorobenzene-d5	9.420	117	219674	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.812	152	115800	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.706	65	86932	50.854	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 101.700%	
35) Dibromofluoromethane	5.292	113	69039	49.738	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 99.480%	
50) Toluene-d8	7.899	98	272178	52.733	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 105.460%	
62) 4-Bromofluorobenzene	10.632	95	109709	53.006	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 106.020%	
Target Compounds						
					Qvalue	
4) Vinyl Chloride	1.607	62	1791	1.086	ug/l	96
8) Diethyl Ether	2.385	74	731	0.847	ug/l	77
11) Tert butyl alcohol	3.186	59	841	2.486	ug/l #	72
12) 1,1-Dichloroethene	2.587	96	1265	1.007	ug/l	83
16) Acetone	2.668	43	1168	1.342	ug/l	95
24) 1,1-Dichloroethane	3.877	63	11415	4.351	ug/l	98
27) cis-1,2-Dichloroethene	4.671	96	6846	4.461	ug/l	90
29) Tetrahydrofuran	5.076	42	3008	4.075	ug/l #	76
31) Cyclohexane	5.378	56	2460	0.986	ug/l #	2
36) 1,1-Dichloropropene	5.375	75	9464	4.668	ug/l #	50
37) Ethyl Acetate	5.076	43	515	0.221	ug/l #	67
38) Carbon Tetrachloride	5.375	117	12113	5.927	ug/l #	15
40) Benzene	5.783	78	3638	0.606	ug/l	99
41) Methacrylonitrile	5.073	41	1647	1.338	ug/l #	31
44) Trichloroethene	6.549	130	2051	1.428	ug/l	91
49) 1,4-Dioxane	7.047	88	209	4.957	ug/l #	13
51) 4-Methyl-2-Pentanone	7.896	43	1087	0.463	ug/l #	1
55) 1,1,2-Trichloroethane	8.275	97	636	0.418	ug/l #	14
59) 2-Hexanone	8.690	43	40	7.554	ug/l #	21
60) Dibromochloromethane	8.555	129	2456	1.549	ug/l #	11
64) Tetrachloroethene	8.552	164	2487	1.973	ug/l	92
65) Chlorobenzene	9.449	112	81233	18.826	ug/l	99
76) 1,2,3-Trichloropropane	10.632	75	56890	16.200	ug/l #	42
79) 2-Chlorotoluene	10.986	91	3281	0.590	ug/l	98
81) trans-1,4-Dichloro-2-b...	10.632	75	56890	52.886	ug/l #	12
82) 4-Chlorotoluene	10.986	91	3281	0.503	ug/l	91
85) sec-Butylbenzene	11.645	105	1870	0.224	ug/l	88
87) 1,3-Dichlorobenzene	11.748	146	7914	2.135	ug/l	98
88) 1,4-Dichlorobenzene	11.838	146	31376	8.370	ug/l	97
91) 1,2-Dichlorobenzene	12.214	146	16755	4.646	ug/l	98
95) Naphthalene	14.089	128	601	1.092	ug/l #	69





(#) = qualifier out of range (m) = manual integration (+) = signals summed



#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.378 min Scan# 11
Delta R.T. 0.003 min
Lab File: VU045938.D
Acq: 23 Nov 2021 01:23




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion:168 Resp: 114144
Ion Ratio Lower Upper
168 100
99 61.2 51.0 76.6

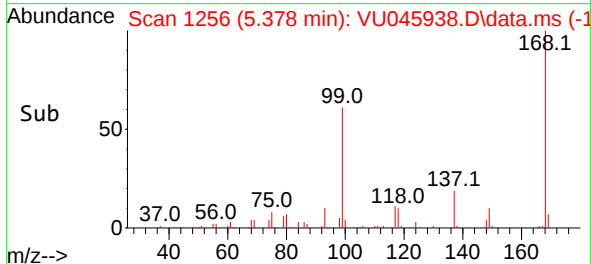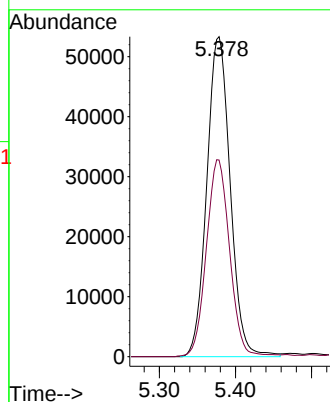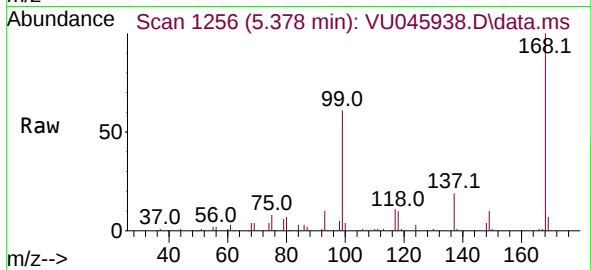

#4
Vinyl Chloride
Concen: 1.086 ug/l
RT: 1.607 min Scan# 83
Delta R.T. -0.000 min
Lab File: VU045938.D
Acq: 23 Nov 2021 01:23

Tgt Ion: 62 Resp: 1791
Ion Ratio Lower Upper
62 100
64 34.2 25.8 38.6

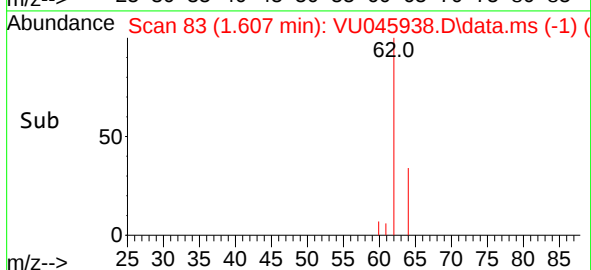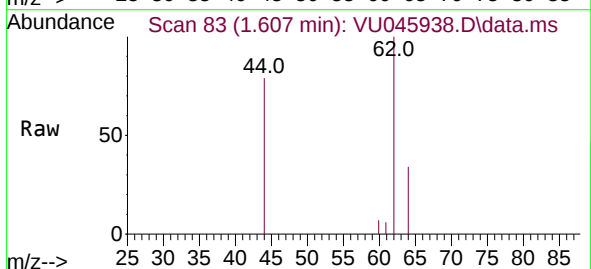



#8

Diethyl Ether

Concen: 0.847 ug/l

RT: 2.385 min Scan# 31

Delta R.T. 0.006 min

Lab File: VU045938.D

Acq: 23 Nov 2021 01:23

Instrument :

MSVOA_U





ClientSampleId :

Tgt Ion: 74 Resp: 731

Ion Ratio Lower Upper

74 100

45 116.7 47.3 141.8

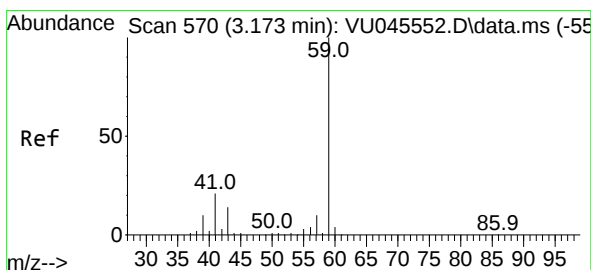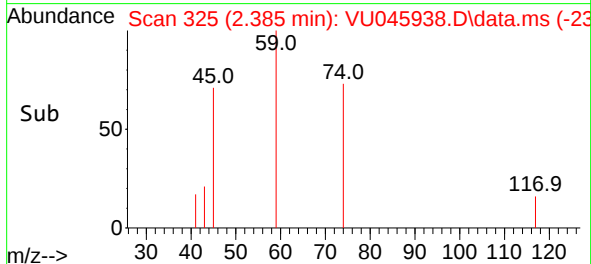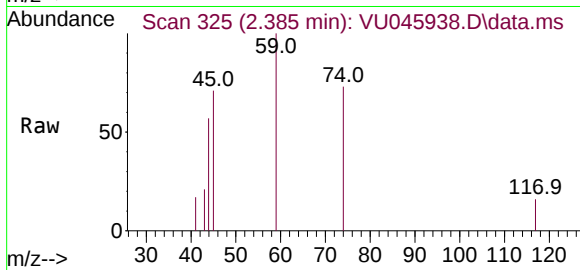

#11

Tert butyl alcohol

Concen: 2.486 ug/l

RT: 3.186 min Scan# 574

Delta R.T. 0.013 min

Lab File: VU045938.D




Acq: 23 Nov 2021 01:23


Tgt Ion: 59 Resp: 841

Ion Ratio Lower Upper

59 100

57 0.0 8.3 12.5#

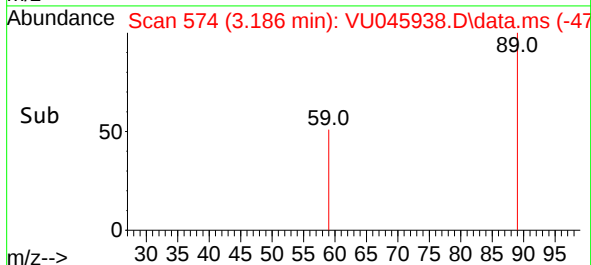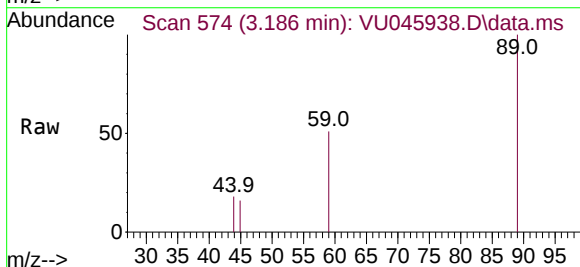



#12

1,1-Dichloroethene

Concen: 1.007 ug/l

RT: 2.587 min Scan# 386

Delta R.T. 0.006 min


Lab File: VU045938.D

Acq: 23 Nov 2021 01:23

Instrument :

MSVOA_U

ClientSampleId :






Tgt Ion: 96 Resp: 1265

Ion Ratio Lower Upper

96 100

61 140.7 137.1 205.7

98 66.0 51.5 77.3

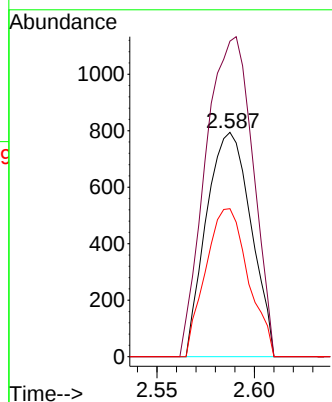

#16

Acetone

Concen: 1.342 ug/l

RT: 2.668 min Scan# 413

Delta R.T. 0.045 min

Lab File: VU045938.D




Acq: 23 Nov 2021 01:23


Tgt Ion: 43 Resp: 1168

Ion Ratio Lower Upper

43 100

58 29.9 26.2 39.2


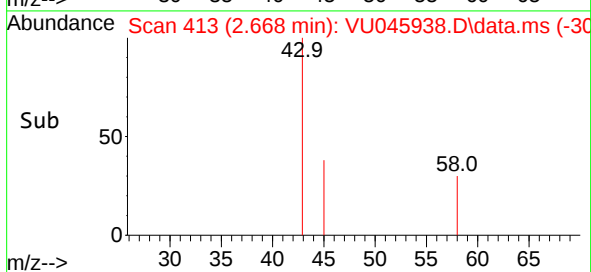
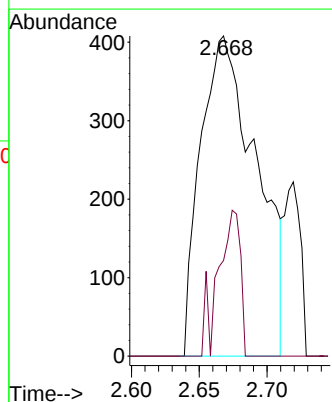





#24
 1,1-Dichloroethane
 Concen: 4.351 ug/l
 RT: 3.877 min Scan# 71
 Delta R.T. 0.003 min
 Lab File: VU045938.D
 Acq: 23 Nov 2021 01:23




Instrument :
 MSVOA_U
 ClientSampleId :


Tgt Ion: 63 Resp: 11415
 Ion Ratio Lower Upper
 63 100
 98 8.1 3.5 10.6
 100 5.2 2.4 7.2

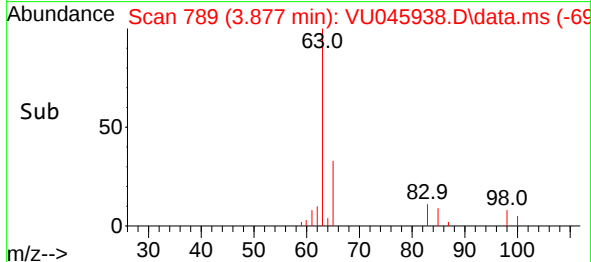

#27
 cis-1,2-Dichloroethene
 Concen: 4.461 ug/l
 RT: 4.671 min Scan# 1036
 Delta R.T. -0.000 min
 Lab File: VU045938.D
 Acq: 23 Nov 2021 01:23

Tgt Ion: 96 Resp: 6846
 Ion Ratio Lower Upper
 96 100
 61 134.2 0.0 299.2
 98 67.5 0.0 127.6

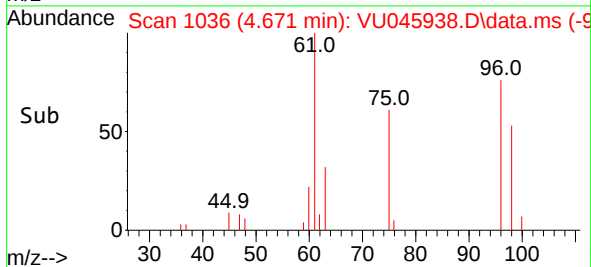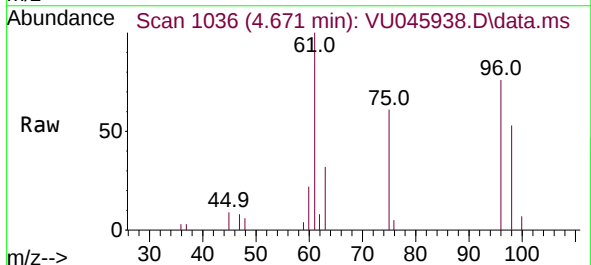



#29

Tetrahydrofuran

Concen: 4.075 ug/l

RT: 5.076 min Scan# 1153

Delta R.T. 0.029 min


Lab File: VU045938.D

Acq: 23 Nov 2021 01:23

Instrument :

MSVOA_U

ClientSampleId :






Tgt Ion: 42 Resp: 3008

Ion Ratio Lower Upper

42 100

72 37.7 38.2 57.4#

71 22.6 35.4 53.2#

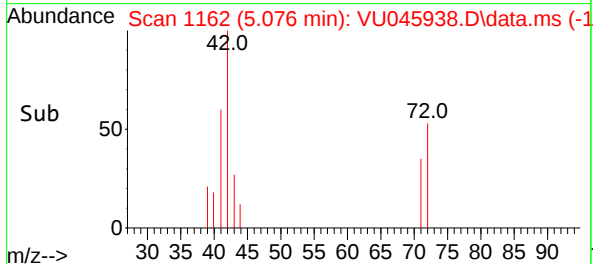

#31

Cyclohexane

Concen: 0.986 ug/l

RT: 5.378 min Scan# 1256

Delta R.T. -0.013 min

Lab File: VU045938.D

Acq: 23 Nov 2021 01:23




Tgt Ion: 56 Resp: 2460


Ion Ratio Lower Upper

56 100

69 173.4 26.4 39.6#

84 121.8 68.4 102.6#

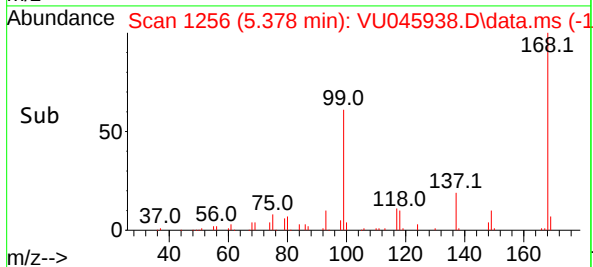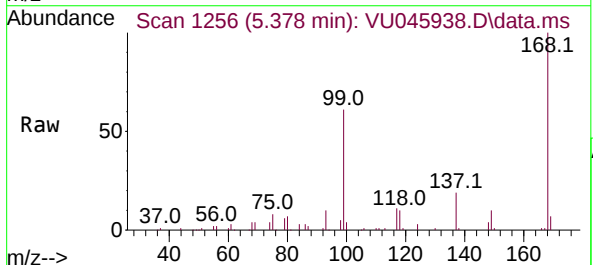



#33

1,2-Dichloroethane-d4

Concen: 50.854 ug/l

RT: 5.706 min Scan# 1

Delta R.T. 0.003 min

Lab File: VU045938.D

Acq: 23 Nov 2021 01:23

Instrument :

MSVOA_U





ClientSampleId :

Tgt Ion: 65 Resp: 86932

Ion Ratio Lower Upper

65 100

67 53.3 0.0 105.8

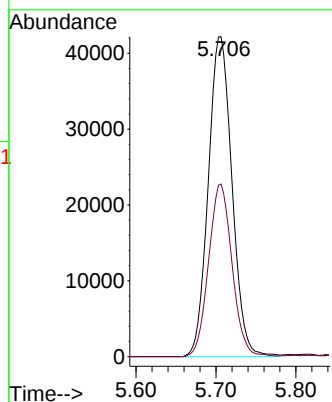

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.253 min Scan# 1528

Delta R.T. -0.000 min

Lab File: VU045938.D

Acq: 23 Nov 2021 01:23




Tgt Ion: 114 Resp: 207903


Ion Ratio Lower Upper

114 100

63 20.7 0.0 45.6

88 16.9 0.0 33.8


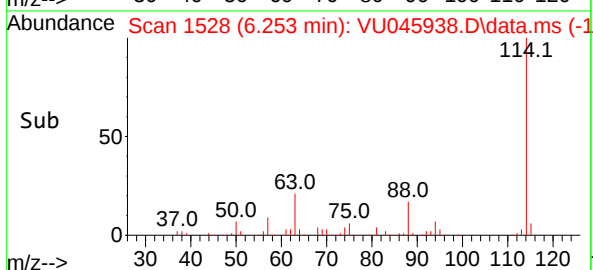






#35
Dibromofluoromethane
Concen: 49.738 ug/l
RT: 5.292 min Scan# 11
Delta R.T. -0.000 min
Lab File: VU045938.D
Acq: 23 Nov 2021 01:23




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion:113 Resp: 69039
Ion Ratio Lower Upper
113 100
111 103.3 82.8 124.2
192 19.1 14.8 22.2

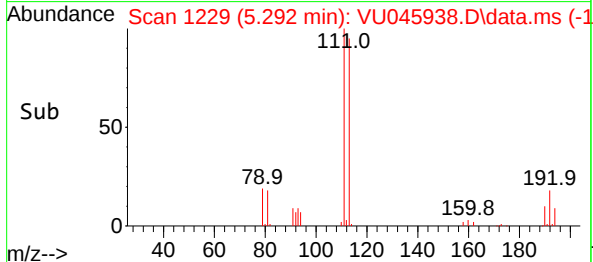

#36
1,1-Dichloropropene
Concen: 4.668 ug/l
RT: 5.375 min Scan# 1255
Delta R.T. -0.154 min
Lab File: VU045938.D
Acq: 23 Nov 2021 01:23

Tgt Ion: 75 Resp: 9464
Ion Ratio Lower Upper
75 100
110 8.2 16.7 50.0#
77 0.0 25.0 37.4#

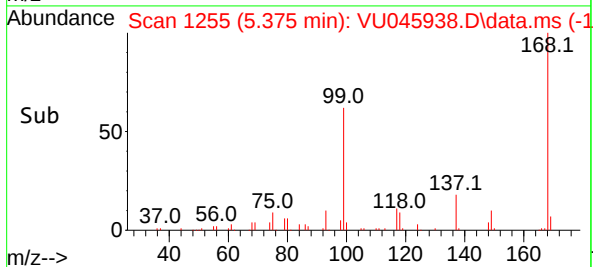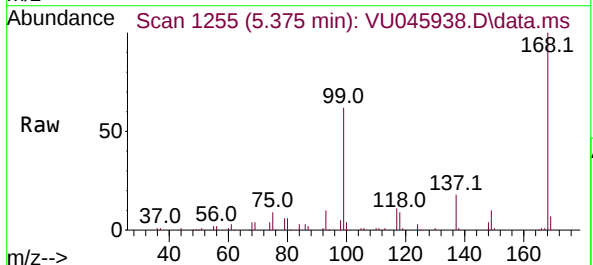



#37

Ethyl Acetate

Concen: 0.221 ug/l

RT: 5.076 min Scan# 1162

Delta R.T. 0.273 min

Lab File: VU045938.D





Acq: 23 Nov 2021 01:23

Instrument :

MSVOA_U

ClientSampleId :

Tgt Ion:	43	Resp:	515
Ion	Ratio	Lower	Upper
43	100		
61	0.0	11.6	17.4#
70	0.0	9.1	13.7#

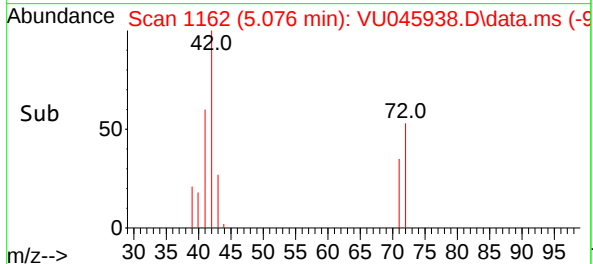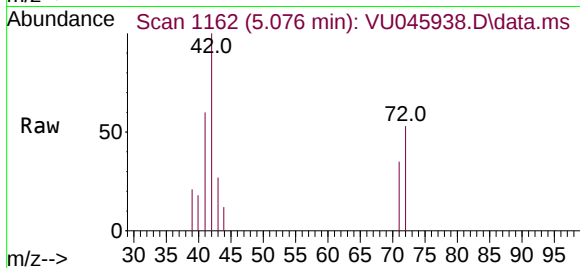

#38

Carbon Tetrachloride

Concen: 5.927 ug/l




RT: 5.375 min Scan# 1255


Delta R.T. -0.154 min

Lab File: VU045938.D

Acq: 23 Nov 2021 01:23

Tgt Ion:	117	Resp:	12113
Ion	Ratio	Lower	Upper
117	100		
119	4.6	77.4	116.0#
121	0.0	24.8	37.2#


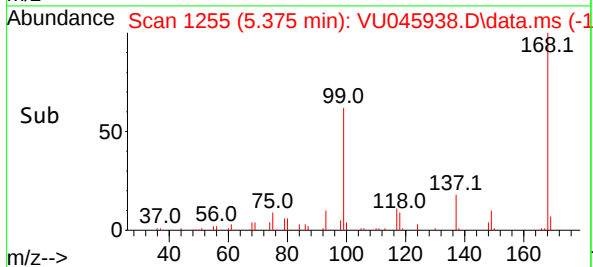

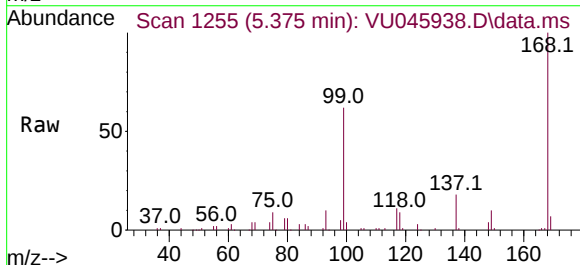




#40
Benzene
Concen: 0.606 ug/l
RT: 5.783 min Scan# 1161
Delta R.T. 0.006 min
Lab File: VU045938.D
Acq: 23 Nov 2021 01:23




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 78 Resp: 3638
Ion Ratio Lower Upper
78 100
77 23.4 19.0 28.4

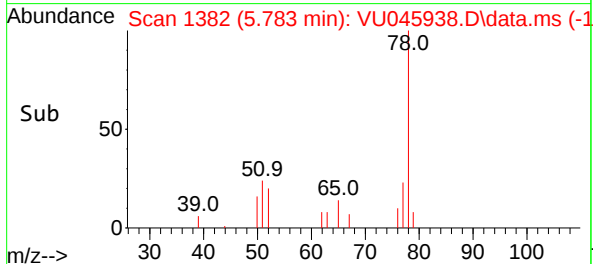

#41
Methacrylonitrile
Concen: 1.338 ug/l
RT: 5.073 min Scan# 1161
Delta R.T. 0.103 min
Lab File: VU045938.D
Acq: 23 Nov 2021 01:23

Tgt Ion: 41 Resp: 1647
Ion Ratio Lower Upper
41 100
39 19.6 43.4 65.0#
67 0.0 61.0 91.4#
52 0.0 23.4 35.0#


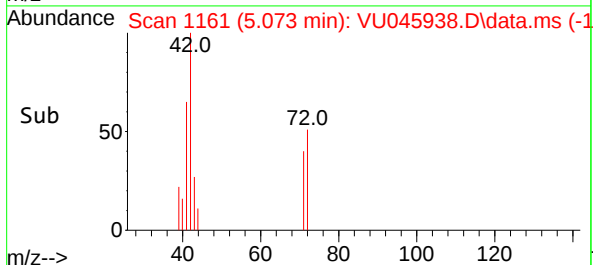
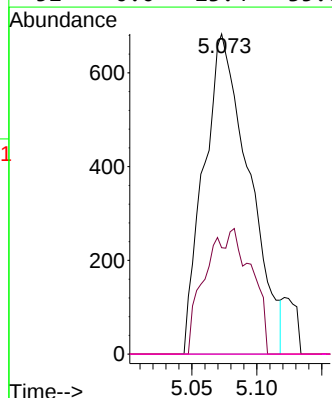
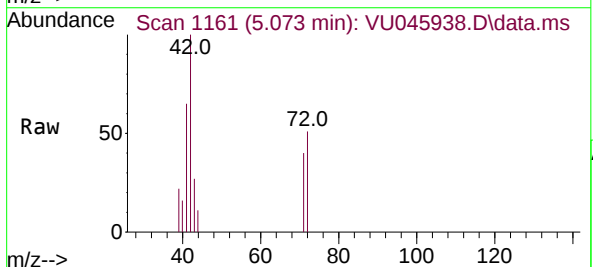




#44
Trichloroethene
Concen: 1.428 ug/l
RT: 6.549 min Scan# 1
Delta R.T. 0.003 min
Lab File: VU045938.D
Acq: 23 Nov 2021 01:23




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion:130 Resp: 2051
Ion Ratio Lower Upper
130 100
95 96.3 0.0 211.4

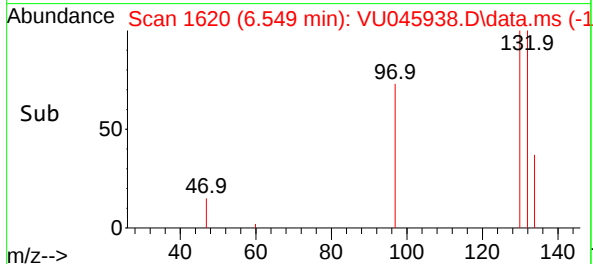

#49
1,4-Dioxane
Concen: 4.957 ug/l
RT: 7.047 min Scan# 1775
Delta R.T. 0.087 min
Lab File: VU045938.D
Acq: 23 Nov 2021 01:23

Tgt Ion: 88 Resp: 209
Ion Ratio Lower Upper
88 100
43 10.0 0.0 0.0#
58 0.0 58.7 88.1#


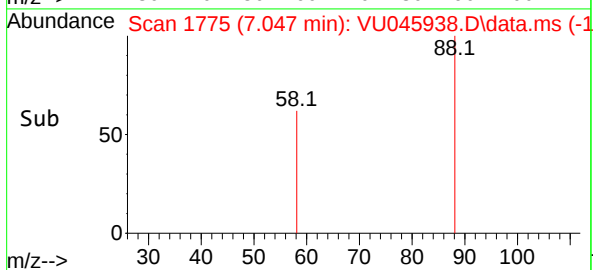

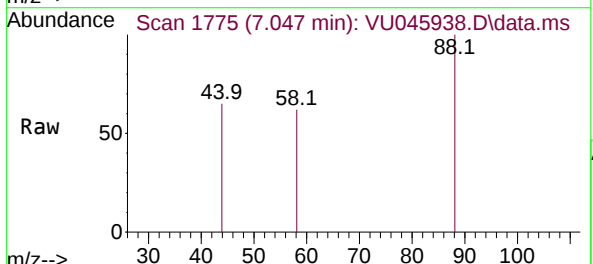




#50
Toluene-d8
Concen: 52.733 ug/l
RT: 7.899 min Scan# 2040
Delta R.T. -0.000 min
Lab File: VU045938.D
Acq: 23 Nov 2021 01:23




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 98 Resp: 272178
Ion Ratio Lower Upper
98 100
100 65.6 52.5 78.7

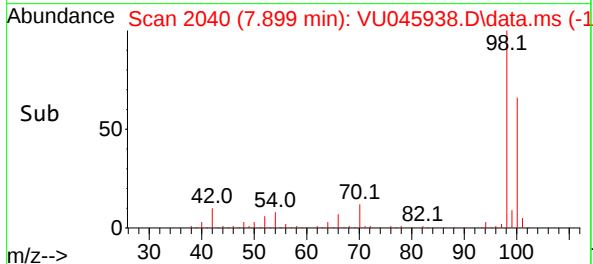

#51
4-Methyl-2-Pentanone
Concen: 0.463 ug/l
RT: 7.896 min Scan# 2039
Delta R.T. 0.103 min
Lab File: VU045938.D
Acq: 23 Nov 2021 01:23


Tgt Ion: 43 Resp: 1087
Ion Ratio Lower Upper
43 100
58 181.2 33.8 50.8#

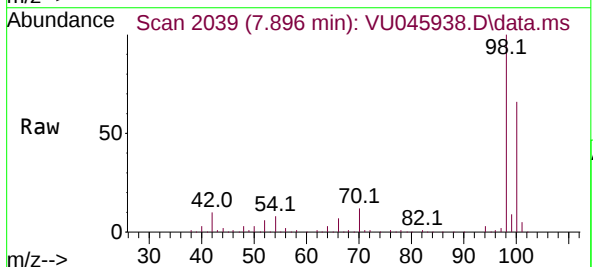






#55
1,1,2-Trichloroethane
Concen: 0.418 ug/l
RT: 8.275 min Scan# 2196
Delta R.T. -0.126 min
Lab File: VU045938.D
Acq: 23 Nov 2021 01:23

Instrument :
MSVOA_U
ClientSampleId :







Tgt Ion: 97 Resp: 636
Ion Ratio Lower Upper
97 100
83 0.0 70.3 105.5#
85 0.0 45.5 68.3#
99 0.0 49.7 74.5#

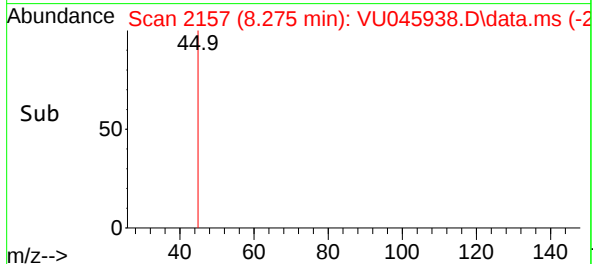

#59
2-Hexanone
Concen: 7.554 ug/l
RT: 8.690 min Scan# 2286
Delta R.T. 0.006 min
Lab File: VU045938.D
Acq: 23 Nov 2021 01:23

Tgt Ion: 43 Resp: 40
Ion Ratio Lower Upper
43 100
58 0.0 29.5 88.6#


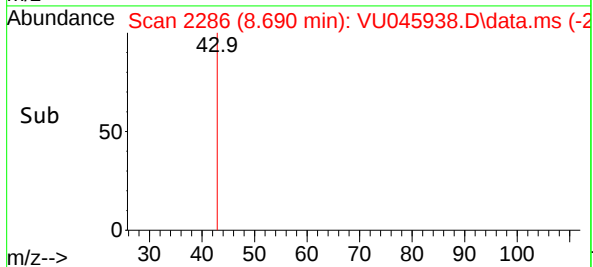

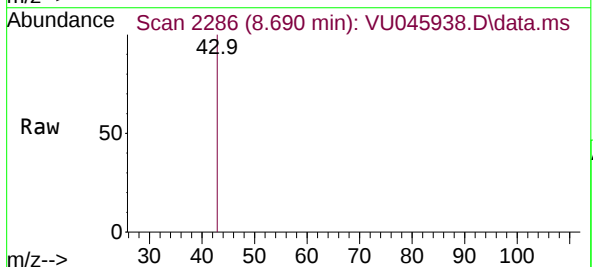




#60
Dibromochloromethane
Concen: 1.549 ug/l
RT: 8.555 min Scan# 211
Delta R.T. -0.257 min
Lab File: VU045938.D
Acq: 23 Nov 2021 01:23




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion:129 Resp: 2456
Ion Ratio Lower Upper
129 100
127 0.0 38.5 115.3#

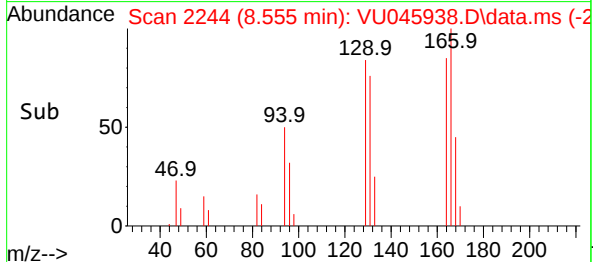

#62
4-Bromofluorobenzene
Concen: 53.006 ug/l
RT: 10.632 min Scan# 2890
Delta R.T. -0.000 min
Lab File: VU045938.D
Acq: 23 Nov 2021 01:23

Tgt Ion: 95 Resp: 109709
Ion Ratio Lower Upper
95 100
174 76.1 0.0 141.8
176 72.2 0.0 138.2


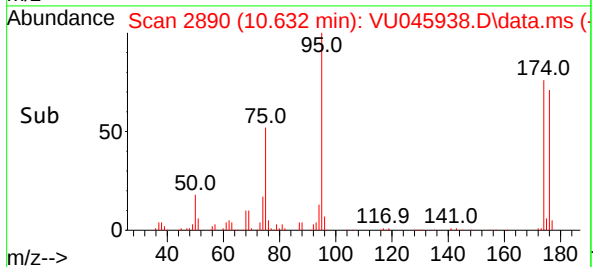

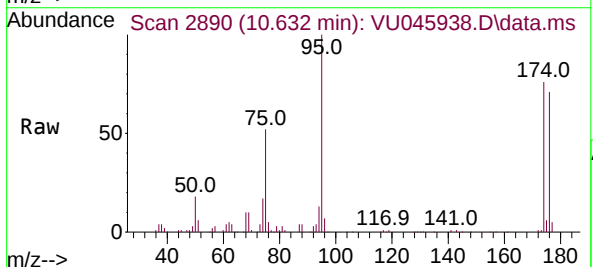




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.420 min Scan# 2196
Delta R.T. 0.000 min
Lab File: VU045938.D
Acq: 23 Nov 2021 01:23




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion:117 Resp: 219674
Ion Ratio Lower Upper
117 100
82 56.9 47.8 71.8
119 31.8 25.8 38.8

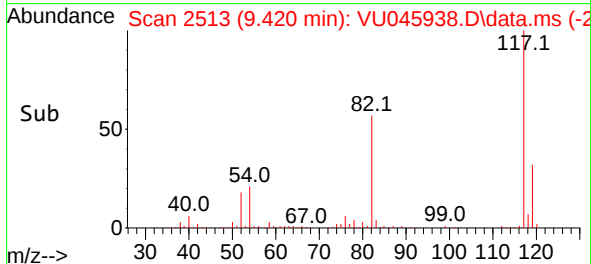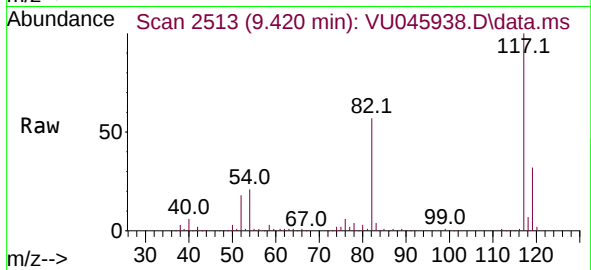

#64
Tetrachloroethene
Concen: 1.973 ug/l
RT: 8.552 min Scan# 2243
Delta R.T. -0.003 min
Lab File: VU045938.D
Acq: 23 Nov 2021 01:23

Tgt Ion:164 Resp: 2487
Ion Ratio Lower Upper
164 100
166 118.3 102.2 153.4
129 93.7 78.2 117.4
131 83.2 75.1 112.7


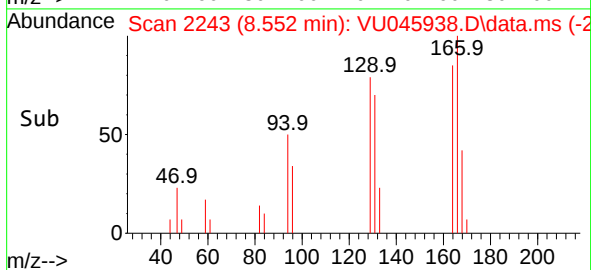

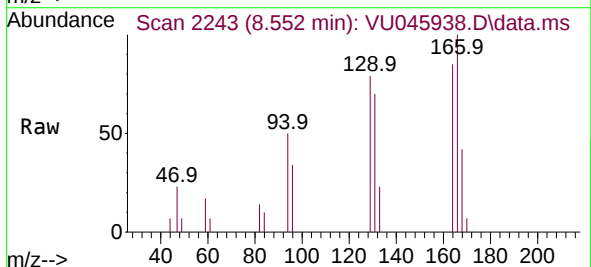




#65
Chlorobenzene
Concen: 18.826 ug/l
RT: 9.449 min Scan# 2522
Delta R.T. -0.000 min
Lab File: VU045938.D
Acq: 23 Nov 2021 01:23




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion:112 Resp: 81233
Ion Ratio Lower Upper
112 100
114 32.4 25.7 38.5

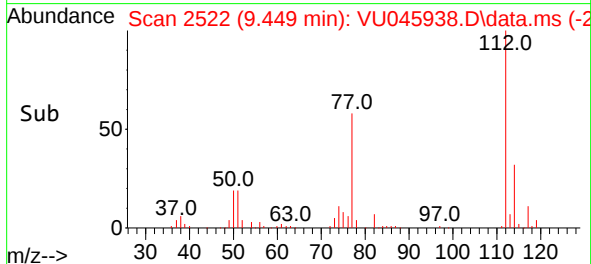

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.812 min Scan# 3257
Delta R.T. -0.000 min
Lab File: VU045938.D
Acq: 23 Nov 2021 01:23

Tgt Ion:152 Resp: 115800
Ion Ratio Lower Upper
152 100
115 61.7 42.7 128.1
150 159.6 0.0 346.8



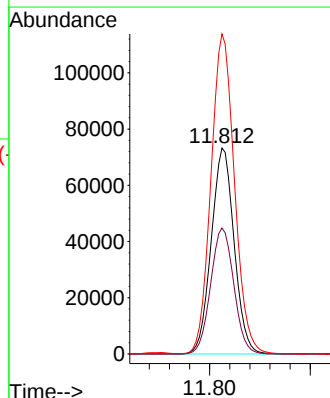
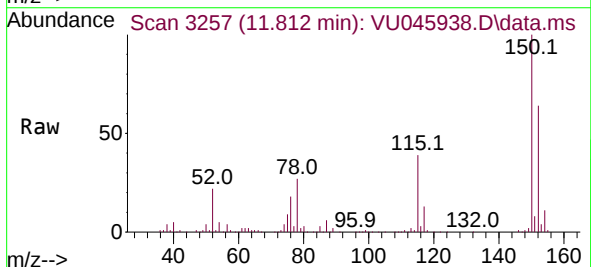




#76
1,2,3-Trichloropropane
Concen: 16.200 ug/l
RT: 10.632 min Scan# 21
Delta R.T. -0.193 min
Lab File: VU045938.D
Acq: 23 Nov 2021 01:23




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 75 Resp: 56890
Ion Ratio Lower Upper
75 100
77 1.1 17.1 51.3#

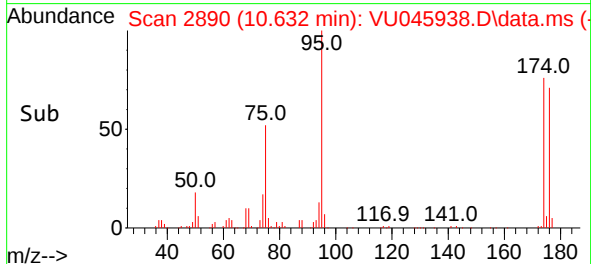

#79
2-Chlorotoluene
Concen: 0.590 ug/l
RT: 10.986 min Scan# 3000
Delta R.T. -0.000 min
Lab File: VU045938.D
Acq: 23 Nov 2021 01:23

Tgt Ion: 91 Resp: 3281
Ion Ratio Lower Upper
91 100
126 32.6 15.6 46.8


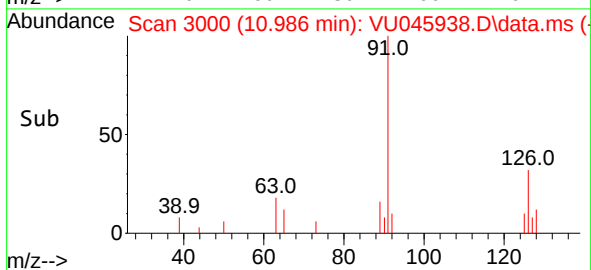

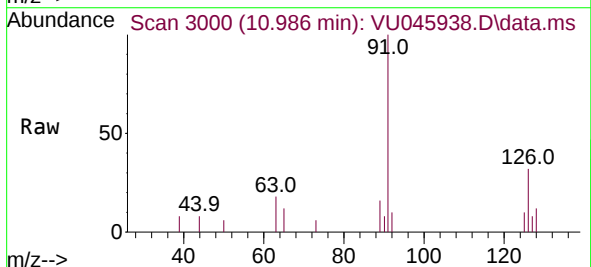




#81
trans-1,4-Dichloro-2-butene
Concen: 52.886 ug/l
RT: 10.632 min Scan# 21
Delta R.T. 0.083 min
Lab File: VU045938.D
Acq: 23 Nov 2021 01:23




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 75 Resp: 56890
Ion Ratio Lower Upper
75 100
53 0.0 76.2 114.4#
89 0.0 34.0 51.0#

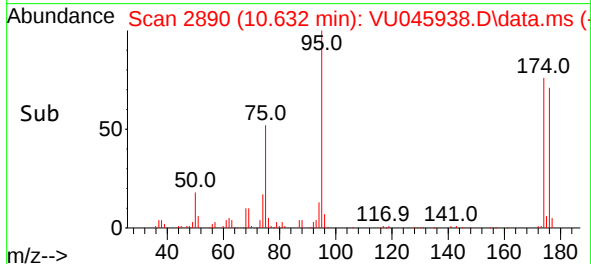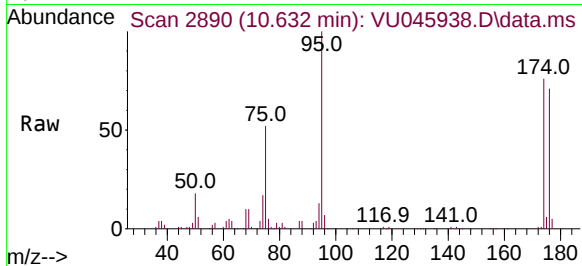

#82
4-Chlorotoluene
Concen: 0.503 ug/l
RT: 10.986 min Scan# 3000
Delta R.T. -0.113 min
Lab File: VU045938.D
Acq: 23 Nov 2021 01:23

Tgt Ion: 91 Resp: 3281
Ion Ratio Lower Upper
91 100
126 32.6 13.8 41.4


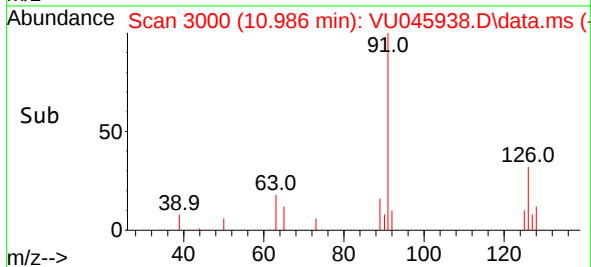

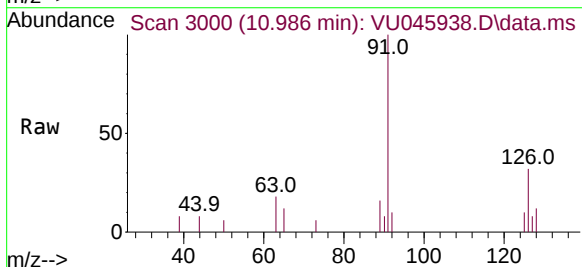




#85
 sec-Butylbenzene
 Concen: 0.224 ug/l
 RT: 11.645 min Scan# 3205
 Delta R.T. -0.000 min
 Lab File: VU045938.D
 Acq: 23 Nov 2021 01:23




Instrument :
 MSVOA_U
 ClientSampleId :


Tgt Ion:105 Resp: 1870
 Ion Ratio Lower Upper
 105 100
 134 13.7 9.4 28.3

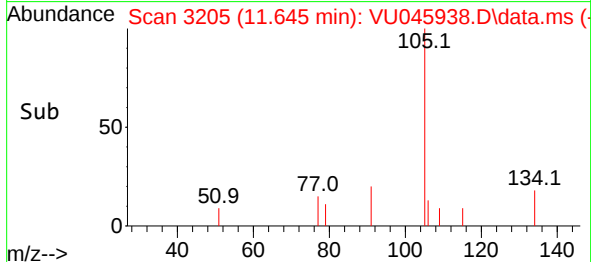

#87
 1,3-Dichlorobenzene
 Concen: 2.135 ug/l
 RT: 11.748 min Scan# 3237
 Delta R.T. -0.000 min
 Lab File: VU045938.D
 Acq: 23 Nov 2021 01:23


Tgt Ion:146 Resp: 7914
 Ion Ratio Lower Upper
 146 100
 111 39.1 21.3 63.9
 148 63.3 31.7 95.1

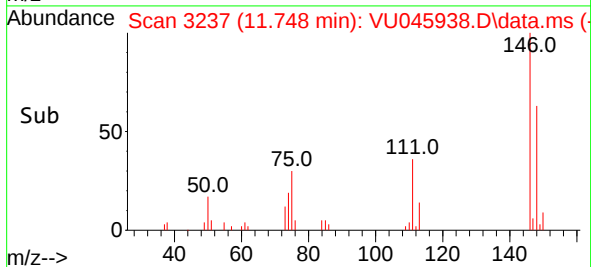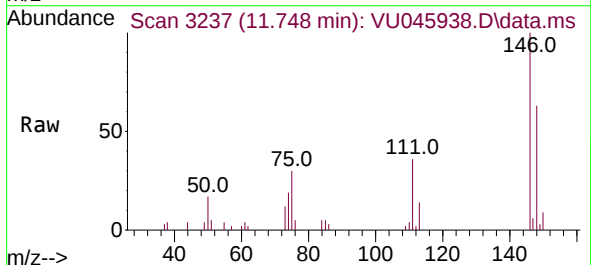






#88
1,4-Dichlorobenzene
Concen: 8.370 ug/l
RT: 11.838 min Scan# 31376
Delta R.T. -0.000 min
Lab File: VU045938.D
Acq: 23 Nov 2021 01:23


Instrument :
MSVOA_U
ClientSampleId :





Tgt Ion:146 Resp: 31376
Ion Ratio Lower Upper
146 100
111 44.6 20.6 61.9
148 63.0 31.9 95.7

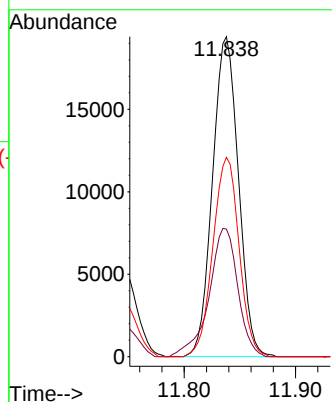


#91
1,2-Dichlorobenzene
Concen: 4.646 ug/l
RT: 12.214 min Scan# 3382
Delta R.T. -0.000 min
Lab File: VU045938.D
Acq: 23 Nov 2021 01:23



Tgt Ion:146 Resp: 16755
Ion Ratio Lower Upper
146 100
111 42.4 21.9 65.5
148 62.3 32.1 96.3

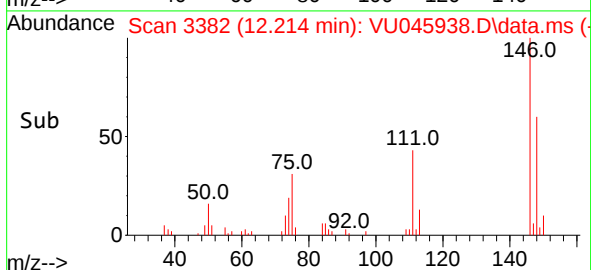



#95

Naphthalene

Concen: 1.092 ug/l

RT: 14.089 min Scan# 3965

Delta R.T. 0.003 min


Lab File: VU045938.D

Acq: 23 Nov 2021 01:23

Instrument :

MSVOA_U

ClientSampleId :

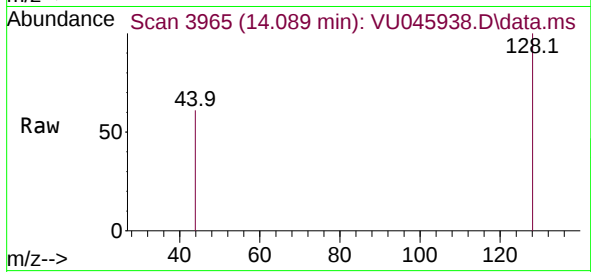

Tgt Ion:128 Resp: 601

Ion Ratio Lower Upper

128 100

127 0.0 10.6 15.8#

129 0.0 8.6 13.0#

