


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112221\
 Data File : VU045904.D
 Acq On : 22 Nov 2021 09:43
 Operator : SY/MD
 Sample : BFB
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U110521W.M
 Title : SW846 8260
 Last Update : Fri Nov 05 13:35:16 2021

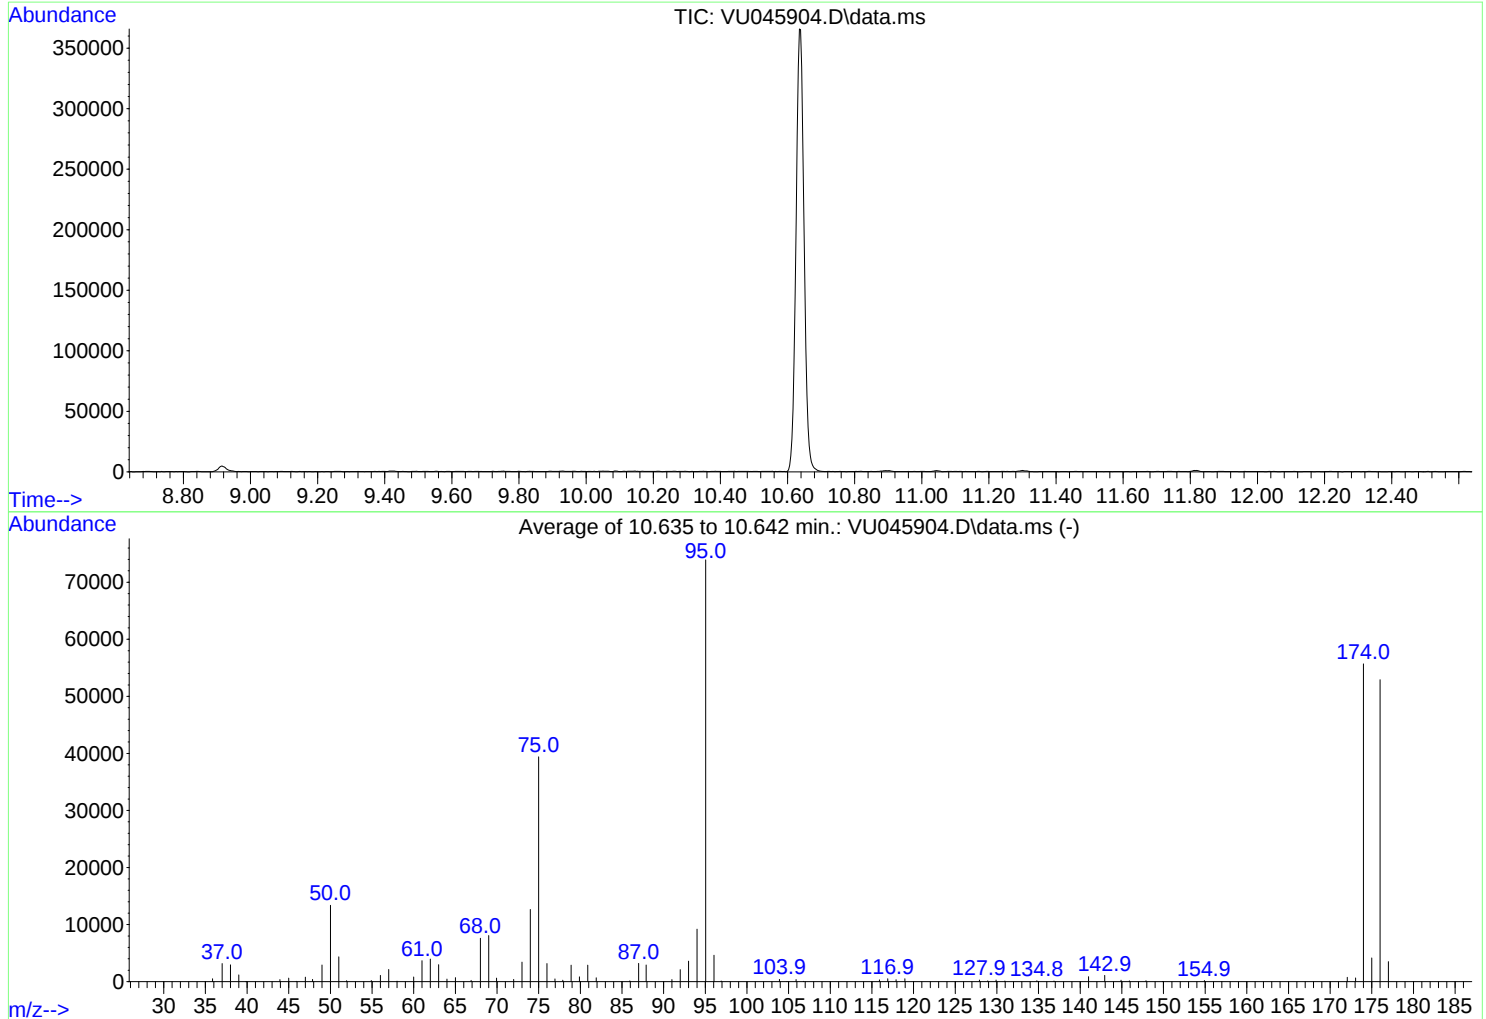

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	13384	PASS
75	95	30	60	53.3	39392	PASS
95	95	100	100	100.0	73923	PASS
96	95	5	9	6.3	4637	PASS
173	174	0.00	2	1.2	650	PASS
174	95	50	100	75.4	55701	PASS
175	174	5	9	7.4	4147	PASS
176	174	95	101	95.0	52925	PASS
177	176	5	9	6.6	3507	PASS