

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112223\
 Data File : VU056588.D
 Acq On : 22 Nov 2023 15:00
 Operator : MD/SY
 Sample : 05452-03
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU056588.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.476	49	58	77	rBV	25329	56348	5.90%	0.699%
2	1.595	87	95	106	rVB	108247	122154	12.78%	1.514%
3	1.907	183	192	209	rVB	90321	125142	13.10%	1.551%
4	2.560	383	395	414	rBV	189469	311181	32.57%	3.858%
5	3.042	533	545	559	rVB3	13937	26969	2.82%	0.334%
6	3.181	569	588	607	rBV	18468	44290	4.64%	0.549%
7	4.618	1021	1035	1062	rBV2	135056	353498	37.00%	4.383%
8	5.055	1156	1171	1192	rBV	187041	420250	43.98%	5.210%
9	5.721	1357	1378	1402	rBV2	361856	955485	100.00%	11.846%
10	6.245	1525	1541	1566	rBV	326058	640173	67.00%	7.937%
11	6.534	1621	1631	1647	rBV7	4846	11463	1.20%	0.142%
12	6.685	1663	1678	1697	rBV	232066	466091	48.78%	5.779%
13	7.563	1939	1951	1973	rBV	121287	220273	23.05%	2.731%
14	7.894	2040	2054	2083	rBV	455191	827052	86.56%	10.254%
15	8.177	2130	2142	2161	rBV2	69214	123584	12.93%	1.532%
16	8.627	2271	2282	2323	rBV	478313	916429	95.91%	11.362%
17	9.412	2513	2526	2552	rBV	444896	788537	82.53%	9.776%
18	10.753	2928	2943	2959	rBV2	160294	261617	27.38%	3.243%
19	11.807	3259	3271	3291	rBV	426605	702403	73.51%	8.708%
20	12.190	3376	3390	3411	rBV	406465	692949	72.52%	8.591%




Sum of corrected areas: 8065888

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112223\
Data File : VU056588.D
Acq On : 22 Nov 2023 15:00
Operator : MD/SY
Sample : 05452-03
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

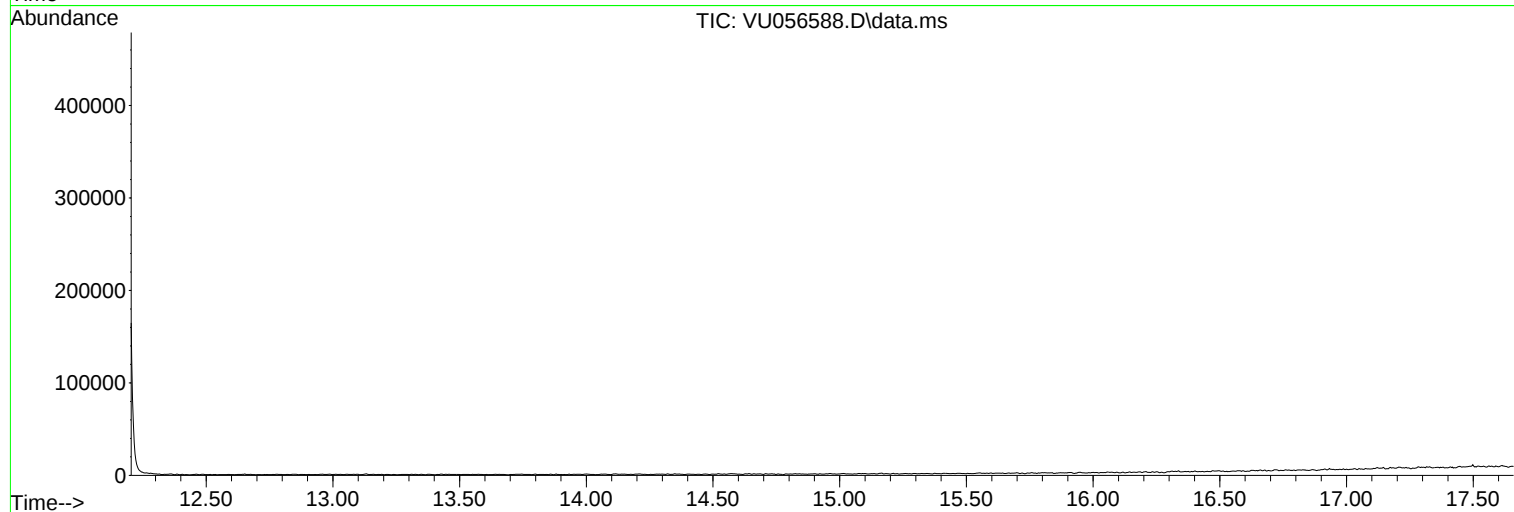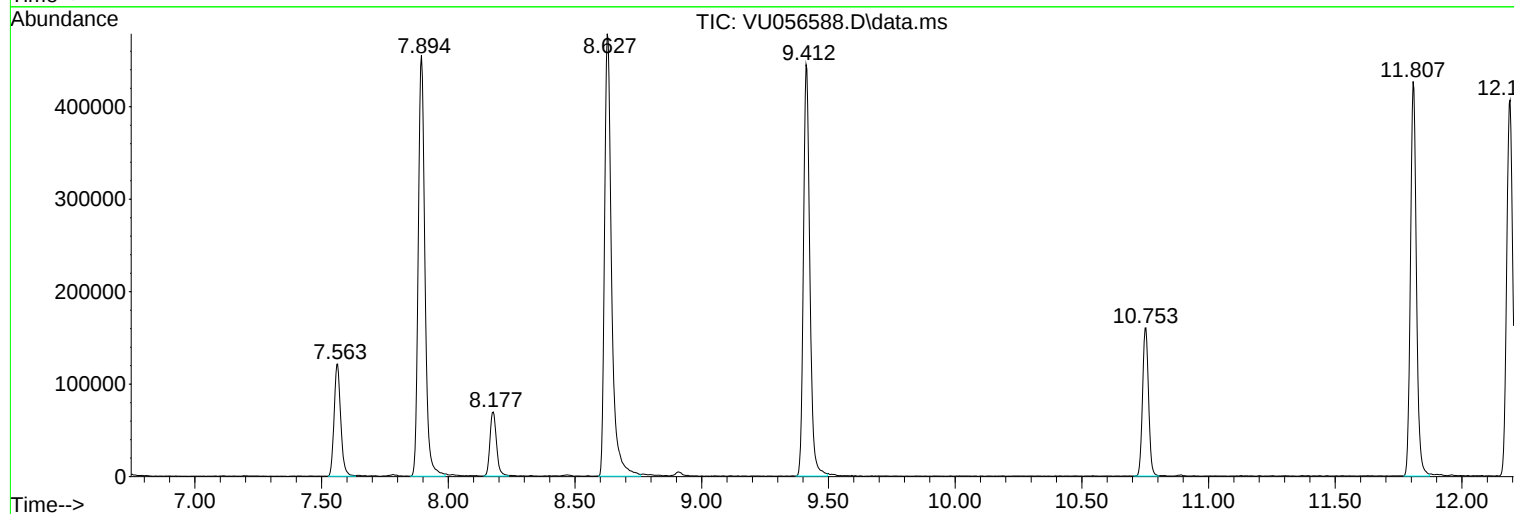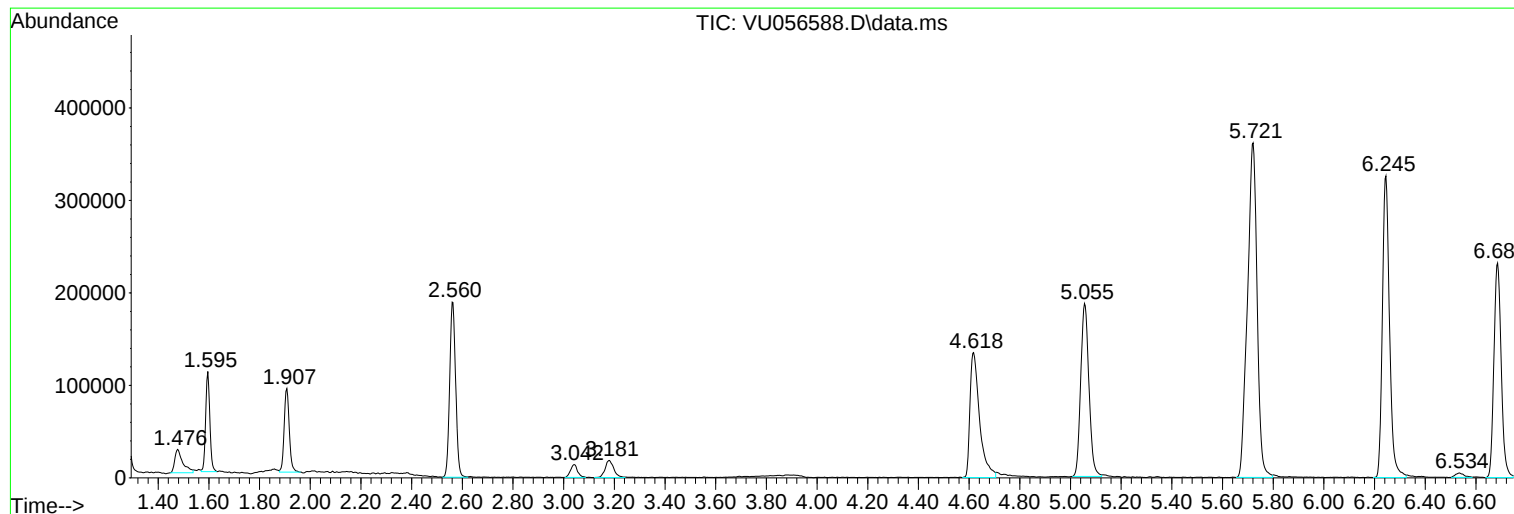

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112223\
Data File : VU056588.D
Acq On : 22 Nov 2023 15:00
Operator : MD/SY
Sample : 05452-03
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112223\
Data File : VU056588.D
Acq On : 22 Nov 2023 15:00
Operator : MD/SY
Sample : 05452-03
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc