

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112223\
 Data File : VU056595.D
 Acq On : 22 Nov 2023 17:50
 Operator : MD/SY
 Sample : 05473-06
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU056595.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.480	51	59	70	rBV	15715	30002	3.00%	0.359%
2	1.595	86	95	109	rVB	114599	137689	13.78%	1.648%
3	1.907	184	192	203	rVB	93232	123308	12.34%	1.476%
4	2.560	383	395	416	rBV	201914	330773	33.11%	3.959%
5	3.039	531	544	560	rBV2	17273	34138	3.42%	0.409%
6	3.177	574	587	604	rBV	15161	38205	3.82%	0.457%
7	4.618	1023	1035	1062	rBV2	141161	367823	36.82%	4.403%
8	5.055	1154	1171	1191	rBV	197990	446412	44.69%	5.343%
9	5.721	1355	1378	1402	rBV2	381155	998917	100.00%	11.956%
10	6.245	1526	1541	1571	rBV	345990	682330	68.31%	8.167%
11	6.534	1621	1631	1643	rBV7	4837	10747	1.08%	0.129%
12	6.685	1663	1678	1705	rBV	237789	475476	47.60%	5.691%
13	7.560	1939	1950	1971	rBV	118401	215583	21.58%	2.580%
14	7.894	2038	2054	2081	rBV	454505	824773	82.57%	9.872%
15	8.177	2130	2142	2159	rBV2	74628	128729	12.89%	1.541%
16	8.627	2271	2282	2315	rBV	500129	935635	93.66%	11.199%
17	9.415	2510	2527	2549	rBV	491590	862722	86.37%	10.326%
18	10.753	2929	2943	2961	rBV	169162	272958	27.33%	3.267%
19	11.807	3259	3271	3296	rBV	440530	733481	73.43%	8.779%
20	12.190	3376	3390	3410	rBV	416259	705009	70.58%	8.438%




Sum of corrected areas: 8354710

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112223\
Data File : VU056595.D
Acq On : 22 Nov 2023 17:50
Operator : MD/SY
Sample : 05473-06
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

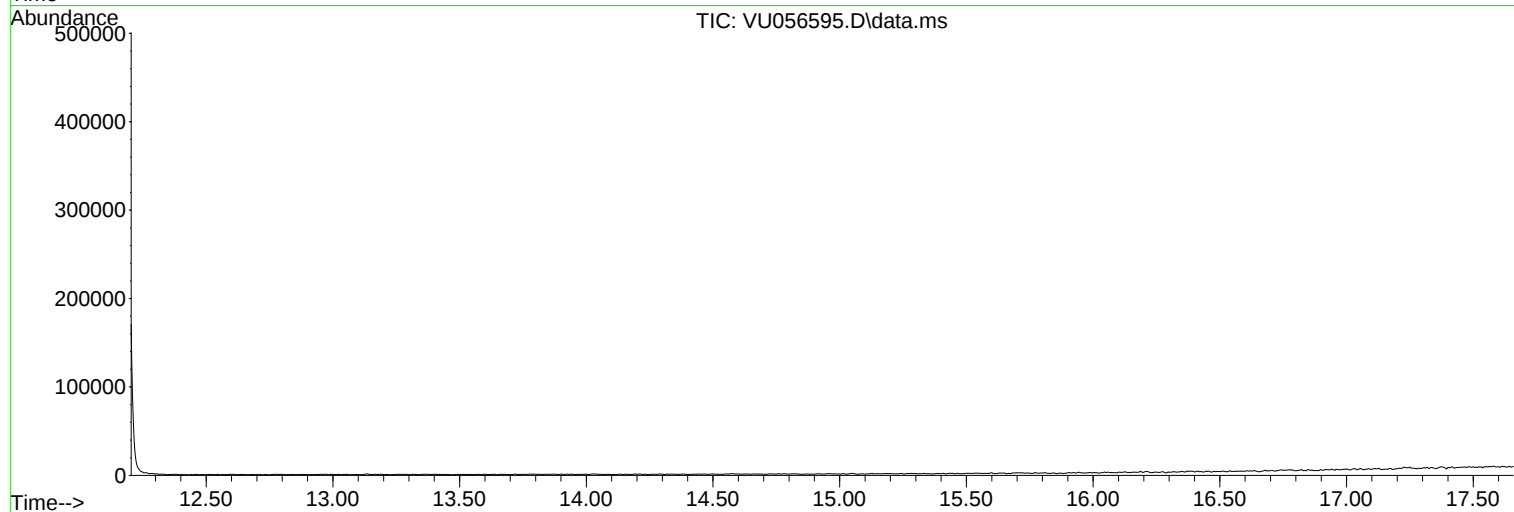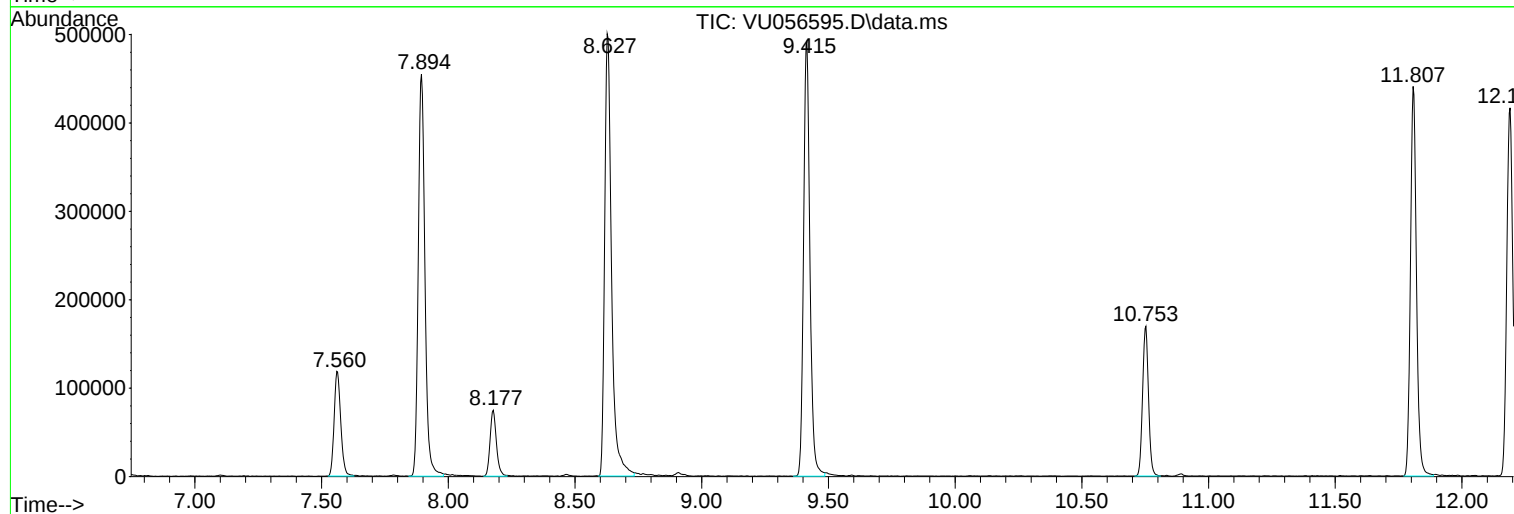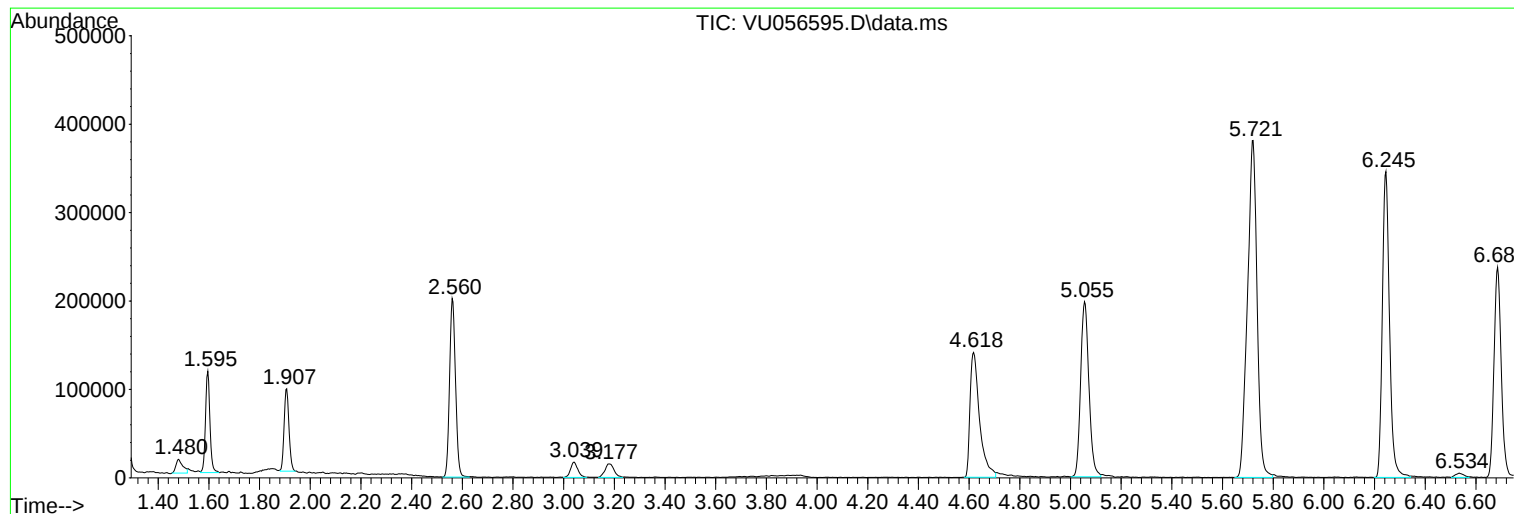

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112223\
Data File : VU056595.D
Acq On : 22 Nov 2023 17:50
Operator : MD/SY
Sample : 05473-06
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112223\
Data File : VU056595.D
Acq On : 22 Nov 2023 17:50
Operator : MD/SY
Sample : 05473-06
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc