


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU112320\
 Data File : VU041379.D
 Acq On : 23 Nov 2020 09:02
 Operator : SY/MD
 Sample : BFB17
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB17

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR112320WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Nov 24 01:52:19 2020

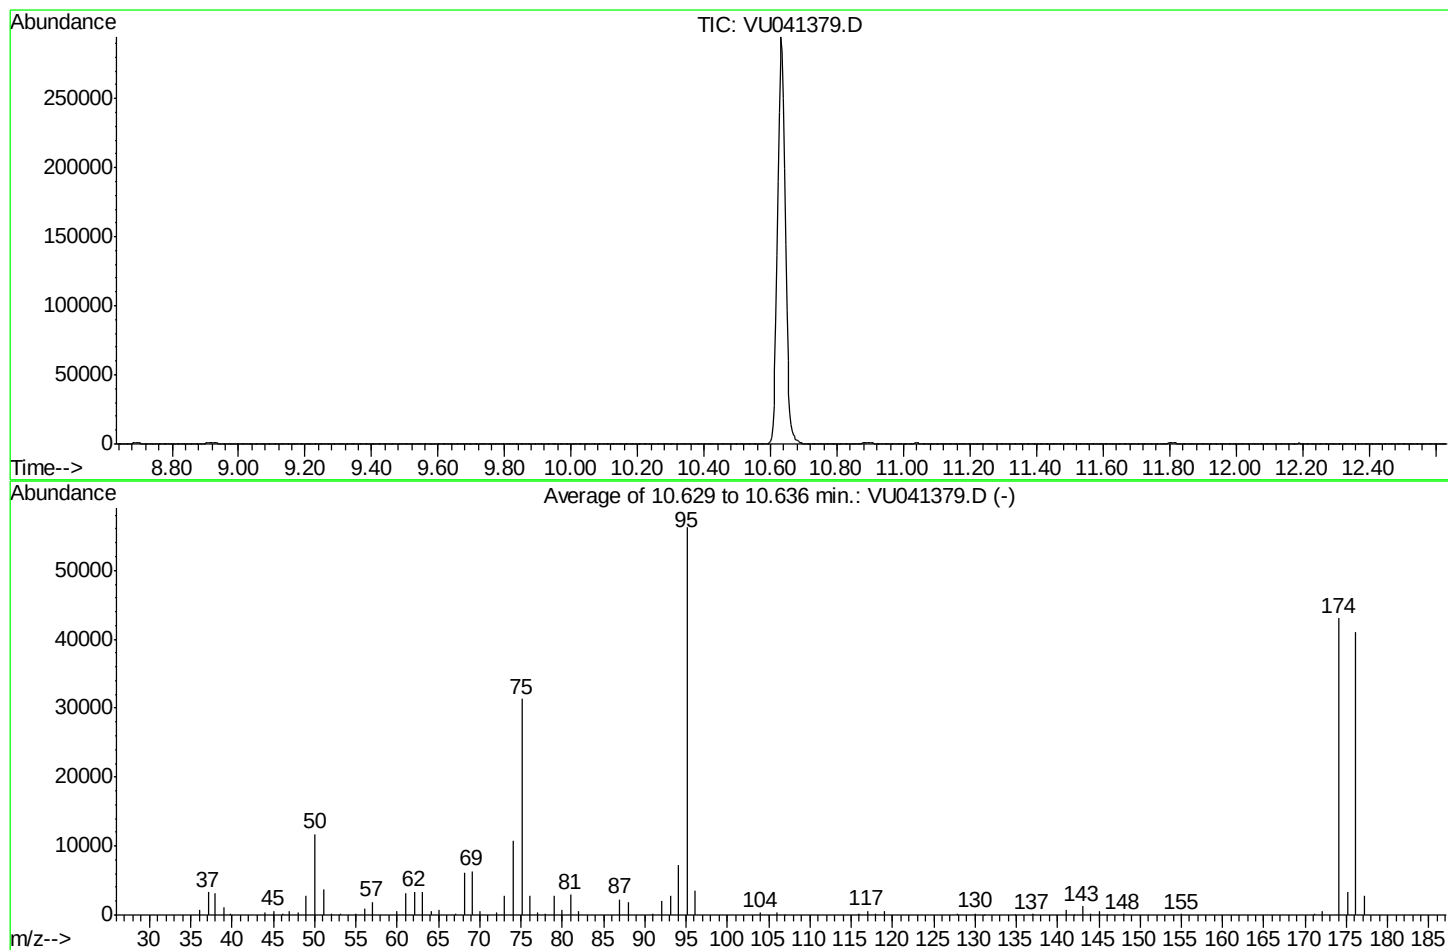

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	11729	PASS
75	95	30	80	55.7	31306	PASS
95	95	100	100	100.0	56232	PASS
96	95	5	9	6.3	3545	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.5	43042	PASS
175	174	5	9	7.7	3293	PASS
176	174	95	101	95.2	40994	PASS
177	176	5	9	6.7	2758	PASS

m/z	Abundance
36.00	626.0
37.10	3270.0
38.00	3049.0
39.00	1166.0
39.90	143.0
44.00	475.0
45.00	548.0
46.20	167.0
47.00	720.0
48.00	343.0
49.00	2675.0
50.10	11515.0
51.10	3648.0
52.00	214.0
53.10	128.0
55.00	192.0
56.00	904.0
57.00	1799.0
60.00	585.0
61.10	3109.0
62.10	3206.0
63.10	3340.0
64.10	694.0
65.10	642.0
67.10	178.0
68.10	5900.0
69.10	6249.0
70.00	566.0
72.00	339.0
73.00	2791.0
74.10	10874.0
75.10	30648.0
76.10	2690.0
77.00	335.0
78.00	272.0
79.00	2753.0
80.00	796.0
81.00	2908.0
81.90	610.0
87.00	2147.0
88.00	1954.0
91.00	288.0
92.00	1962.0
93.10	2789.0
94.10	6971.0
95.10	54888.0
96.10	3591.0
104.00	315.0
105.90	367.0
116.00	275.0
117.00	629.0
118.00	224.0
119.00	472.0
127.90	161.0
130.00	189.0
137.00	121.0
141.00	623.0
143.00	1294.0
144.00	120.0
145.00	548.0
148.00	156.0
155.10	125.0
171.20	150.0
172.10	622.0
174.10	41224.0
175.10	3248.0
176.10	39016.0
177.10	2576.0

Instrument :
MSVOA_U
ClientSampleId :
BFB17

m/z	Abundance
36.00	698.0
37.10	3414.0
38.00	3250.0
39.00	1149.0
39.80	155.0
44.00	456.0
45.00	613.0
46.10	209.0
47.00	675.0
48.00	335.0
49.00	2807.0
50.10	12152.0
51.10	3825.0
52.00	195.0
53.10	133.0
55.00	192.0
56.00	945.0
57.00	1950.0
60.00	629.0
61.10	3376.0
62.10	3423.0
63.10	3394.0
64.10	648.0
65.10	702.0
67.10	164.0
68.10	6267.0
69.10	6551.0
70.00	576.0
72.00	367.0
73.00	2913.0
74.10	11157.0
75.10	32312.0
76.10	2836.0
77.00	290.0
79.00	2902.0
80.00	816.0
81.00	3000.0
81.90	592.0
87.00	2315.0
88.00	1966.0
91.00	279.0
92.00	2070.0
93.10	2956.0
94.10	7371.0
95.10	57792.0
96.10	3689.0
104.00	349.0
105.90	339.0
116.00	290.0
116.90	666.0
118.00	249.0
118.90	499.0
127.90	180.0
130.10	203.0
131.10	104.0
137.00	132.0
141.00	703.0
142.00	114.0
143.00	1341.0
144.00	128.0
145.00	545.0
146.00	103.0
148.00	186.0
155.00	161.0
171.20	181.0
172.10	634.0
174.10	44368.0
175.10	3378.0
176.10	42360.0
177.10	2827.0

Instrument :
MSVOA_U
ClientSampleId :
BFB17

m/z	Abundance
36.00	644.0
37.10	3188.0
38.00	3040.0
39.00	1071.0
39.80	127.0
44.10	446.0
45.00	573.0
46.10	188.0
47.00	558.0
47.90	336.0
49.00	2721.0
50.10	11522.0
51.10	3675.0
52.00	140.0
53.10	121.0
55.10	170.0
56.00	914.0
57.00	1866.0
60.00	666.0
61.10	3244.0
62.10	3412.0
63.10	3139.0
64.10	531.0
65.00	711.0
67.10	147.0
68.10	6103.0
69.10	6321.0
70.00	551.0
72.00	346.0
73.00	2767.0
74.10	10404.0
75.10	30960.0
76.10	2673.0
77.00	276.0
77.90	180.0
78.90	2820.0
80.00	783.0
81.00	2910.0
82.00	555.0
87.00	2304.0
88.00	1817.0
91.00	262.0
92.10	2000.0
93.10	2847.0
94.10	7167.0
95.10	56016.0
96.10	3355.0
104.00	363.0
106.00	304.0
106.90	100.0
116.00	290.0
117.00	608.0
118.00	269.0
118.90	506.0
127.90	189.0
130.10	194.0
131.10	136.0
134.80	105.0
137.00	108.0
141.10	730.0
141.90	127.0
143.00	1197.0
144.00	108.0
145.00	451.0
148.00	170.0
155.00	198.0
171.10	178.0
172.10	637.0
174.10	43536.0
175.10	3255.0
176.10	41608.0
177.10	2871.0

Instrument :
MSVOA_U
ClientSampleId :
BFB17

m/z	Abundance
44.00	129.0

Instrument :
MSVOA_U
ClientSampleId :
BFB17