

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112321\
 Data File : VU045968.D
 Acq On : 23 Nov 2021 20:06
 Operator : SY/MD
 Sample : M4722-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Nov 24 00:34:38 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 24 00:27:16 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	91246	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	92668	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	50214	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	17297	2.393	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	47.800%
7) Chloroethane-d5	1.919	69	26418	5.020	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.400%
11) 1,1-Dichloroethene-d2	2.575	65	12050	3.974	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	79.400%
20) 2-Butanone-d5	4.652	46	126169	65.124	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	130.240%#
24) Chloroform-d	5.067	84	66106	5.489	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	109.800%
26) 1,2-Dichloroethane-d4	5.710	65	37376	5.289	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.800%
32) Benzene-d6	5.735	84	133904	5.247	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.000%
36) 1,2-Dichloropropane-d6	6.694	67	41482	5.158	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.200%
41) Toluene-d8	7.899	98	121865	5.279	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.600%
43) trans-1,3-Dichloroprop...	8.179	79	16114	4.935	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	98.800%
46) 2-Hexanone-d5	8.636	63	113328	77.117	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	154.240%#
56) 1,1,2,2-Tetrachloroeth...	10.758	84	41075	6.045	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	121.000%#
66) 1,2-Dichlorobenzene-d4	12.195	152	48373	5.611	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	112.200%
Target Compounds						
					Qvalue	
3) Chloromethane	1.520	50	2097	0.266	ug/L	99
8) Chloroethane	2.002	64	789	0.175	ug/L #	1
13) Acetone	2.604	43	31746	27.840	ug/L	49
14) Carbon disulfide	2.803	76	8591	0.481	ug/L	96
15) Methyl Acetate	3.051	43	256213	91.575	ug/L #	51
21) 2-Butanone	4.652	43	3343	1.742	ug/L #	64
22) cis-1,2-Dichloroethene	4.674	96	7405	1.128	ug/L	96
25) Chloroform	5.131	83	36688	2.981	ug/L #	31
27) 1,2-Dichloroethane	5.787	62	159900	20.365	ug/L #	82
30) Cyclohexane	5.395	56	427598	42.821	ug/L	98
33) Benzene	5.787	78	17996953	695.950	ug/L	100
34) Trichloroethene	6.549	95	4298	0.645	ug/L	90
35) Methylcyclohexane	6.768	83	223345	21.823	ug/L	89
37) 1,2-Dichloropropane	6.768	63	2798	0.411	ug/L #	82
38) Bromodichloromethane	7.160	83	29344	3.495	ug/L #	26
39) cis-1,3-Dichloropropene	7.568	75	966	0.100	ug/L #	1
42) Toluene	7.970	91	1294573	48.498	ug/L	100
45) 1,1,2-Trichloroethane	8.372	97	33012	6.534	ug/L #	19
47) Tetrachloroethene	8.555	164	9849	2.111	ug/L	93

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112321\
 Data File : VU045968.D
 Acq On : 23 Nov 2021 20:06
 Operator : SY/MD
 Sample : M4722-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :


Quant Time: Nov 24 00:34:38 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 24 00:27:16 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

49) Dibromochloromethane	8.555	129	9244	1.606	ug/L #	10
50) 1,2-Dibromoethane	8.925	107	7267	1.527	ug/L #	76
51) Chlorobenzene	9.665	112	12482	0.745	ug/L #	50
52) Ethylbenzene	9.575	91	6305014	225.661	ug/L	99
53) m,p-Xylene	9.697	106	282700	26.414	ug/L	95
54) o-Xylene	10.102	106	30233	2.927	ug/L	96
55) Styrene	10.105	104	3182	0.183	ug/L #	1
57) 1,1,2,2-Tetrachloroethane	10.793	83	591	0.091	ug/L #	82
60) Isopropylbenzene	10.484	105	396228	13.441	ug/L	99
61) 1,2,3-Trichloropropane	10.906	75	8202	1.573	ug/L #	1
62) 1,3,5-Trimethylbenzene	11.468	105	141371	5.865	ug/L	95
63) 1,2,4-Trimethylbenzene	11.468	105	141371	5.854	ug/L	99
67) 1,2-Dichlorobenzene	12.214	146	1196	0.091	ug/L #	55
68) 1,2-Dibromo-3-chloropr...	12.973	75	3637	3.354	ug/L #	7
71) Naphthalene	14.086	128	1092035	61.058	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Nov 24 00:34:38 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 24 00:27:16 2021
Response via : Initial Calibration







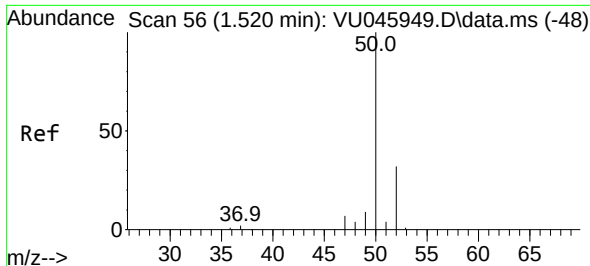

#3
Chloromethane
Concen: 0.266 ug/L
RT: 1.520 min Scan# 50
Delta R.T. 0.000 min
Lab File: VU045968.D
Acq: 23 Nov 2021 20:06




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 50 Resp: 2097
Ion Ratio Lower Upper
50 100
52 32.2 23.0 42.8

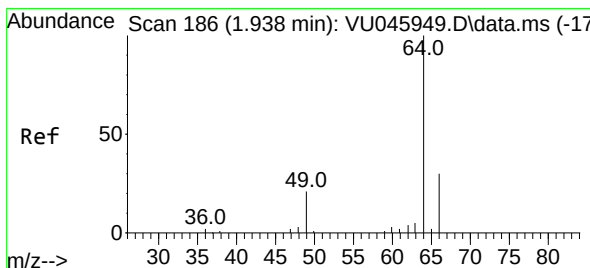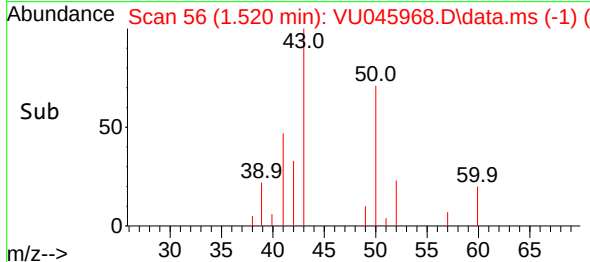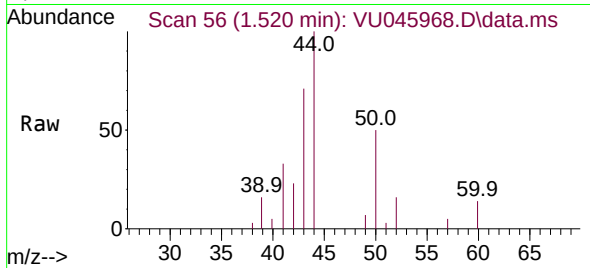

#8
Chloroethane
Concen: 0.175 ug/L
RT: 2.002 min Scan# 206
Delta R.T. 0.064 min
Lab File: VU045968.D
Acq: 23 Nov 2021 20:06

Tgt Ion: 64 Resp: 789
Ion Ratio Lower Upper
64 100
66 118.8 22.1 41.1#

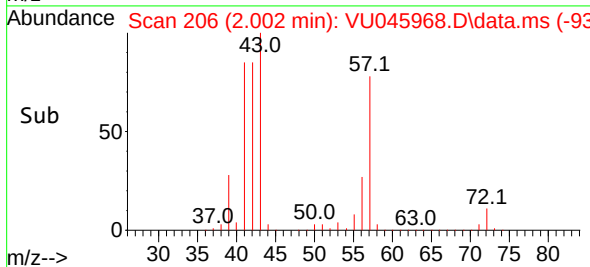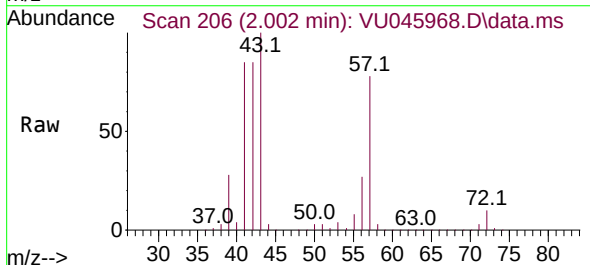



#13

Acetone

Concen: 27.840 ug/L

RT: 2.604 min Scan# 393

Delta R.T. -0.077 min

Lab File: VU045968.D

Acq: 23 Nov 2021 20:06

Instrument :

MSVOA_U





ClientSampleId :

Tgt Ion: 43 Resp: 31746

Ion Ratio Lower Upper

43 100

58 6.0 0.0 71.6

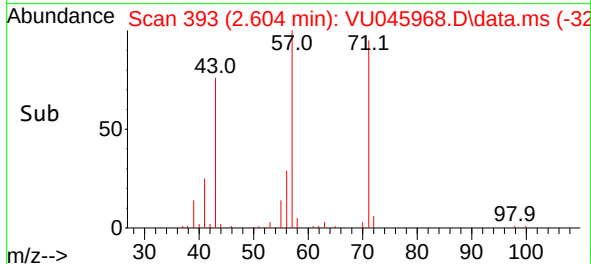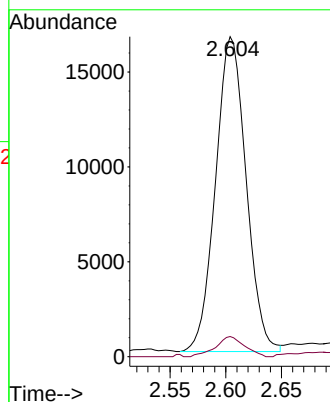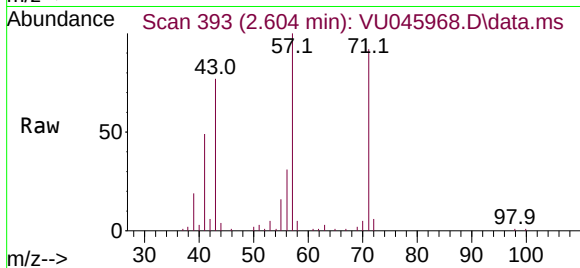

#14

Carbon disulfide

Concen: 0.481 ug/L

RT: 2.803 min Scan# 455

Delta R.T. 0.003 min

Lab File: VU045968.D




Acq: 23 Nov 2021 20:06


Tgt Ion: 76 Resp: 8591

Ion Ratio Lower Upper

76 100

78 10.7 7.5 11.3


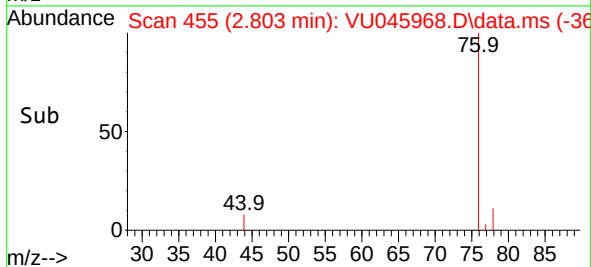
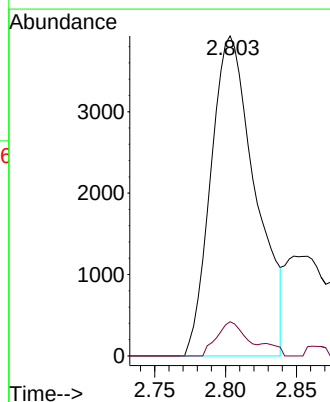
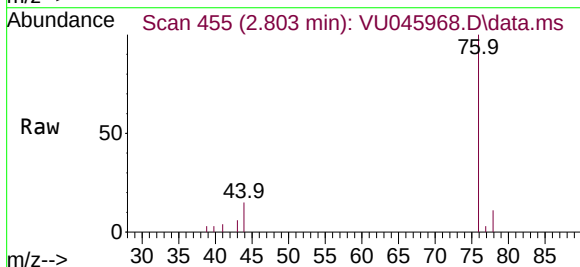




#15
Methyl Acetate
Concen: 91.575 ug/L
RT: 3.051 min Scan# 51
Delta R.T. 0.084 min
Lab File: VU045968.D
Acq: 23 Nov 2021 20:06




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 43 Resp: 256213
Ion Ratio Lower Upper
43 100
74 0.0 19.1 28.7#

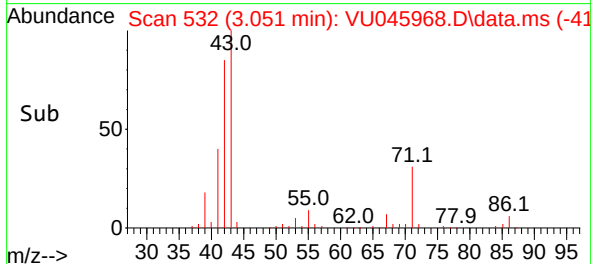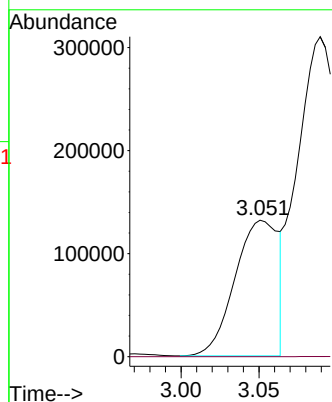

#21
2-Butanone
Concen: 1.742 ug/L
RT: 4.652 min Scan# 1030
Delta R.T. -0.080 min
Lab File: VU045968.D
Acq: 23 Nov 2021 20:06

Tgt Ion: 43 Resp: 3343
Ion Ratio Lower Upper
43 100
72 9.1 14.1 42.3#

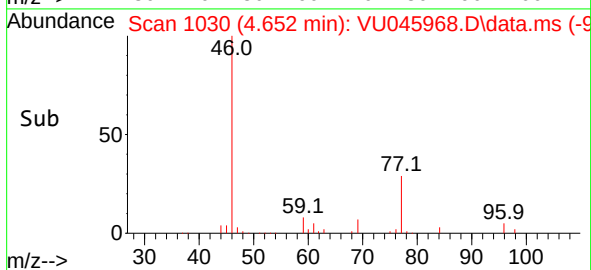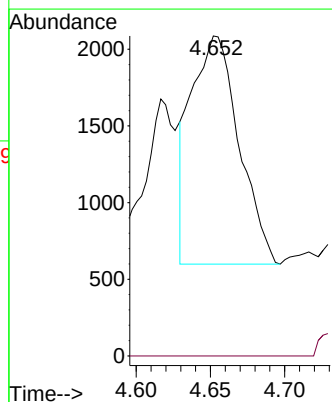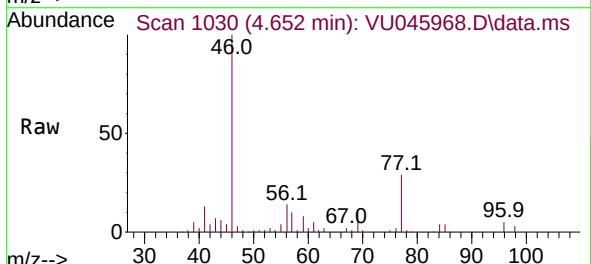

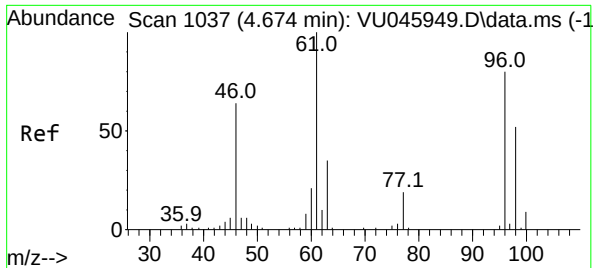

#22

cis-1,2-Dichloroethene

Concen: 1.128 ug/L

RT: 4.674 min Scan# 1107

Delta R.T. 0.000 min

Lab File: VU045968.D

Acq: 23 Nov 2021 20:06

Instrument :

MSVOA_U

ClientSampleId :





Tgt Ion: 96 Resp: 7405

Ion Ratio Lower Upper

96 100

61 127.0 88.5 164.3

98 71.7 44.4 82.5

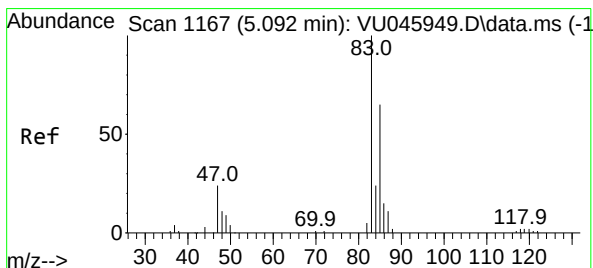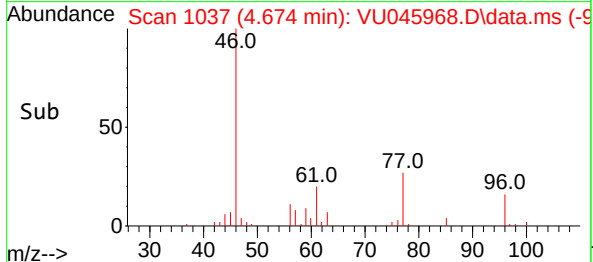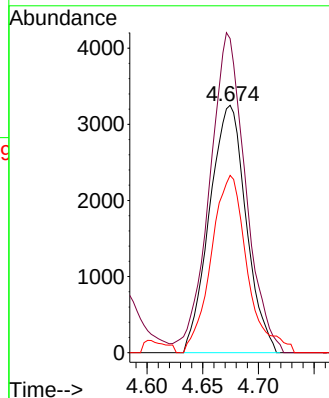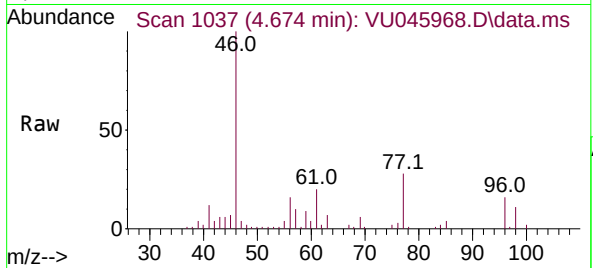

#25

Chloroform

Concen: 2.981 ug/L

RT: 5.131 min Scan# 1179

Delta R.T. 0.039 min

Lab File: VU045968.D




Acq: 23 Nov 2021 20:06


Tgt Ion: 83 Resp: 36688

Ion Ratio Lower Upper

83 100

85 11.7 46.9 87.1#


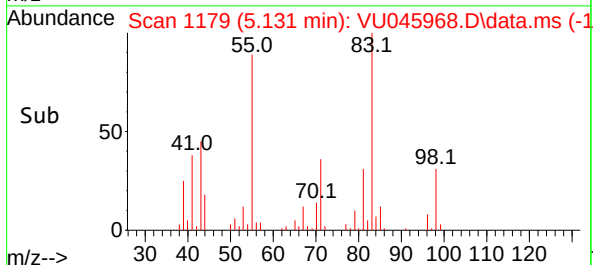
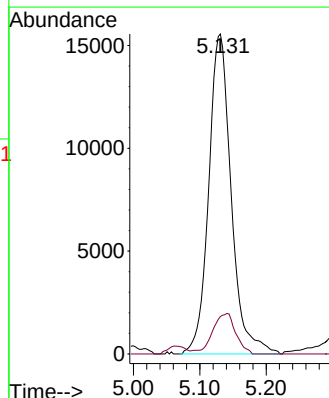
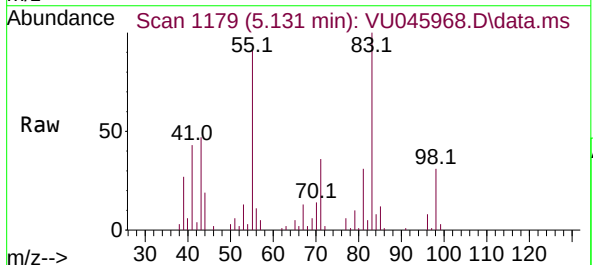


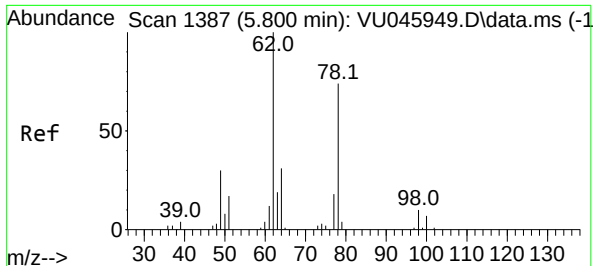

#27
1,2-Dichloroethane
Concen: 20.365 ug/L
RT: 5.787 min Scan# 11
Delta R.T. -0.013 min
Lab File: VU045968.D
Acq: 23 Nov 2021 20:06




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 62 Resp: 159900
Ion Ratio Lower Upper
62 100
98 3.0 7.8 11.8#

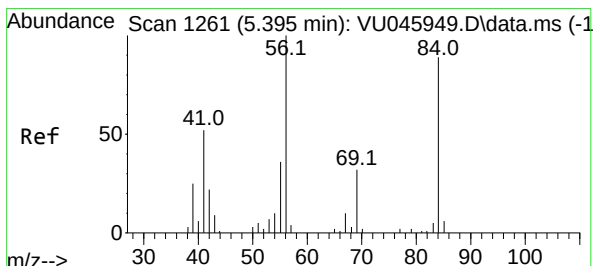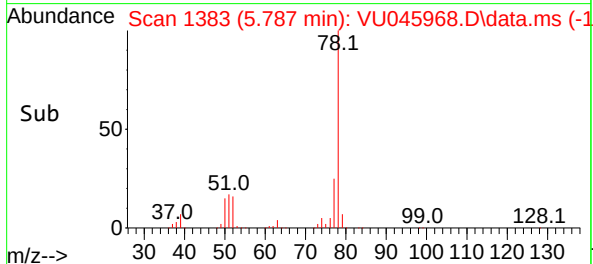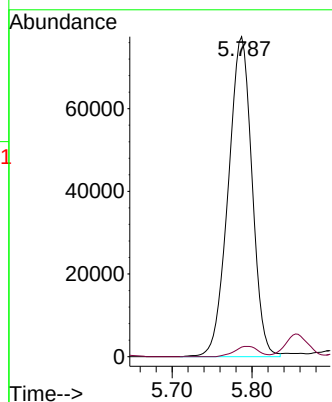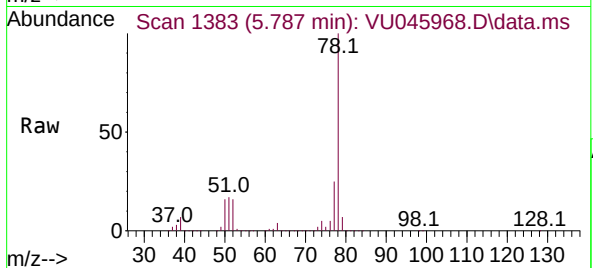

#30
Cyclohexane
Concen: 42.821 ug/L
RT: 5.395 min Scan# 1261
Delta R.T. 0.000 min
Lab File: VU045968.D
Acq: 23 Nov 2021 20:06

Tgt Ion: 56 Resp: 427598
Ion Ratio Lower Upper
56 100
69 32.2 24.7 37.1
84 88.1 71.8 107.6


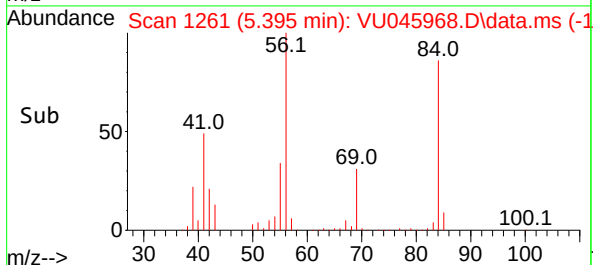
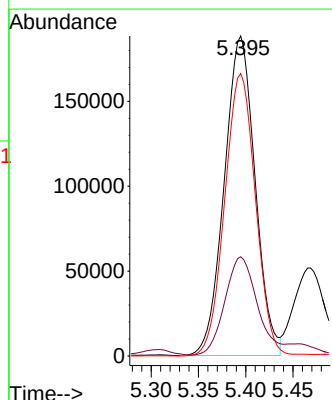
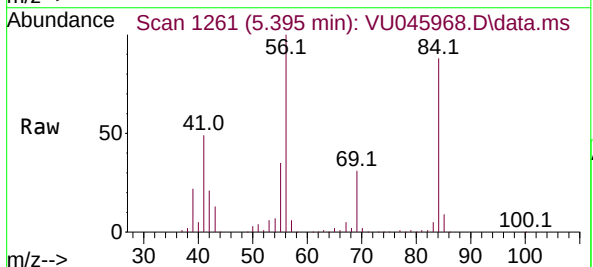


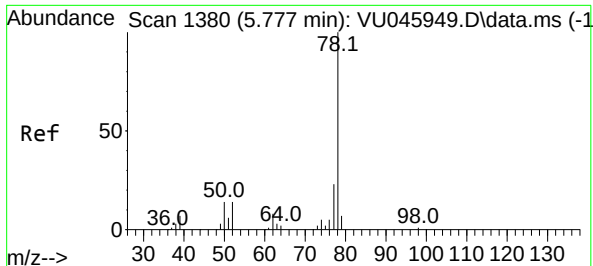

#33
Benzene
Concen: 695.950 ug/L
RT: 5.787 min Scan# 11
Delta R.T. 0.010 min
Lab File: VU045968.D
Acq: 23 Nov 2021 20:06




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 78 Resp:17996953

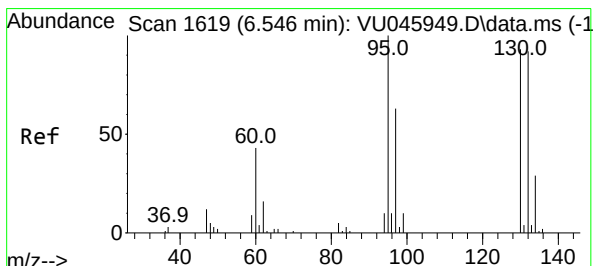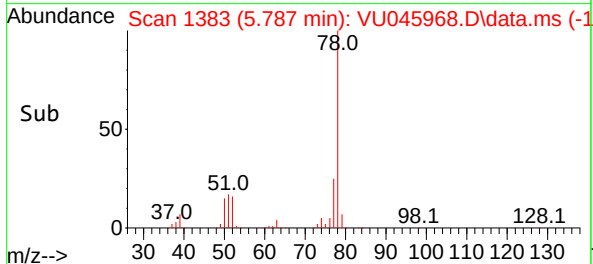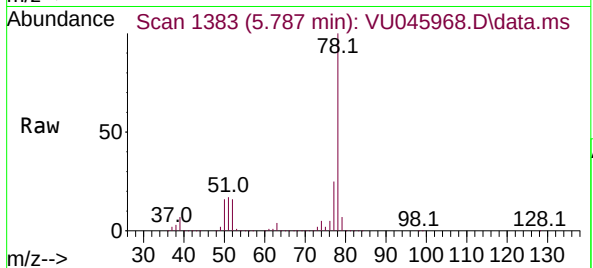

#34
Trichloroethene
Concen: 0.645 ug/L
RT: 6.549 min Scan# 1620
Delta R.T. 0.003 min
Lab File: VU045968.D
Acq: 23 Nov 2021 20:06

Tgt Ion: 95 Resp: 4298
Ion Ratio Lower Upper
95 100
97 68.3 46.5 86.5
132 82.7 65.1 120.9
130 81.5 67.3 124.9

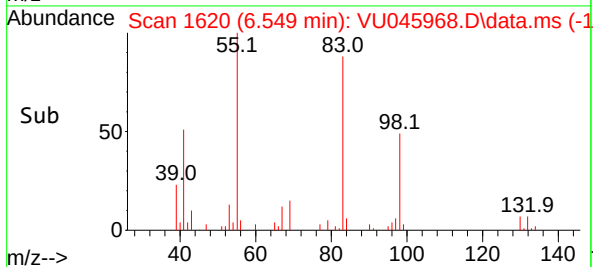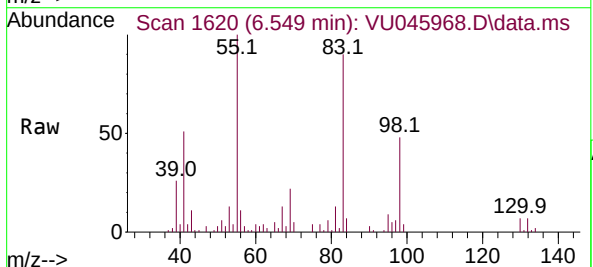

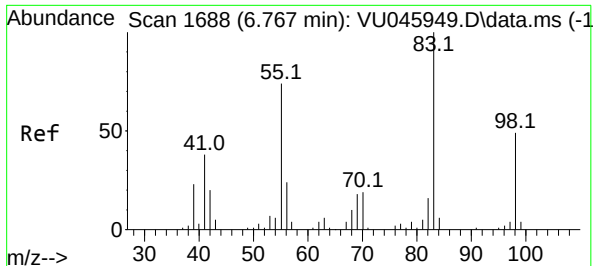

#35

Methylcyclohexane

Concen: 21.823 ug/L

RT: 6.768 min Scan# 1

Delta R.T. 0.000 min

Lab File: VU045968.D

Acq: 23 Nov 2021 20:06

Instrument :

MSVOA_U

ClientSampleId :





Tgt Ion: 83 Resp: 223345

Ion Ratio Lower Upper

83 100

55 92.8 61.9 92.9

98 49.4 39.0 58.6

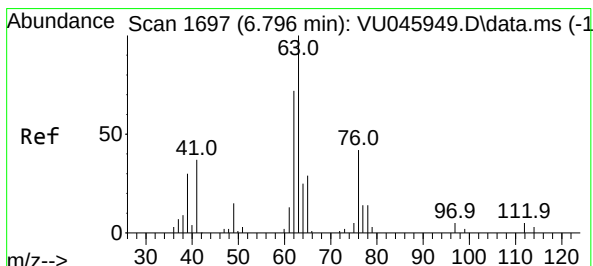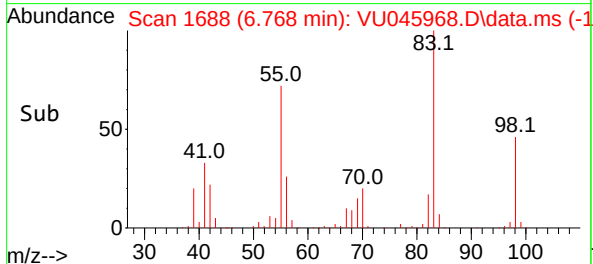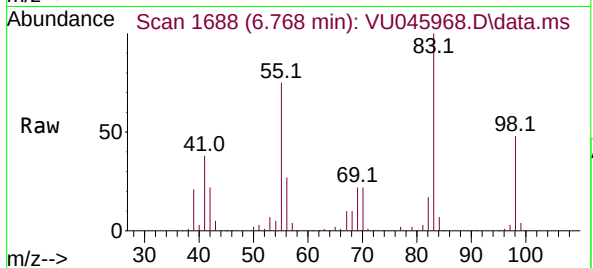

#37

1,2-Dichloropropane

Concen: 0.411 ug/L

RT: 6.768 min Scan# 1688

Delta R.T. -0.029 min

Lab File: VU045968.D




Acq: 23 Nov 2021 20:06


Tgt Ion: 63 Resp: 2798

Ion Ratio Lower Upper

63 100

112 10.0 3.2 4.8#

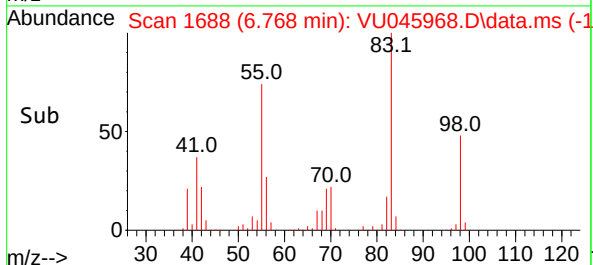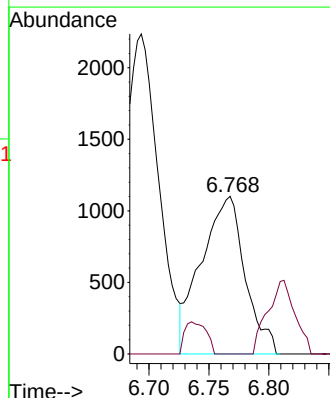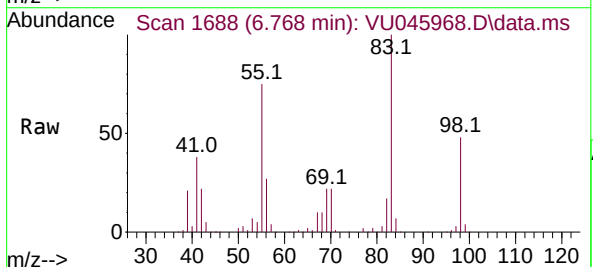

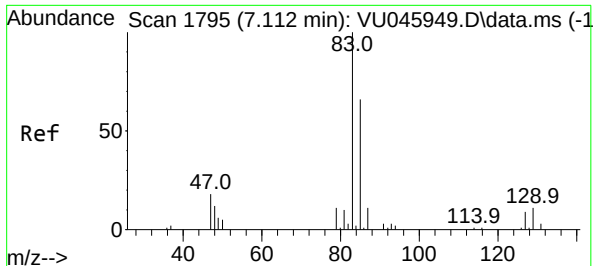

#38

Bromodichloromethane

Concen: 3.495 ug/L

RT: 7.160 min Scan# 11

Delta R.T. 0.048 min

Lab File: VU045968.D

Acq: 23 Nov 2021 20:06

Instrument :

MSVOA_U

ClientSampleId :





Tgt Ion: 83 Resp: 29344

Ion Ratio Lower Upper

83 100

85 0.7 44.0 81.8#

127 0.0 6.3 9.5#

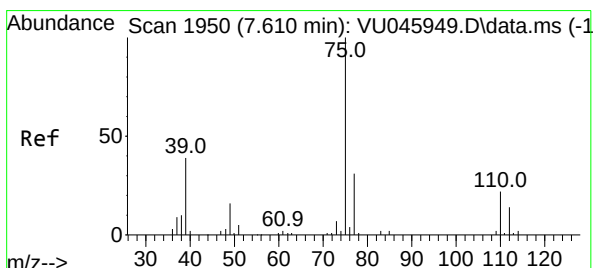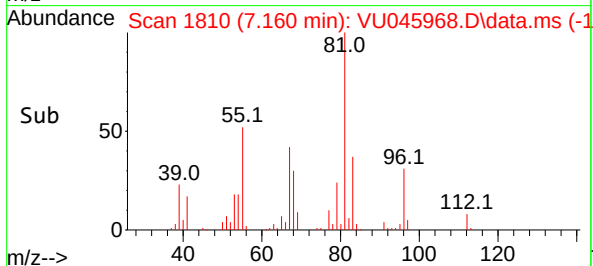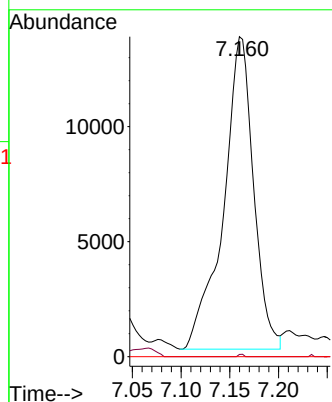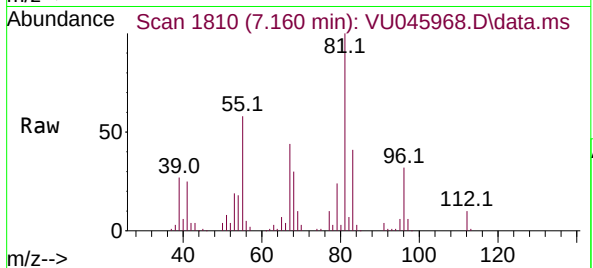

#39

cis-1,3-Dichloropropene

Concen: 0.100 ug/L

RT: 7.568 min Scan# 1937

Delta R.T. -0.042 min

Lab File: VU045968.D




Acq: 23 Nov 2021 20:06


Tgt Ion: 75 Resp: 966

Ion Ratio Lower Upper

75 100

77 147.5 22.5 41.9#

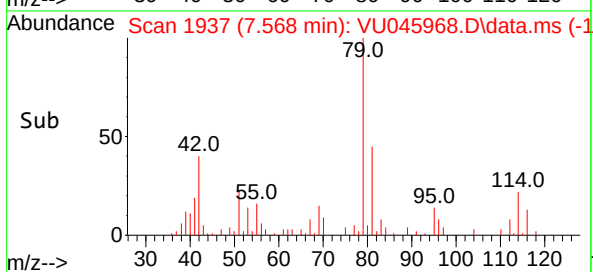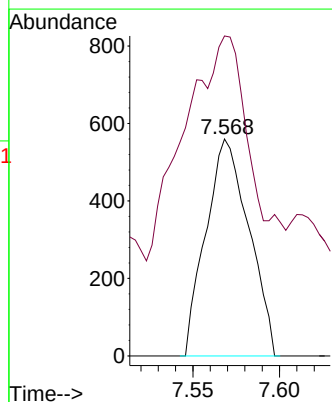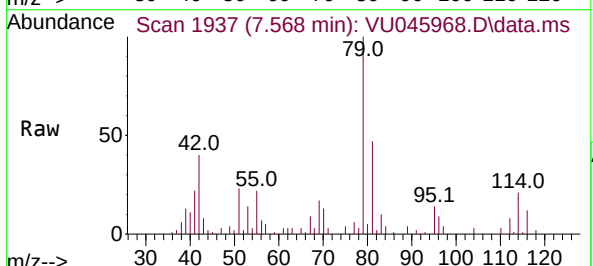



#42

Toluene

Concen: 48.498 ug/L

RT: 7.970 min Scan# 2063

Delta R.T. -0.003 min

Lab File: VU045968.D

Acq: 23 Nov 2021 20:06

Instrument :

MSVOA_U





ClientSampleId :

Tgt Ion: 91 Resp: 1294573

Ion Ratio Lower Upper

91 100

92 59.3 41.3 76.7

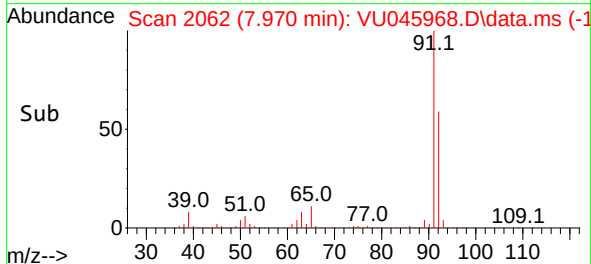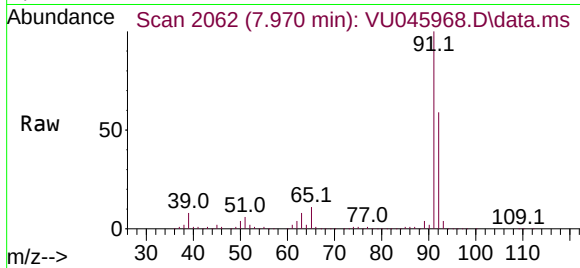

#45

1,1,2-Trichloroethane

Concen: 6.534 ug/L

RT: 8.372 min Scan# 2187

Delta R.T. -0.032 min

Lab File: VU045968.D

Acq: 23 Nov 2021 20:06

Tgt Ion: 97 Resp: 33012




Ion Ratio Lower Upper


97 100

99 0.0 42.3 78.5#

83 9.3 62.0 115.2#

85 0.0 40.1 74.5#

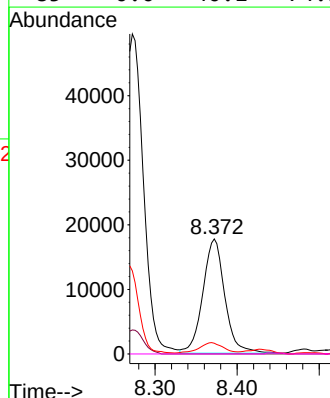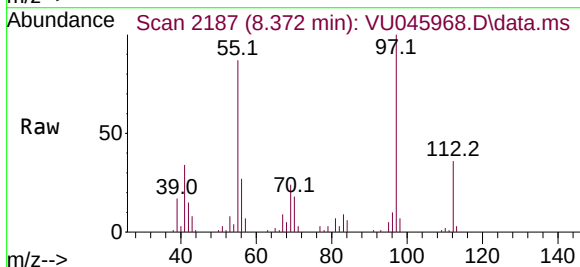



#47

Tetrachloroethene

Concen: 2.111 ug/L

RT: 8.555 min Scan# 2244

Delta R.T. 0.000 min


Lab File: VU045968.D

Acq: 23 Nov 2021 20:06

Instrument :

MSVOA_U

ClientSampleId :



Tgt Ion:164 Resp: 9849




Ion Ratio Lower Upper

164 100

129 88.7 71.8 133.4

131 96.3 68.5 127.3

166 126.8 94.1 174.8

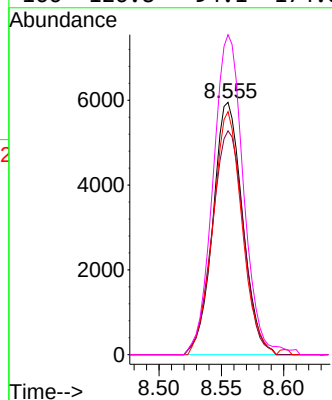

#49

Dibromochloromethane

Concen: 1.606 ug/L

RT: 8.555 min Scan# 2244

Delta R.T. -0.257 min

Lab File: VU045968.D




Acq: 23 Nov 2021 20:06


Tgt Ion:129 Resp: 9244

Ion Ratio Lower Upper

129 100

127 0.0 55.4 102.8#


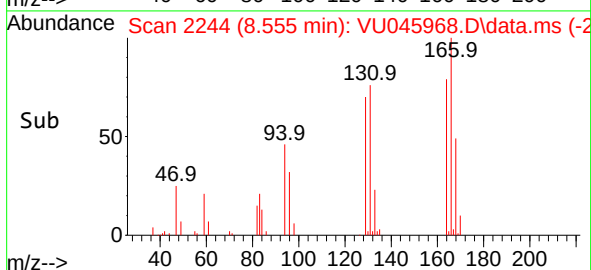
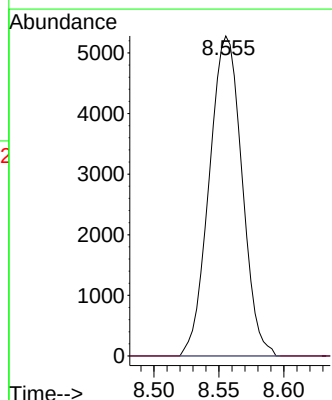





#50
1,2-Dibromoethane
Concen: 1.527 ug/L
RT: 8.925 min Scan# 21
Delta R.T. -0.003 min
Lab File: VU045968.D
Acq: 23 Nov 2021 20:06




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion:107 Resp: 7267
Ion Ratio Lower Upper
107 100
109 114.7 64.0 119.0
188 4.6 2.4 3.6#

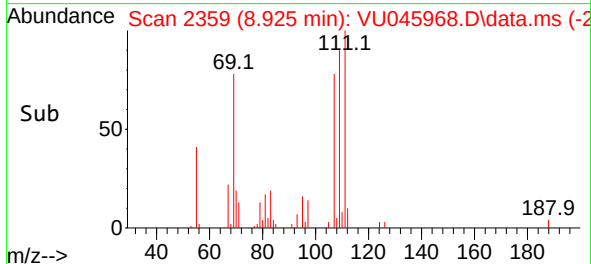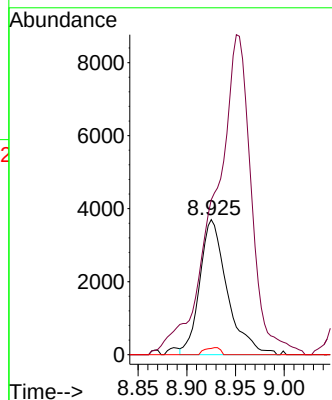

#51
Chlorobenzene
Concen: 0.745 ug/L
RT: 9.665 min Scan# 2589
Delta R.T. 0.216 min
Lab File: VU045968.D
Acq: 23 Nov 2021 20:06

Tgt Ion:112 Resp: 12482
Ion Ratio Lower Upper
112 100
114 5.7 22.1 41.1#
77 21.2 48.3 72.5#


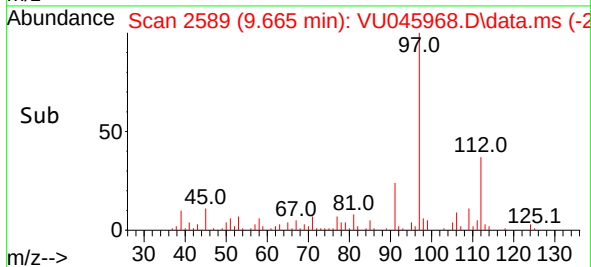
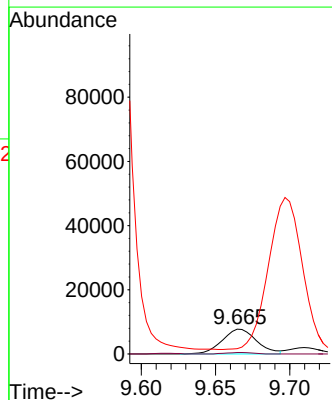
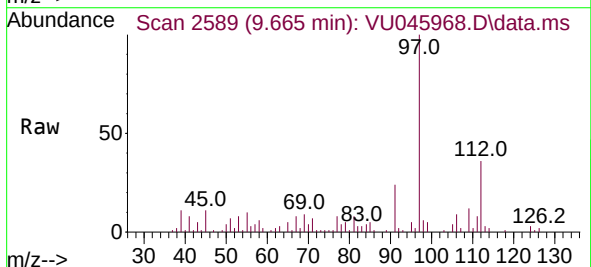




#52
Ethylbenzene
Concen: 225.661 ug/L
RT: 9.575 min Scan# 2561
Delta R.T. 0.000 min
Lab File: VU045968.D
Acq: 23 Nov 2021 20:06




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 91 Resp: 6305014
Ion Ratio Lower Upper
91 100
106 30.4 21.5 39.9

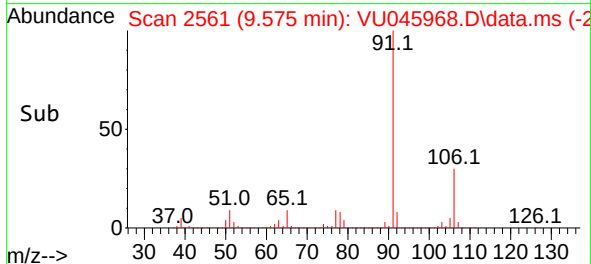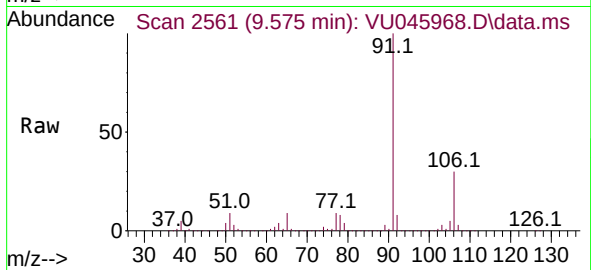

#53
m,p-Xylene
Concen: 26.414 ug/L
RT: 9.697 min Scan# 2599
Delta R.T. 0.000 min
Lab File: VU045968.D
Acq: 23 Nov 2021 20:06

Tgt Ion:106 Resp: 282700
Ion Ratio Lower Upper
106 100
91 207.1 139.4 259.0




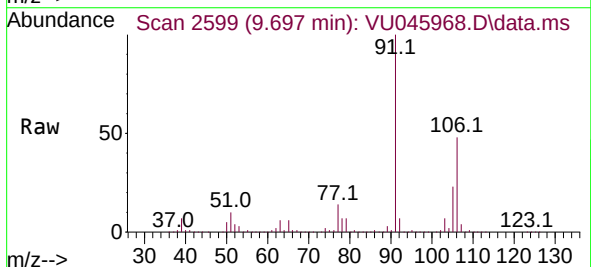


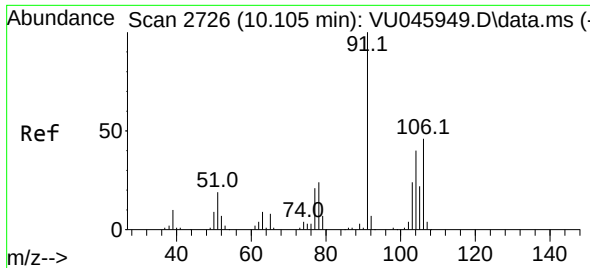

#54
o-Xylene
Concen: 2.927 ug/L
RT: 10.102 min Scan# 2725
Delta R.T. -0.003 min
Lab File: VU045968.D
Acq: 23 Nov 2021 20:06




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion:106 Resp: 30233
Ion Ratio Lower Upper
106 100
91 217.1 147.5 273.9

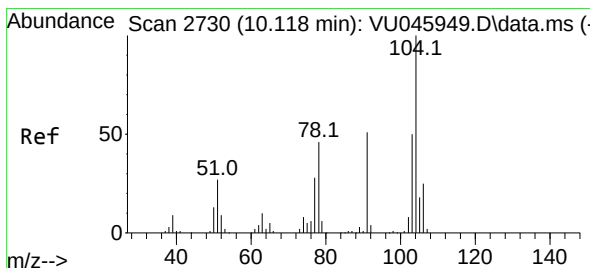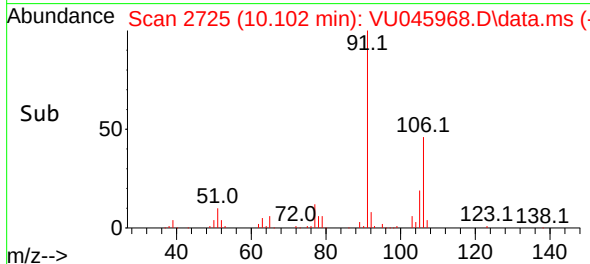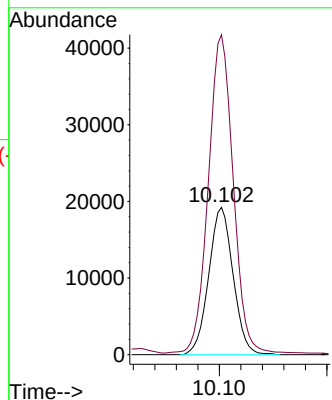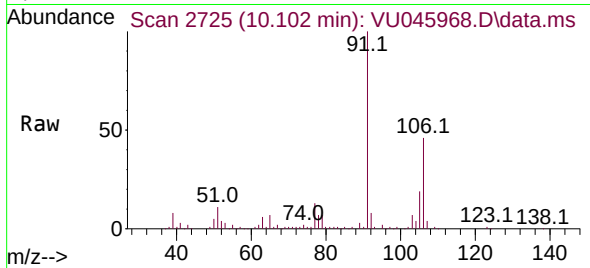

#55
Styrene
Concen: 0.183 ug/L
RT: 10.105 min Scan# 2726
Delta R.T. -0.013 min
Lab File: VU045968.D
Acq: 23 Nov 2021 20:06

Tgt Ion:104 Resp: 3182
Ion Ratio Lower Upper
104 100
78 160.8 33.0 61.4#

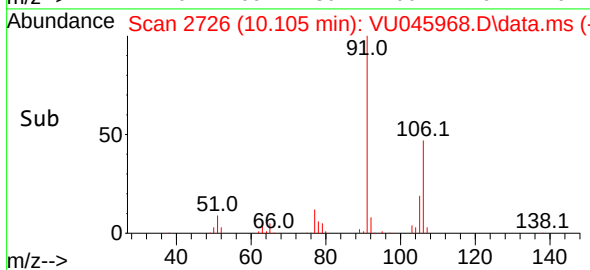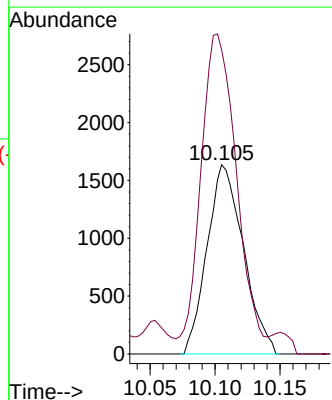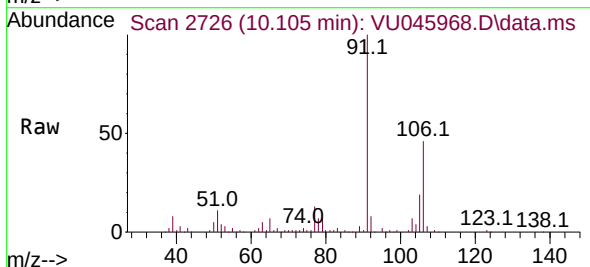



#57

1,1,2,2-Tetrachloroethane

Concen: 0.091 ug/L

RT: 10.793 min Scan# 2938

Delta R.T. 0.007 min

Lab File: VU045968.D

Acq: 23 Nov 2021 20:06

Instrument :

MSVOA_U

ClientSampleId :





Tgt Ion: 83 Resp: 591

Ion Ratio Lower Upper

83 100

85 55.4 47.9 89.1

131 0.0 8.1 12.1#

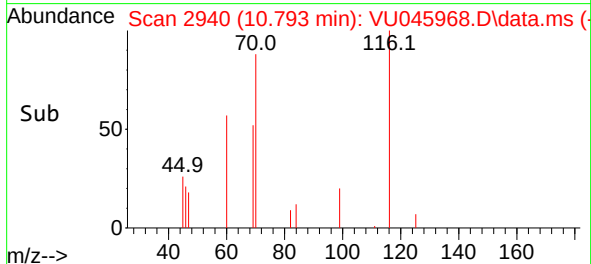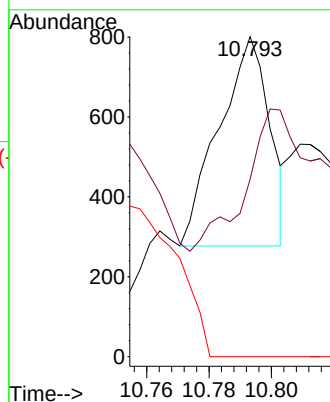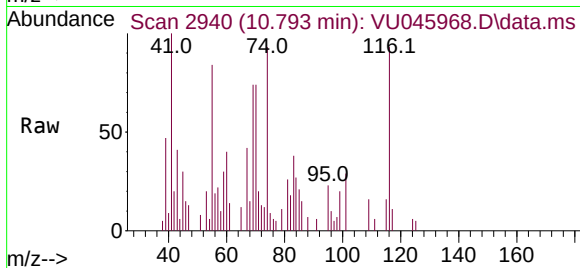

#60

Isopropylbenzene

Concen: 13.441 ug/L

RT: 10.484 min Scan# 2844

Delta R.T. -0.003 min

Lab File: VU045968.D

Acq: 23 Nov 2021 20:06




Tgt Ion:105 Resp: 396228


Ion Ratio Lower Upper

105 100

120 25.5 20.7 31.1

77 15.8 12.6 19.0


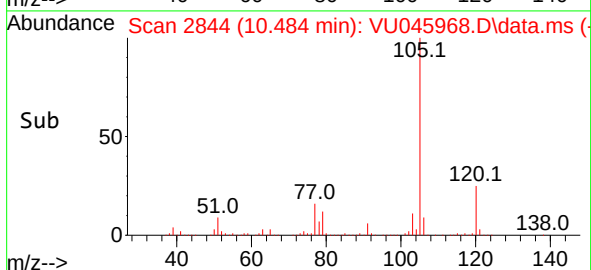

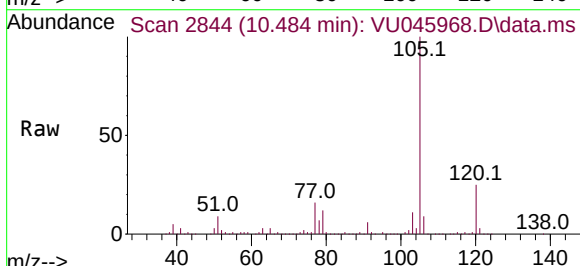


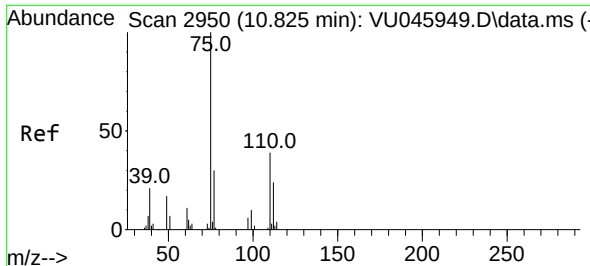

#61
1,2,3-Trichloropropane
Concen: 1.573 ug/L
RT: 10.906 min Scan# 2950
Delta R.T. 0.081 min
Lab File: VU045968.D
Acq: 23 Nov 2021 20:06




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 75 Resp: 8202
Ion Ratio Lower Upper
75 100
110 3.1 29.9 44.9#
77 599.0 25.5 38.3#

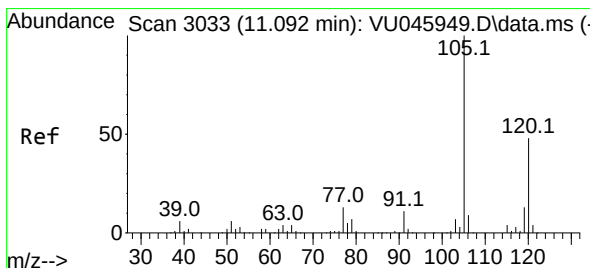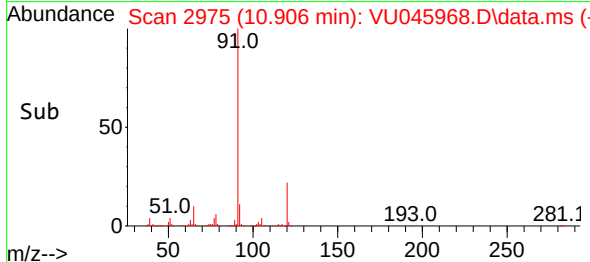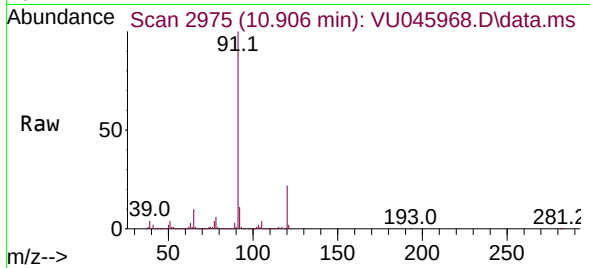

#62
1,3,5-Trimethylbenzene
Concen: 5.865 ug/L
RT: 11.468 min Scan# 3150
Delta R.T. 0.376 min
Lab File: VU045968.D
Acq: 23 Nov 2021 20:06

Tgt Ion:105 Resp: 141371
Ion Ratio Lower Upper
105 100
120 44.2 38.3 57.5


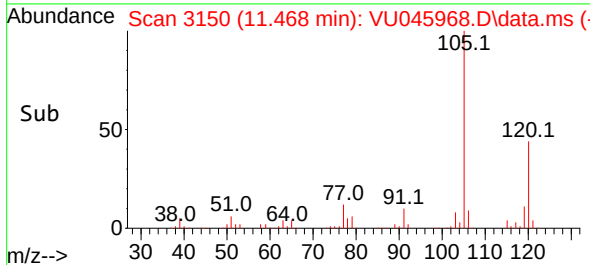

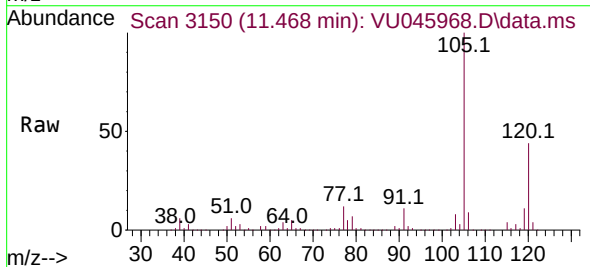




#63
1,2,4-Trimethylbenzene
Concen: 5.854 ug/L
RT: 11.468 min Scan# 3151
Delta R.T. -0.003 min
Lab File: VU045968.D
Acq: 23 Nov 2021 20:06




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion:105 Resp: 141371
Ion Ratio Lower Upper
105 100
120 44.2 35.8 53.8

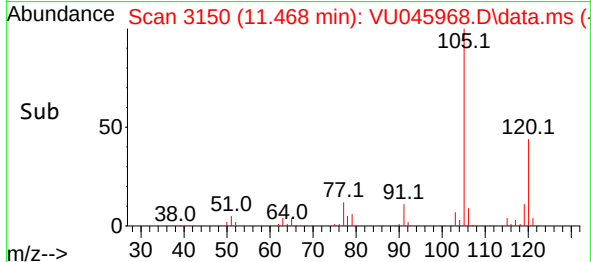

#67
1,2-Dichlorobenzene
Concen: 0.091 ug/L
RT: 12.214 min Scan# 3382
Delta R.T. 0.000 min
Lab File: VU045968.D
Acq: 23 Nov 2021 20:06

Tgt Ion:146 Resp: 1196
Ion Ratio Lower Upper
146 100
111 106.6 35.4 53.0#
148 56.2 51.1 76.7


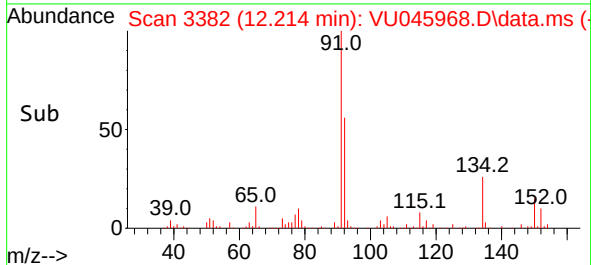

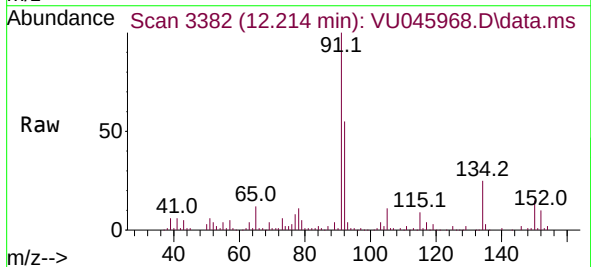


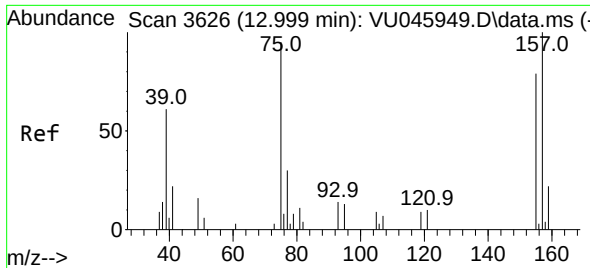

#68
 1,2-Dibromo-3-chloropropane
 Concen: 3.354 ug/L
 RT: 12.973 min Scan# 3618
 Delta R.T. -0.026 min
 Lab File: VU045968.D
 Acq: 23 Nov 2021 20:06

Instrument :
 MSVOA_U
 ClientSampleId :

Tgt Ion: 75 Resp: 3637
 Ion Ratio Lower Upper
 75 100
 155 0.0 59.2 88.8#
 157 0.0 76.5 114.7#

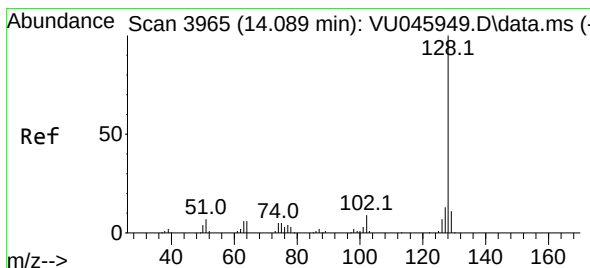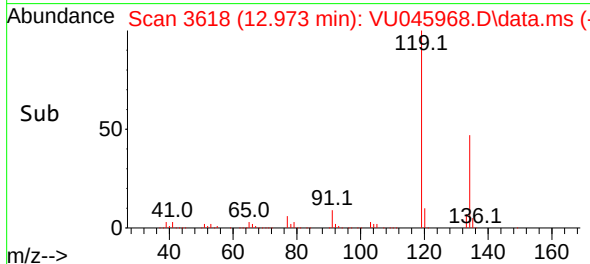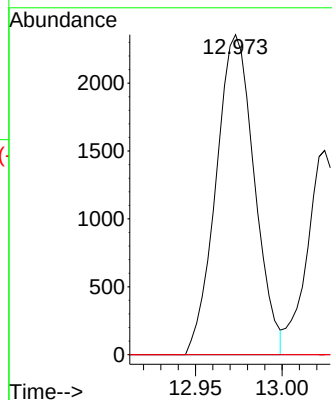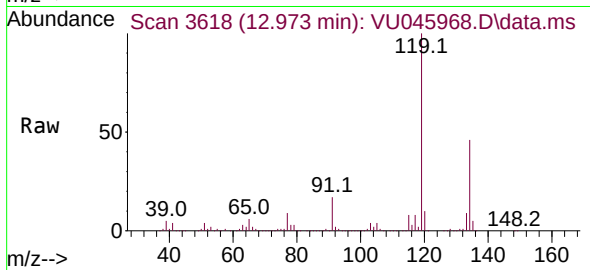

#71
 Naphthalene
 Concen: 61.058 ug/L
 RT: 14.086 min Scan# 3964
 Delta R.T. -0.003 min
 Lab File: VU045968.D
 Acq: 23 Nov 2021 20:06

Tgt Ion:128 Resp: 1092035
 Ion Ratio Lower Upper
 128 100
 129 11.3 8.4 12.6
 127 12.9 10.2 15.2

