




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112321\
 Data File : VU045956.D
 Acq On : 23 Nov 2021 15:19
 Operator : SY/MD
 Sample : M4779-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4L22

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 11/24/2021
 Supervised By :Mahesh Dadoda 11/28/2021

Quant Time: Nov 24 00:32:13 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR11521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 24 00:27:16 2021
 Response via : Initial Calibration

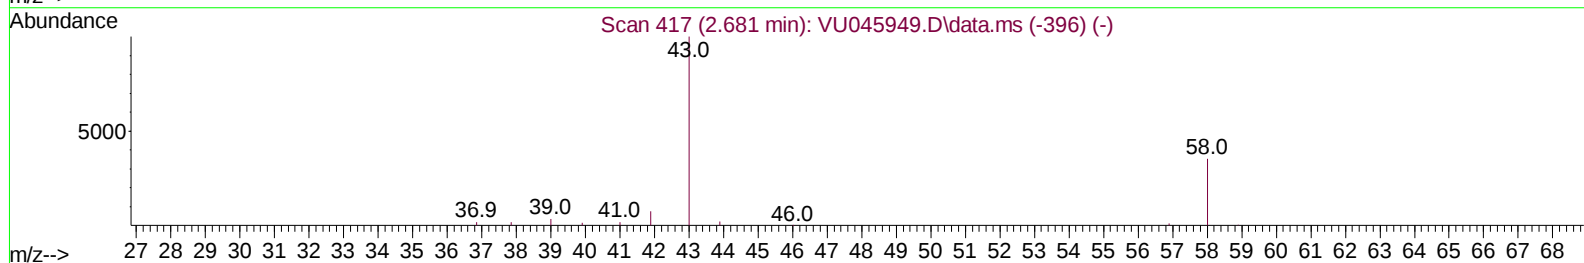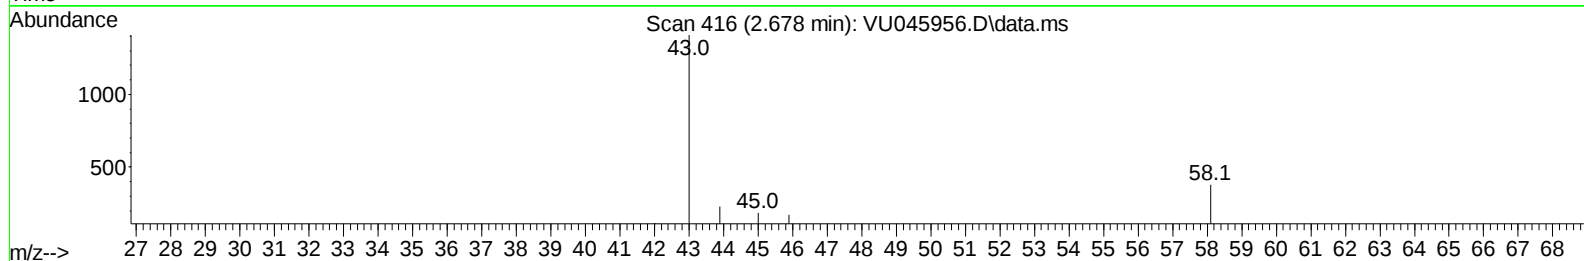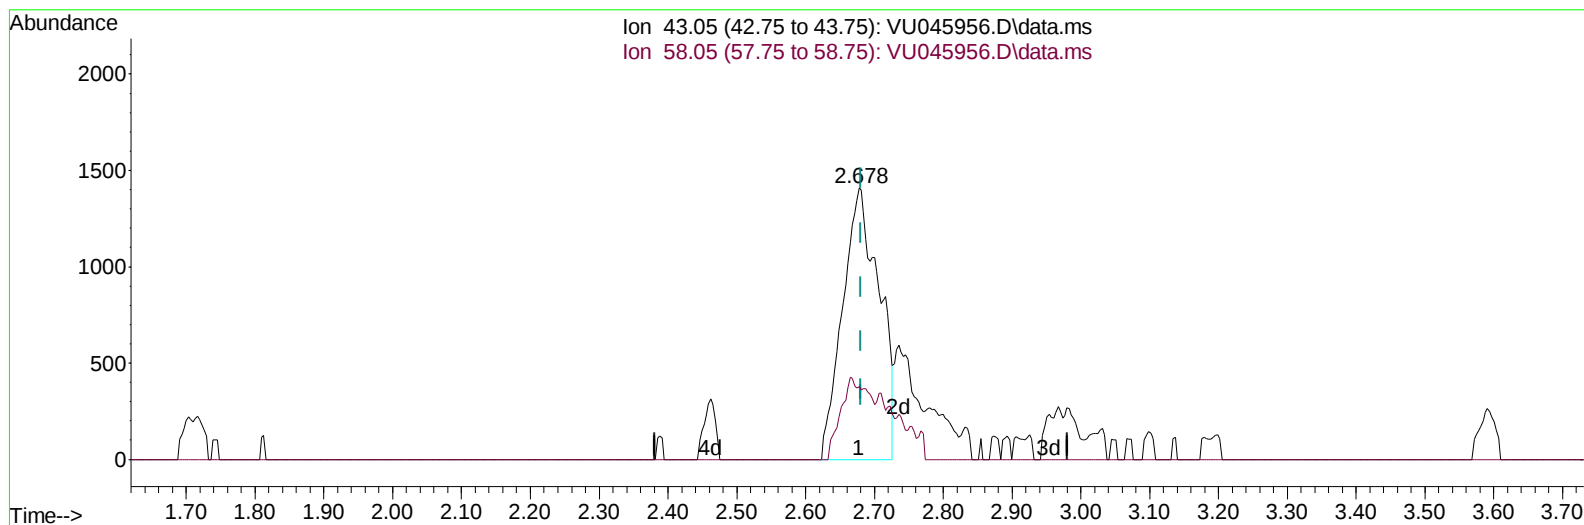

TIC: VU045956.D\data.ms

(13) Acetone (T)

2.678min (-0.003) 4.26 ug/L

response 5189

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.80	23.65
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112321\
 Data File : VU045956.D
 Acq On : 23 Nov 2021 15:19
 Operator : SY/MD
 Sample : M4779-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4L22

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 11/24/2021
 Supervised By :Mahesh Dadoda 11/28/2021

Quant Time: Nov 24 00:32:13 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR11521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 24 00:27:16 2021
 Response via : Initial Calibration

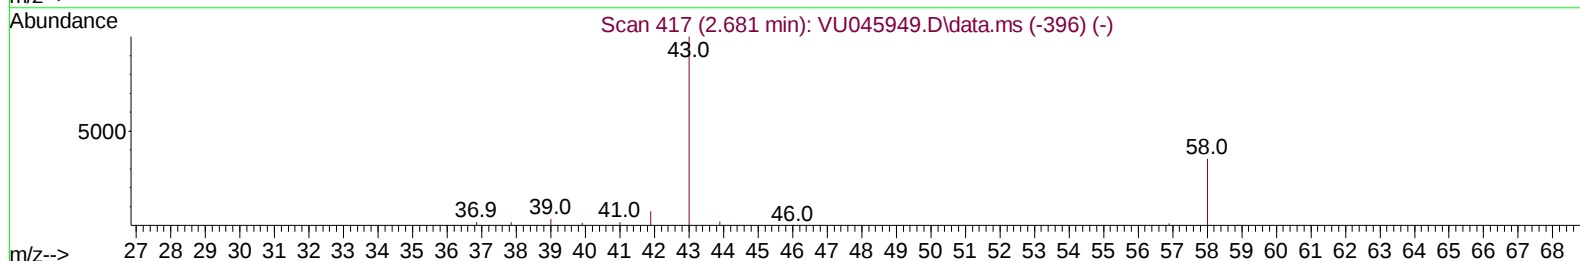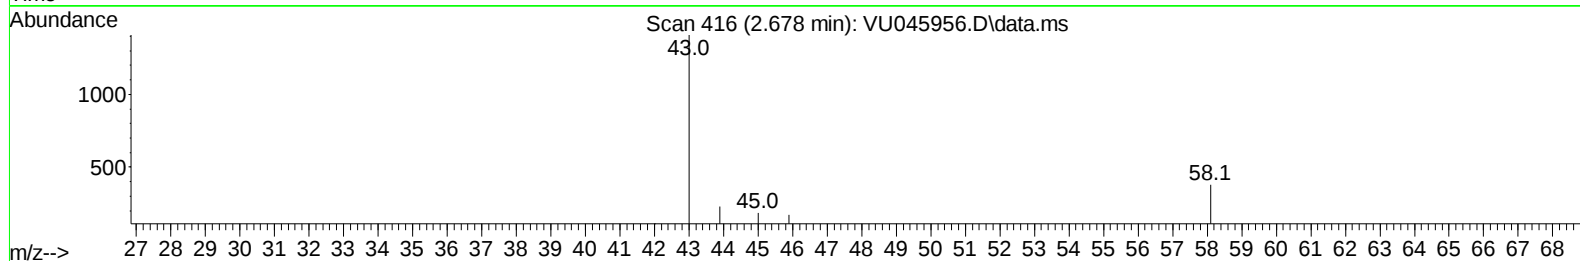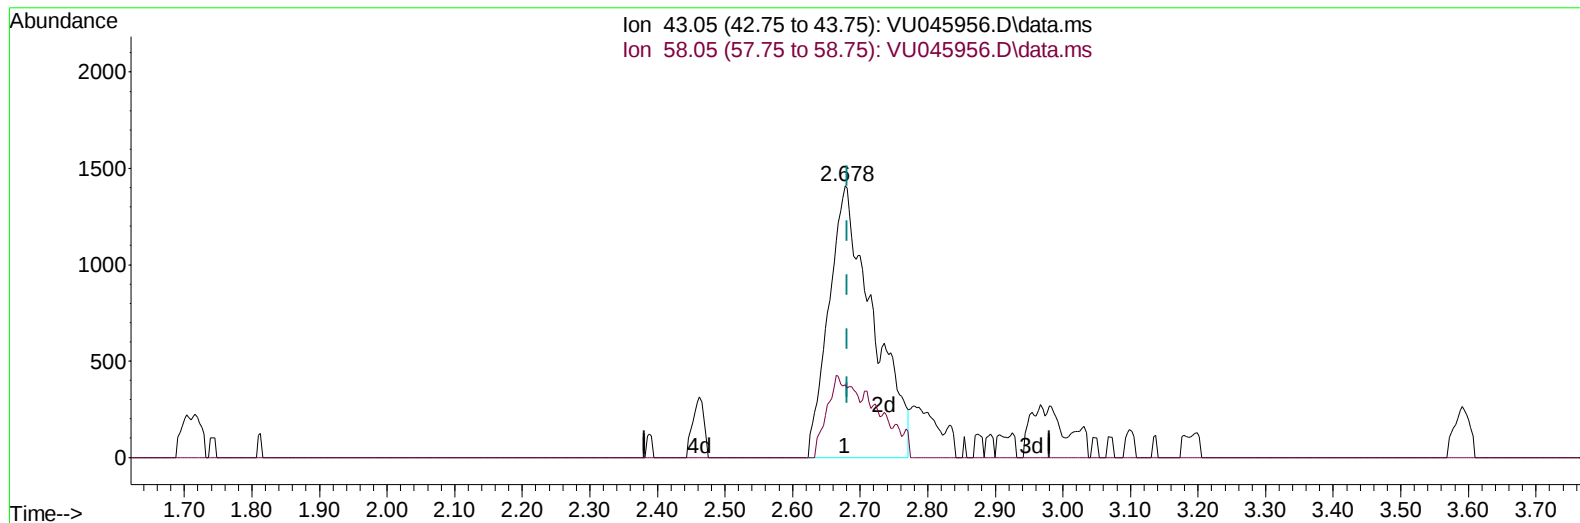

TIC: VU045956.D\data.ms

(13) Acetone (T)

2.678min (-0.003) 5.22 ug/L m

response 6357

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.80	19.30
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112321\
 Data File : VU045956.D
 Acq On : 23 Nov 2021 15:19
 Operator : SY/MD
 Sample : M4779-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4L22

Manual IntegrationsAPPROVED

Reviewed By : John Carlone 11/24/2021
 Supervised By : Mahesh Dadoda 11/28/2021

Quant Time: Nov 24 00:32:13 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 24 00:27:16 2021
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.253	114		97534	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117		96421	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152		44887	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.600	65		22498	2.911	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery =	58.200%		
7) Chloroethane-d5	1.919	69		20606	3.663	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery =	73.200%		
11) 1,1-Dichloroethene-d2	2.571	65		9613	2.966	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery =	59.400%#		
20) 2-Butanone-d5	4.649	46		131614	63.555	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery =	127.120%		
24) Chloroform-d	5.067	84		51764	4.021	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	80.400%		
26) 1,2-Dichloroethane-d4	5.706	65		33278	4.405	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	88.200%		
32) Benzene-d6	5.732	84		97543	3.674	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	73.400%		
36) 1,2-Dichloropropane-d6	6.694	67		33862	4.046	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery =	81.000%		
41) Toluene-d8	7.899	98		77521	3.227	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	64.600%#		
43) trans-1,3-Dichloroprop...	8.182	79		13069	3.847	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery =	77.000%		
46) 2-Hexanone-d5	8.636	63		87907	57.491	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery =	114.980%		
56) 1,1,2,2-Tetrachloroeth...	10.758	84		37290	5.274	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery =	105.400%		
66) 1,2-Dichlorobenzene-d4	12.195	152		34866	4.524	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery =	90.400%		
Target Compounds							Qvalue
13) Acetone	2.678	43		6357m	5.215	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112321\
Data File : VU045956.D
Acq On : 23 Nov 2021 15:19
Operator : SY/MD
Sample : M4779-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4L22

Manual IntegrationsAPPROVED

Quant Time: Nov 24 00:32:13 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR11521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 24 00:27:16 2021
Response via : Initial Calibration

Reviewed By :John Carlone 11/24/2021
Supervised By :Mahesh Dadoda 11/28/2021

