




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112321\
Data File : VU045957.D
Acq On : 23 Nov 2021 15:43
Operator : SY/MD
Sample : M4779-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4L23

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 11/24/2021
Supervised By :Mahesh Dadoda 11/28/2021

Quant Time: Nov 24 00:32:24 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR11521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 24 00:27:16 2021
Response via : Initial Calibration

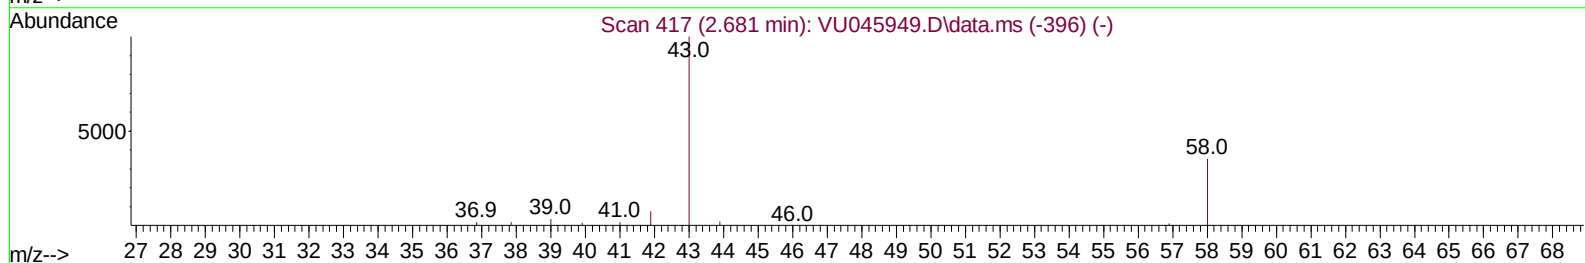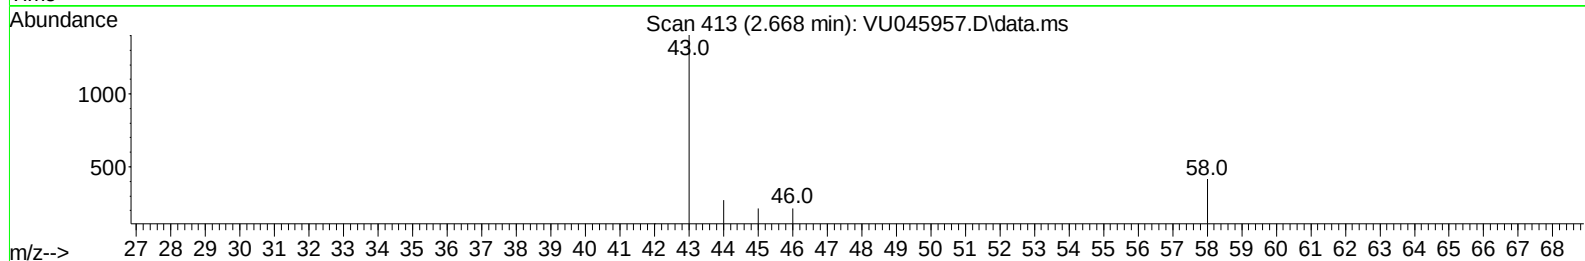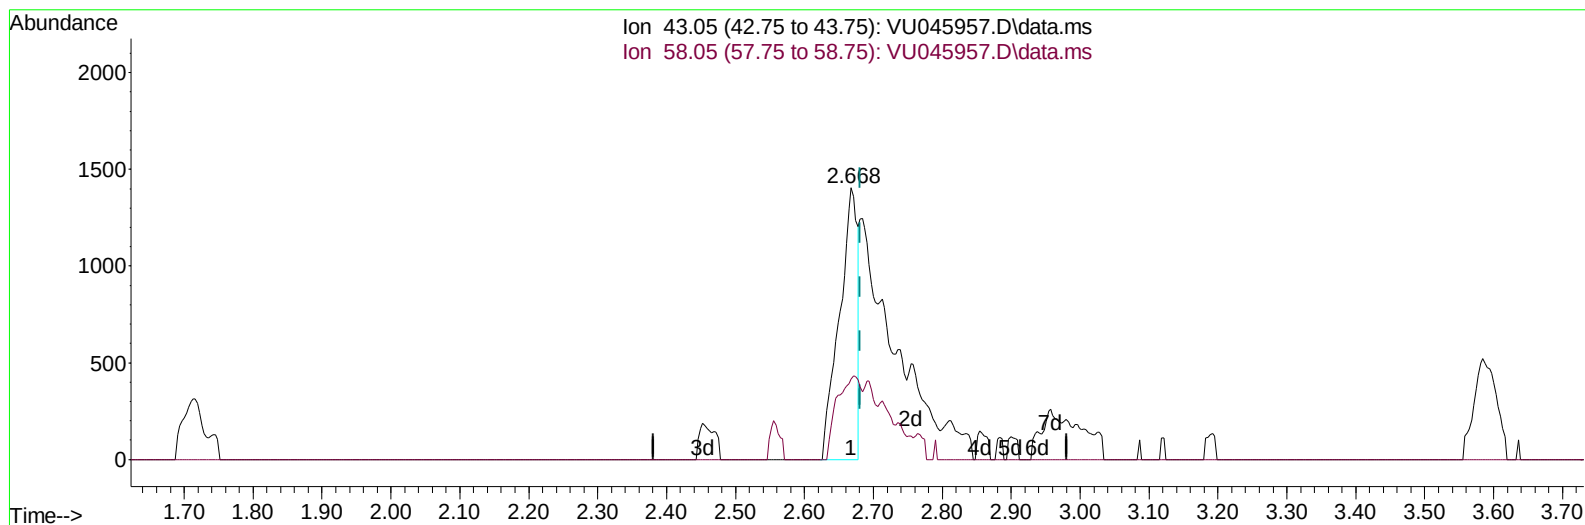

TIC: VU045957.D\data.ms

(13) Acetone (T)

2.668min (-0.013) 2.06 ug/L

response 2538

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.80	41.25
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112321\
Data File : VU045957.D
Acq On : 23 Nov 2021 15:43
Operator : SY/MD
Sample : M4779-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4L23

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 11/24/2021
Supervised By :Mahesh Dadoda 11/28/2021

Quant Time: Nov 24 00:32:24 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 24 00:27:16 2021
Response via : Initial Calibration

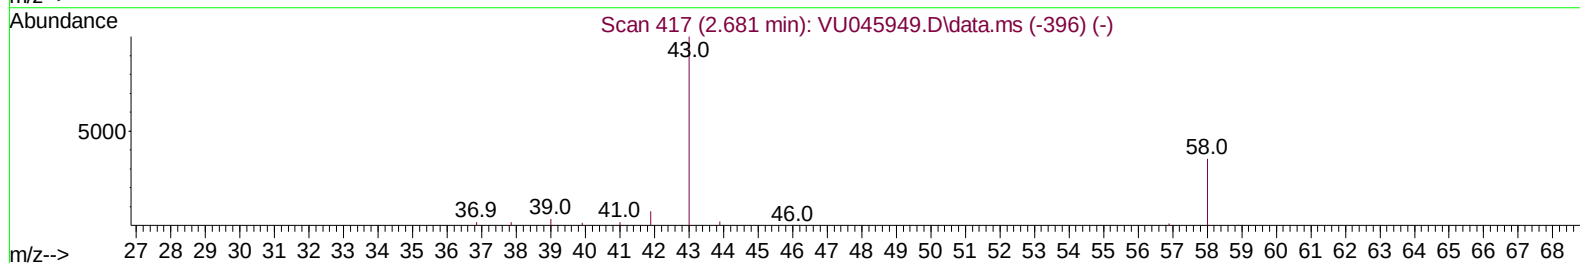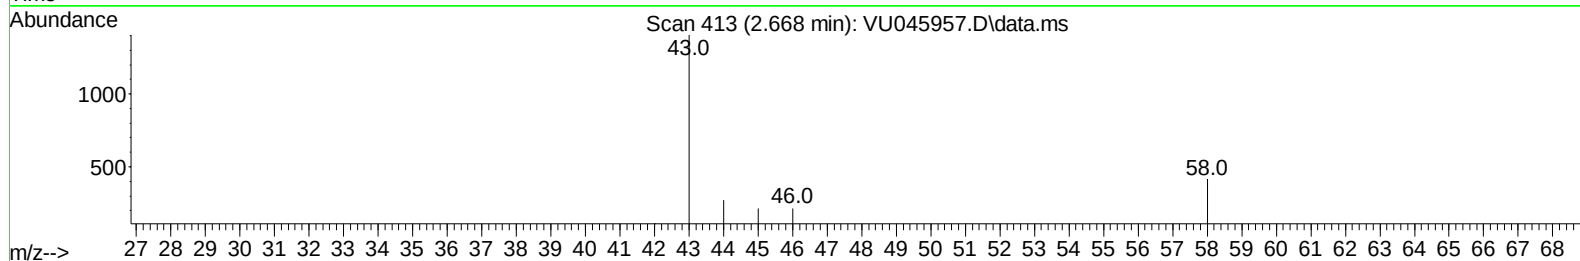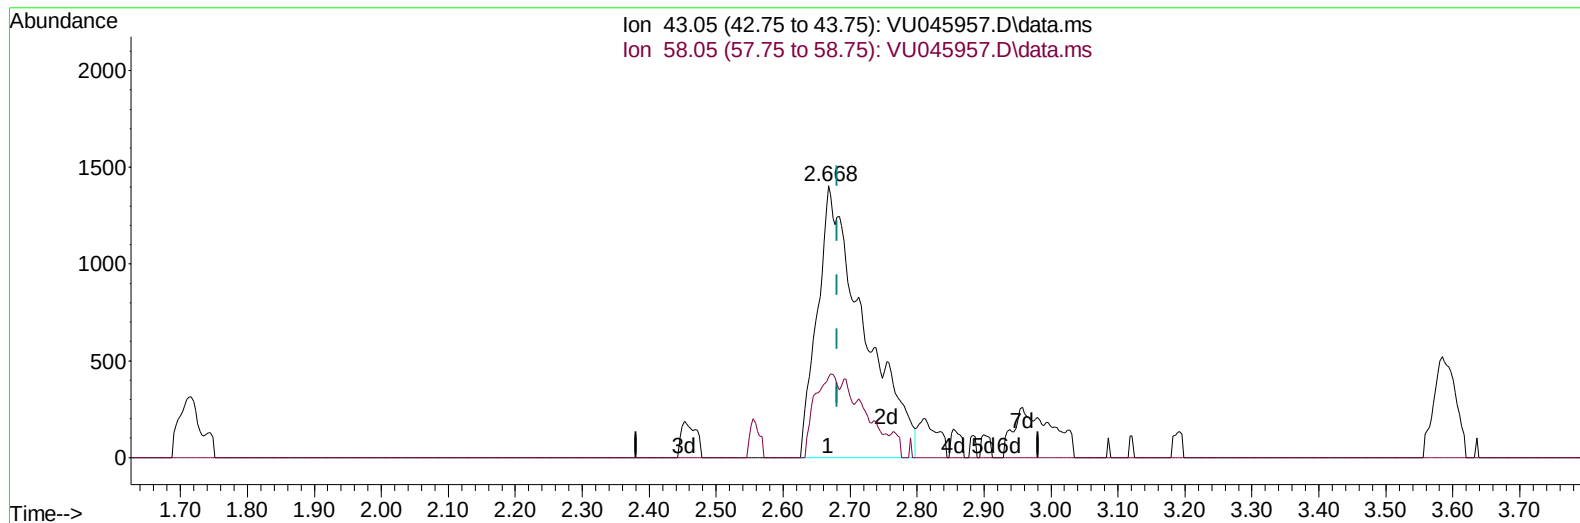

TIC: VU045957.D\data.ms

(13) Acetone (T)

2.668min (-0.013) 5.48 ug/L m

response 6733

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.80	15.55
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112321\
 Data File : VU045957.D
 Acq On : 23 Nov 2021 15:43
 Operator : SY/MD
 Sample : M4779-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4L23

Manual IntegrationsAPPROVED

Quant Time: Nov 24 00:32:24 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 24 00:27:16 2021
 Response via : Initial Calibration

Reviewed By :John Carlone 11/24/2021
 Supervised By :Mahesh Dadoda 11/28/2021

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.253	114		98378	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117		99289	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152		45519	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.600	65		23228	2.980	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery =	59.600%		
7) Chloroethane-d5	1.919	69		21111	3.721	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery =	74.400%		
11) 1,1-Dichloroethene-d2	2.571	65		10049	3.074	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery =	61.400%		
20) 2-Butanone-d5	4.648	46		134706	64.490	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery =	128.980%		
24) Chloroform-d	5.066	84		52982	4.080	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	81.600%		
26) 1,2-Dichloroethane-d4	5.706	65		32960	4.326	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	86.600%		
32) Benzene-d6	5.732	84		99170	3.627	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	72.600%		
36) 1,2-Dichloropropane-d6	6.693	67		34639	4.020	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery =	80.400%		
41) Toluene-d8	7.899	98		79180	3.201	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	64.000%#		
43) trans-1,3-Dichloroprop...	8.182	79		13327	3.810	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery =	76.200%		
46) 2-Hexanone-d5	8.635	63		91019	57.806	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery =	115.620%		
56) 1,1,2,2-Tetrachloroeth...	10.758	84		37913	5.208	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery =	104.200%		
66) 1,2-Dichlorobenzene-d4	12.195	152		35251	4.510	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery =	90.200%		
Target Compounds							
13) Acetone	2.668	43		6733m	5.477	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112321\
Data File : VU045957.D
Acq On : 23 Nov 2021 15:43
Operator : SY/MD
Sample : M4779-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4L23

Manual IntegrationsAPPROVED

Quant Time: Nov 24 00:32:24 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR11521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 24 00:27:16 2021
Response via : Initial Calibration

Reviewed By :John Carlone 11/24/2021
Supervised By :Mahesh Dadoda 11/28/2021

