




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112321\
Data File : VU045963.D
Acq On : 23 Nov 2021 18:06
Operator : SY/MD
Sample : M4722-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0G05

Manual IntegrationsAPPROVED

Quant Time: Nov 24 00:33:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR11521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 24 00:27:16 2021
Response via : Initial Calibration

Reviewed By :John Carlone 11/24/2021
Supervised By :Semsettin Yesilyurt 11/29/2021

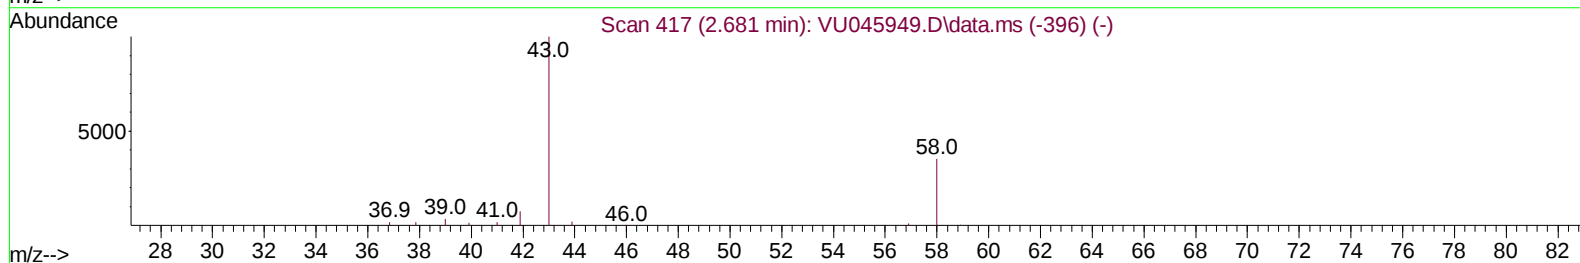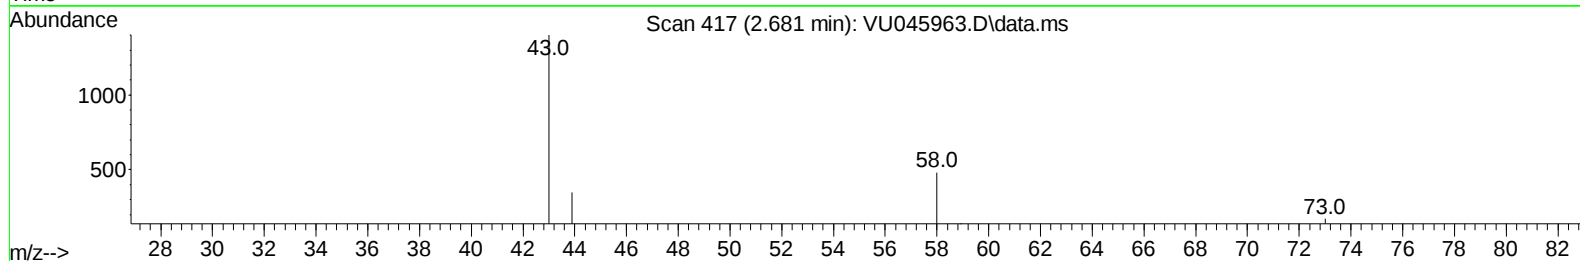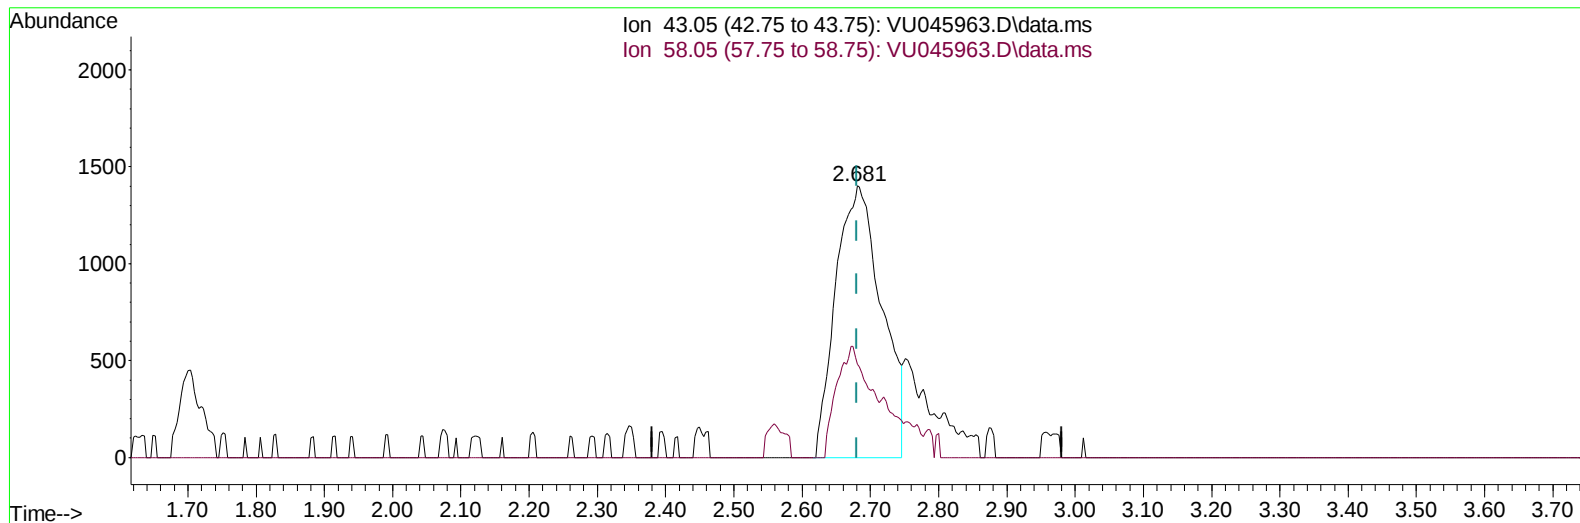

TIC: VU045963.D\data.ms

(13) Acetone (T)

2.681min (+ 0.000) 5.75 ug/L

response 6538

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.80	28.80
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112321\
Data File : VU045963.D
Acq On : 23 Nov 2021 18:06
Operator : SY/MD
Sample : M4722-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0G05

Manual IntegrationsAPPROVED

Quant Time: Nov 24 00:33:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR11521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 24 00:27:16 2021
Response via : Initial Calibration

Reviewed By :John Carlone 11/24/2021
Supervised By :Semsettin Yesilyurt 11/29/2021

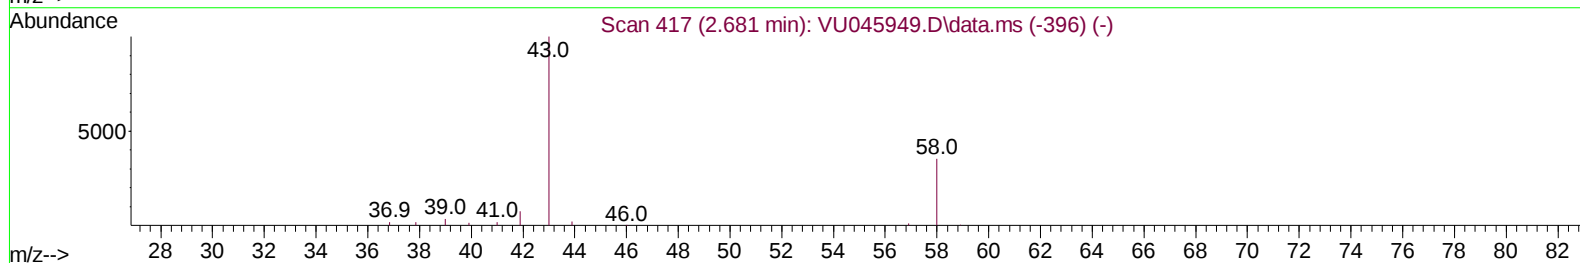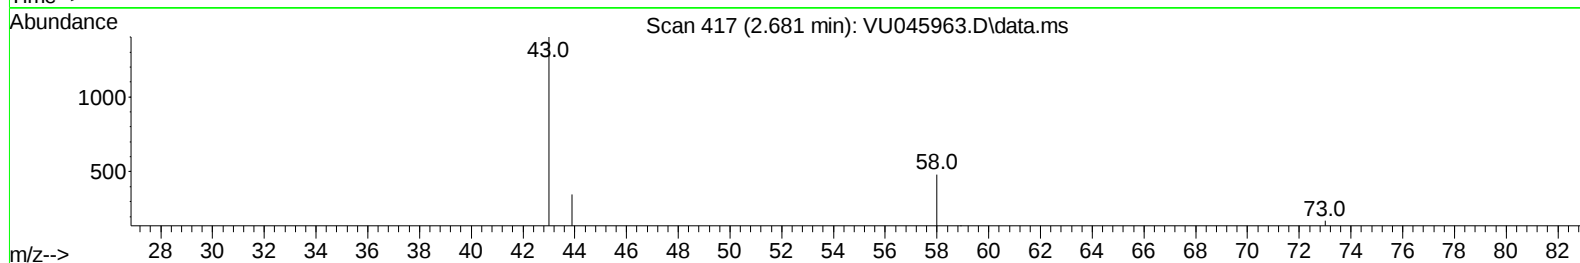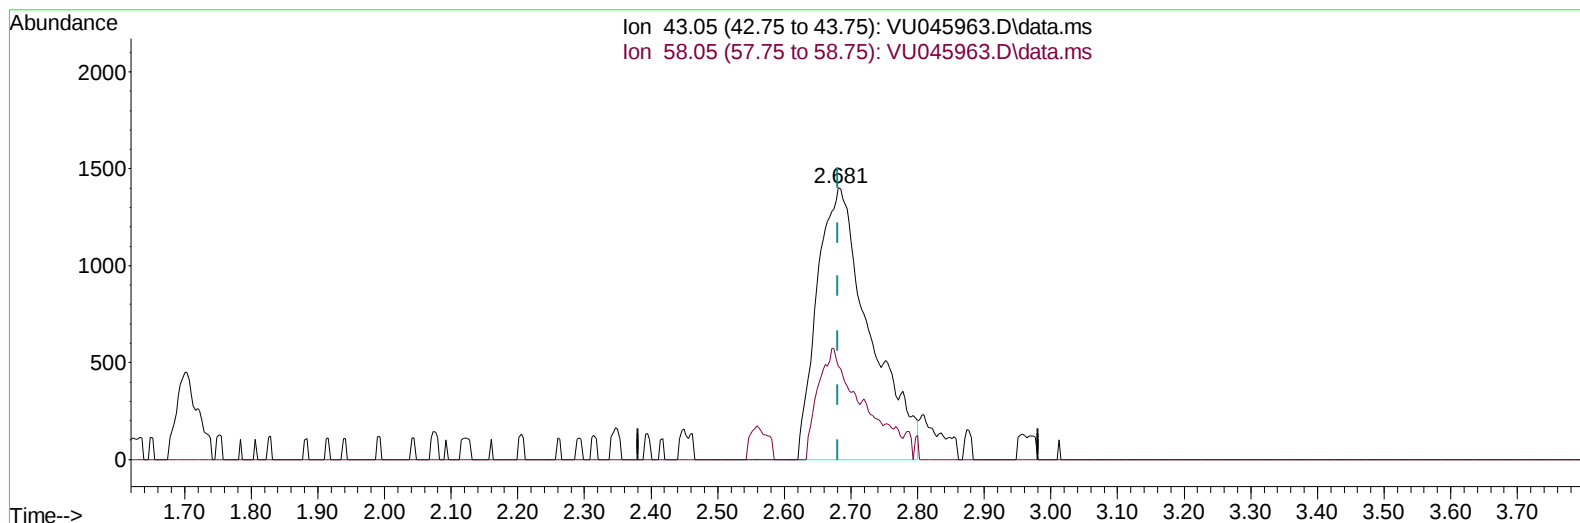

TIC: VU045963.D\data.ms

(13) Acetone (T)

2.681min (+ 0.000) 6.73 ug/L m

response 7654

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.80	24.60
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112321\
 Data File : VU045963.D
 Acq On : 23 Nov 2021 18:06
 Operator : SY/MD
 Sample : M4722-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0G05

Manual IntegrationsAPPROVED

Quant Time: Nov 24 00:33:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 24 00:27:16 2021
 Response via : Initial Calibration

Reviewed By :John Carlone 11/24/2021
 Supervised By :Semsettin Yesilyurt 11/29/2021

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.253	114		90972	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117		90123	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152		42225	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.601	65		17973	2.494	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	49.800%	
7) Chloroethane-d5	1.919	69		26460	5.043	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.800%	
11) 1,1-Dichloroethene-d2	2.572	65		12449	4.118	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.400%	
20) 2-Butanone-d5	4.649	46		129722	67.160	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	134.320%#	
24) Chloroform-d	5.067	84		66252	5.517	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	110.400%	
26) 1,2-Dichloroethane-d4	5.707	65		38345	5.442	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.800%	
32) Benzene-d6	5.732	84		135290	5.451	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	109.000%	
36) 1,2-Dichloropropane-d6	6.694	67		44906	5.741	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	114.800%	
41) Toluene-d8	7.899	98		111580	4.970	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.400%	
43) trans-1,3-Dichloroprop...	8.182	79		12698	3.999	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.000%	
46) 2-Hexanone-d5	8.636	63		92677	64.846	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	129.700%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84		40011	6.055	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	121.000%#	
66) 1,2-Dichlorobenzene-d4	12.195	152		43851	6.048	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	121.000%#	
Target Compounds							
13) Acetone	2.681	43		7654m	6.733	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112321\
Data File : VU045963.D
Acq On : 23 Nov 2021 18:06
Operator : SY/MD
Sample : M4722-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0G05

Manual IntegrationsAPPROVED

Quant Time: Nov 24 00:33:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 24 00:27:16 2021
Response via : Initial Calibration

Reviewed By :John Carlone 11/24/2021
Supervised By :Semsettin Yesilyurt 11/29/2021

