
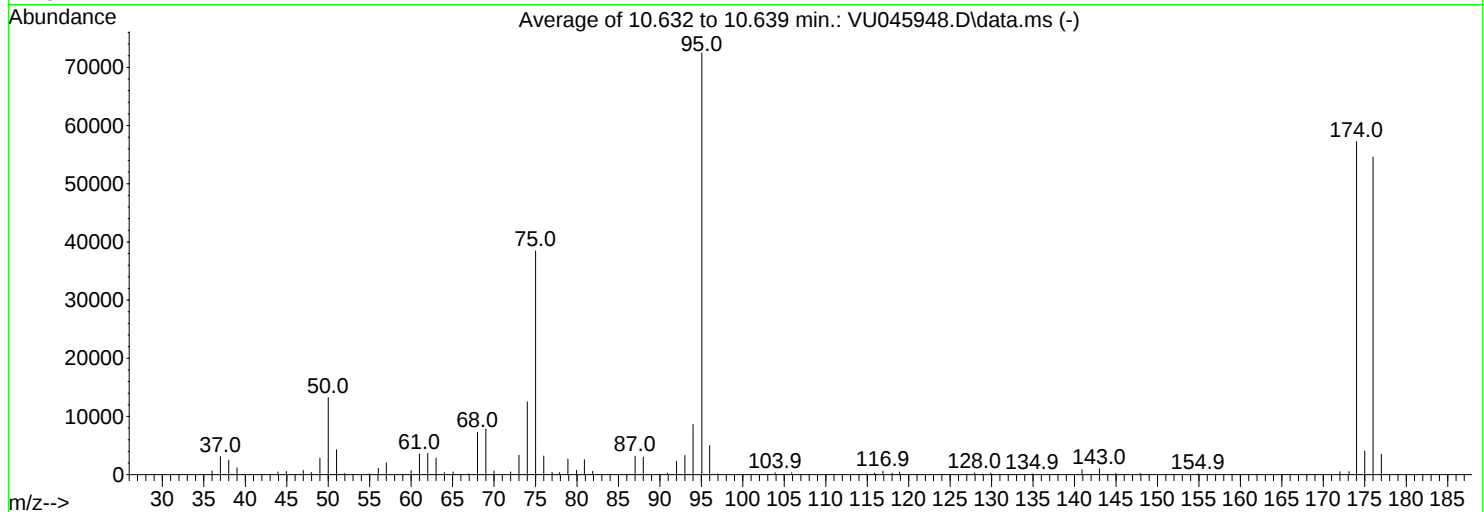


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112321\
Data File : VU045948.D
Acq On : 23 Nov 2021 09:33
Operator : SY/MD
Sample : BFB030
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB030

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Nov 26 23:26:55 2021

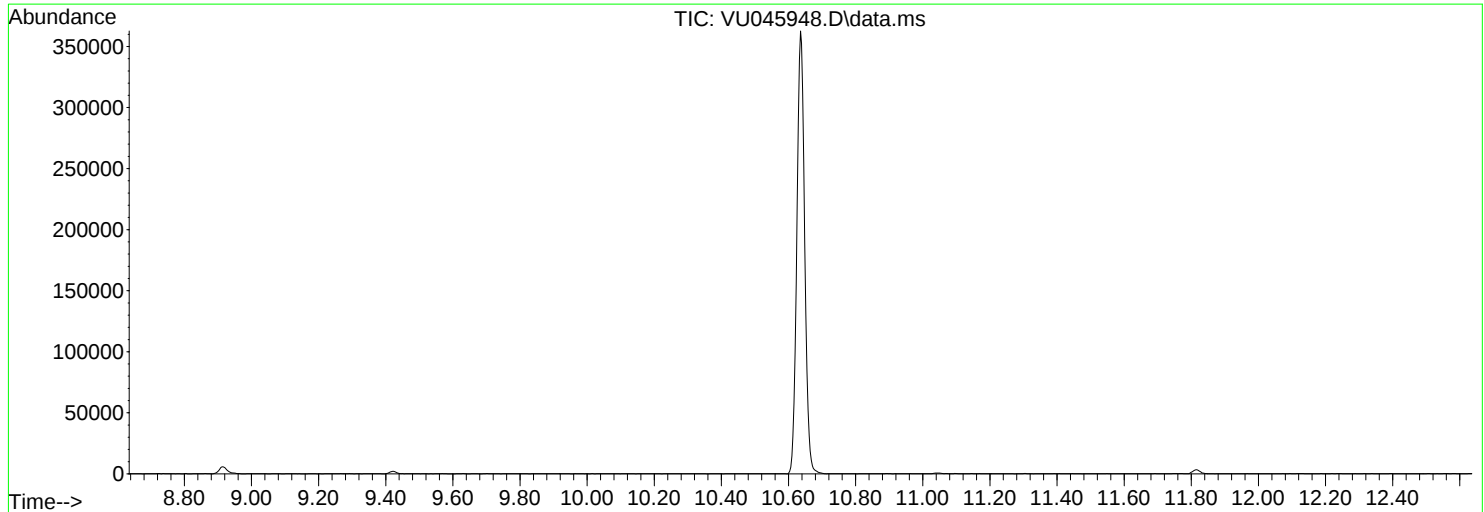

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	13244	PASS
75	95	30	80	53.0	38443	PASS
95	95	100	100	100.0	72499	PASS
96	95	5	9	6.9	5011	PASS
173	174	0.00	2	0.9	523	PASS
174	95	50	120	79.0	57272	PASS
175	174	5	9	7.1	4060	PASS
176	174	95	101	95.3	54595	PASS
177	176	5	9	6.4	3509	PASS

m/z	Abundance
43.80	105.0

Instrument :
MSVOA_U
ClientSampleId :
BFB030

m/z	Abundance
36.00	620.0
37.00	3090.0
38.00	2475.0
39.00	1183.0
39.90	141.0
44.00	562.0
44.90	560.0
47.00	708.0
47.90	350.0
49.00	2759.0
50.00	12777.0
51.00	4385.0
52.00	187.0
55.00	172.0
56.00	1114.0
57.00	1948.0
60.00	711.0
61.00	3384.0
62.00	3582.0
63.00	2898.0
64.00	367.0
65.00	482.0
66.90	172.0
68.00	7000.0
69.00	7524.0
70.00	603.0
72.00	378.0
73.00	3266.0
74.00	12287.0
75.00	37376.0
76.00	3131.0
77.00	380.0
77.90	387.0
78.90	2622.0
79.90	746.0
80.90	2485.0
81.90	556.0
87.00	2963.0
88.00	2957.0
90.80	235.0
92.00	2349.0
93.00	3365.0
94.00	8241.0
95.00	70544.0
96.00	4941.0
96.90	170.0
103.90	310.0
104.90	102.0
105.90	307.0
114.90	134.0
115.90	291.0
116.90	534.0
118.00	224.0
118.90	449.0
128.00	270.0
128.90	135.0
129.90	242.0
130.90	126.0
134.90	139.0
136.80	112.0
140.90	850.0
143.00	951.0
145.00	171.0
145.90	110.0
147.90	183.0
154.90	161.0
172.00	537.0
173.10	506.0
174.00	54096.0
175.00	3823.0
176.00	51896.0
177.00	3345.0
177.90	100.0

Instrument :
MSVOA_U
ClientSampleId :
BFB030

m/z	Abundance
36.00	664.0
37.00	3220.0
38.00	2516.0
39.00	1202.0
39.90	117.0
44.00	587.0
45.00	577.0
47.00	728.0
48.00	402.0
49.00	2945.0
50.00	13639.0
51.00	4460.0
52.00	196.0
55.00	152.0
56.10	1154.0
57.00	2115.0
60.00	755.0
61.00	3676.0
62.00	3760.0
63.00	2923.0
64.00	363.0
65.00	484.0
67.00	177.0
68.00	7495.0
69.00	8113.0
70.00	660.0
72.00	481.0
73.00	3484.0
74.00	12892.0
75.00	39712.0
76.00	3254.0
77.00	452.0
77.90	363.0
78.90	2690.0
79.90	757.0
80.90	2631.0
81.90	588.0
87.00	3282.0
88.00	3123.0
90.90	279.0
92.00	2392.0
93.00	3418.0
94.00	8901.0
95.10	74768.0
96.00	5153.0
96.90	187.0
103.90	338.0
105.90	339.0
114.90	129.0
115.90	300.0
116.90	621.0
118.00	256.0
118.90	508.0
127.90	325.0
128.90	169.0
129.90	253.0
130.90	132.0
134.90	178.0
136.80	109.0
140.90	868.0
143.00	1070.0
144.90	199.0
147.90	216.0
154.90	181.0
157.00	139.0
158.90	102.0
172.00	508.0
173.10	544.0
174.00	59144.0
175.00	4182.0
176.00	56360.0
177.00	3584.0

Instrument :
MSVOA_U
ClientSampleId :
BFB030

m/z	Abundance
36.00	604.0
37.00	3028.0
38.00	2405.0
39.00	1158.0
44.00	581.0
45.00	539.0
47.00	717.0
48.00	414.0
49.00	2860.0
50.00	13315.0
51.00	4019.0
51.90	202.0
54.90	156.0
56.00	1030.0
57.00	2076.0
60.00	702.0
61.00	3570.0
62.00	3665.0
63.00	2667.0
64.00	356.0
65.10	455.0
67.00	177.0
68.00	7352.0
69.00	7918.0
70.00	623.0
72.00	513.0
73.00	3280.0
74.00	12380.0
75.00	38240.0
76.00	3179.0
77.00	434.0
77.90	314.0
78.90	2658.0
80.00	724.0
80.90	2550.0
81.90	564.0
87.00	3277.0
88.00	3020.0
91.00	331.0
92.00	2169.0
93.00	3154.0
94.00	8786.0
95.10	72184.0
96.00	4938.0
97.00	159.0
103.90	334.0
105.90	334.0
114.90	101.0
115.90	268.0
116.90	657.0
118.00	280.0
118.90	454.0
127.90	342.0
128.90	162.0
129.90	252.0
131.00	117.0
134.90	190.0
140.90	829.0
143.00	1044.0
144.90	193.0
147.90	219.0
154.90	185.0
157.00	174.0
158.90	126.0
172.00	458.0
173.10	518.0
174.00	58576.0
175.00	4176.0
176.00	55528.0
177.00	3598.0

Instrument :
MSVOA_U
ClientSampleId :
BFB030