

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112322\
 Data File : VU052104.D
 Acq On : 23 Nov 2022 22:23
 Operator : JC/MD
 Sample : N5739-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBNK2

Quant Time: Nov 24 04:16:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Nov 24 04:13:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	218671	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	226596	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	86546	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	81296	3.822	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	76.400%
7) Chloroethane-d5	1.912	69	74294	4.497	ug/L	0.02
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.000%
11) 1,1-Dichloroethene-d2	2.565	65	31233	4.097	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.000%
20) 2-Butanone-d5	4.620	46	215101	55.791	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	111.580%
24) Chloroform-d	5.060	84	157313	5.034	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.600%
26) 1,2-Dichloroethane-d4	5.700	65	79530	5.038	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.800%
32) Benzene-d6	5.726	84	309139	4.595	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.000%
36) 1,2-Dichloropropane-d6	6.690	67	104947	5.041	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.800%
41) Toluene-d8	7.896	98	238342	3.916	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.400%
43) trans-1,3-Dichloroprop...	8.179	79	32081	4.229	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.600%
46) 2-Hexanone-d5	8.632	63	165501	51.475	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.960%
56) 1,1,2,2-Tetrachloroeth...	10.755	84	89284	4.946	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.000%
66) 1,2-Dichlorobenzene-d4	12.192	152	85792	5.178	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.600%
Target Compounds					Qvalue	
13) Acetone	2.636	43	9299	3.552	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112322\
Data File : VU052104.D
Acq On : 23 Nov 2022 22:23
Operator : JC/MD
Sample : N5739-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBNK2

Quant Time: Nov 24 04:16:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Nov 24 04:13:15 2022
Response via : Initial Calibration

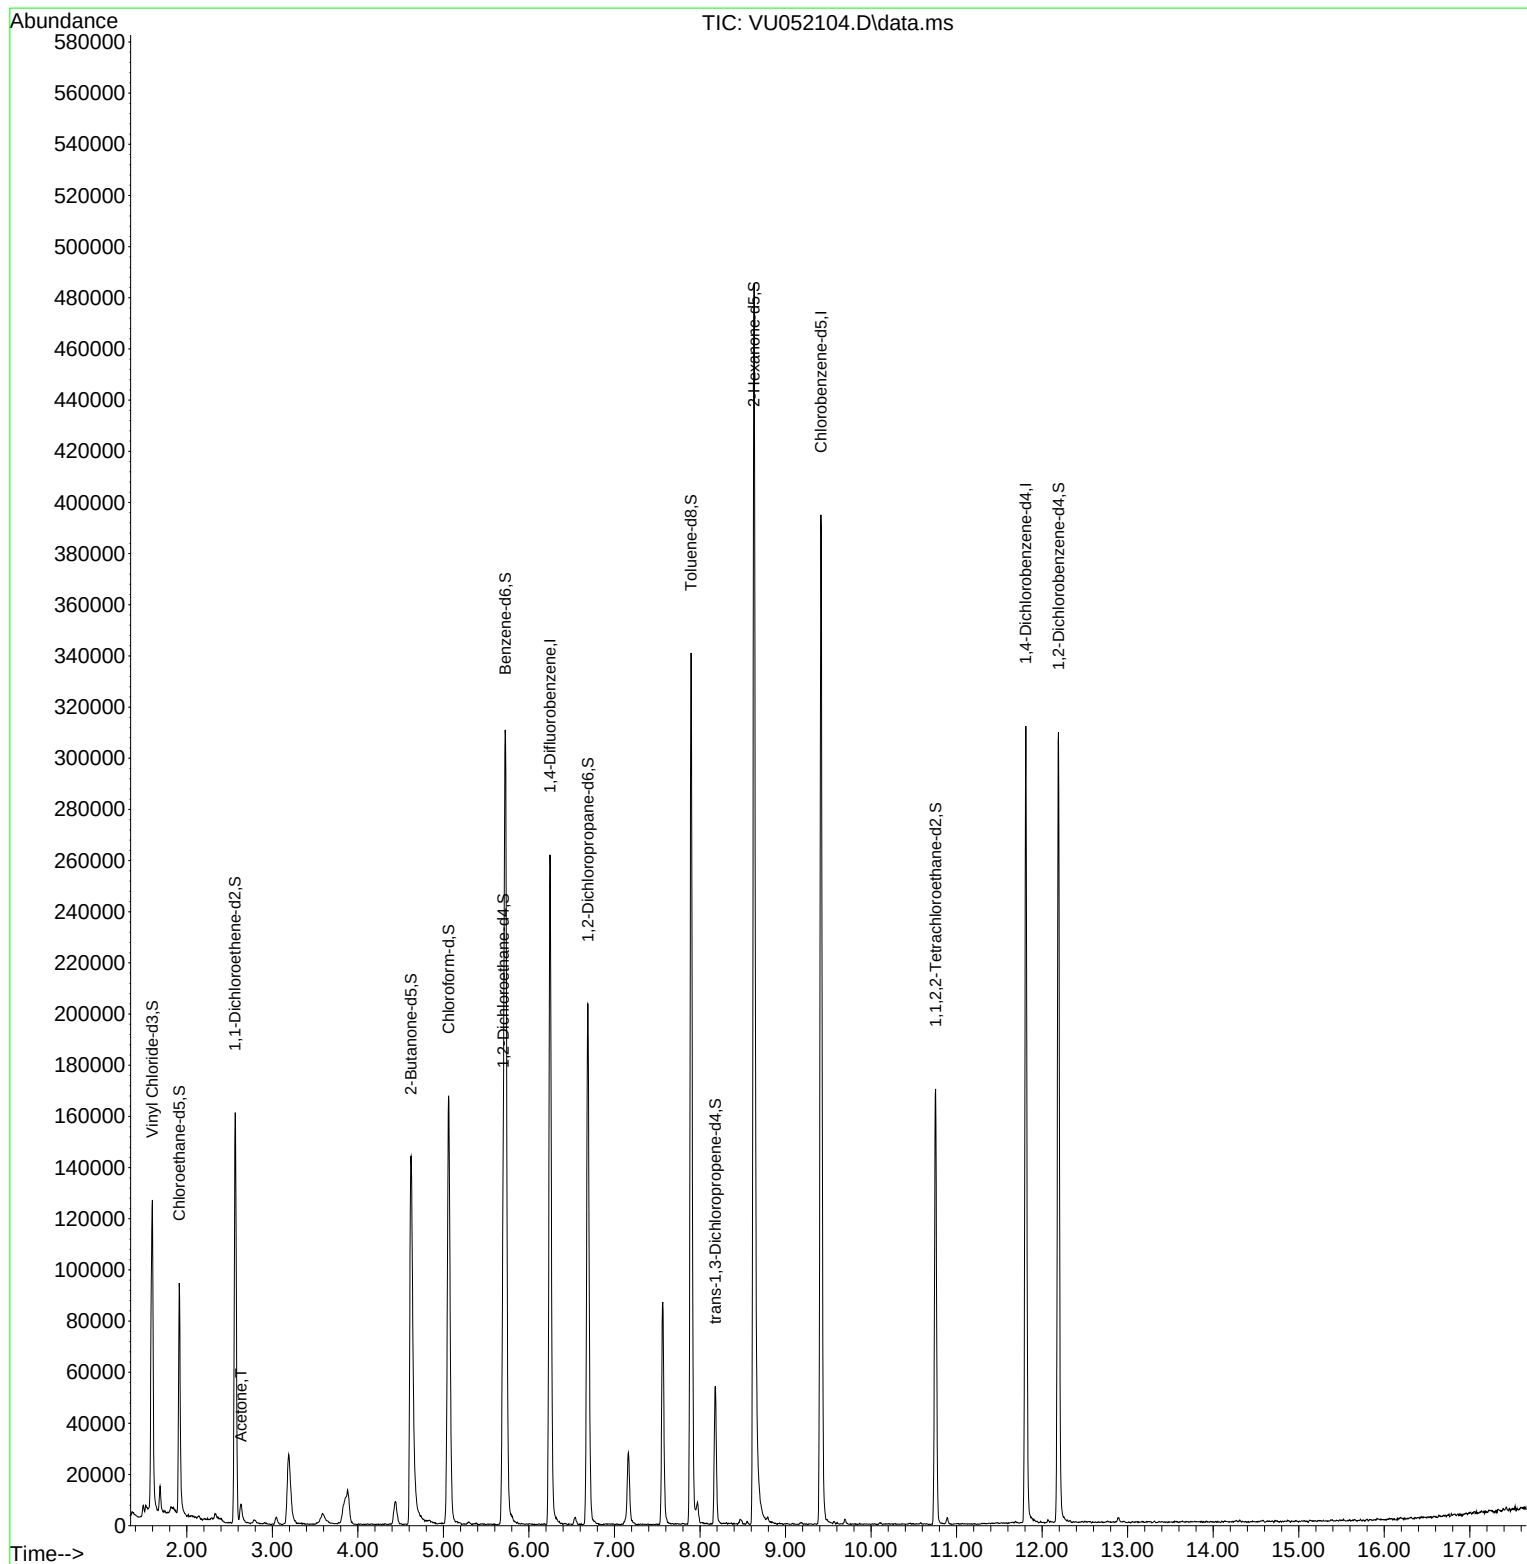

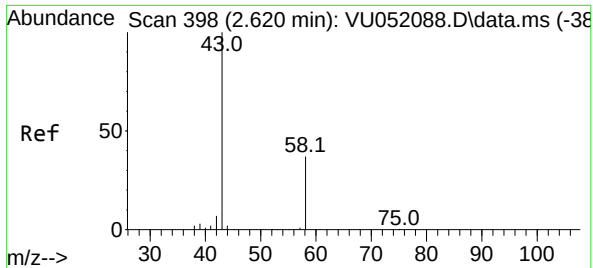

#13
 Acetone
 Concen: 3.552 ug/L
 RT: 2.636 min Scan# 40
 Delta R.T. 0.016 min
 Lab File: VU052104.D
 Acq: 23 Nov 2022 22:23

Instrument :
 MSVOA_U
 ClientSampleId :
 GBNK2

Tgt Ion: 43 Resp: 9299
 Ion Ratio Lower Upper
 43 100
 58 37.3 0.0 76.0

