

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112322\
 Data File : VU052107.D
 Acq On : 23 Nov 2022 23:45
 Operator : JC/MD
 Sample : N5759-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHB77

Quant Time: Nov 24 04:17:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Nov 24 04:13:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	214218	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	226134	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	87118	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	76277	3.661	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	73.200%
7) Chloroethane-d5	1.912	69	72460	4.477	ug/L	0.02
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.600%
11) 1,1-Dichloroethene-d2	2.568	65	30107	4.031	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	80.600%
20) 2-Butanone-d5	4.616	46	200307	53.034	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.060%
24) Chloroform-d	5.060	84	150685	4.922	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.400%
26) 1,2-Dichloroethane-d4	5.700	65	78270	5.061	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.200%
32) Benzene-d6	5.726	84	295650	4.404	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.000%
36) 1,2-Dichloropropane-d6	6.687	67	98297	4.731	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.600%
41) Toluene-d8	7.896	98	225874	3.719	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.400%
43) trans-1,3-Dichloroprop...	8.179	79	30726	4.058	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.200%
46) 2-Hexanone-d5	8.629	63	155405	48.434	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.860%
56) 1,1,2,2-Tetrachloroeth...	10.754	84	88520	4.914	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.200%
66) 1,2-Dichlorobenzene-d4	12.192	152	84247	5.051	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.000%
Target Compounds						
					Qvalue	
13) Acetone	2.623	43	8479	3.306	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112322\
Data File : VU052107.D
Acq On : 23 Nov 2022 23:45
Operator : JC/MD
Sample : N5759-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHB77

Quant Time: Nov 24 04:17:25 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Nov 24 04:13:15 2022
Response via : Initial Calibration

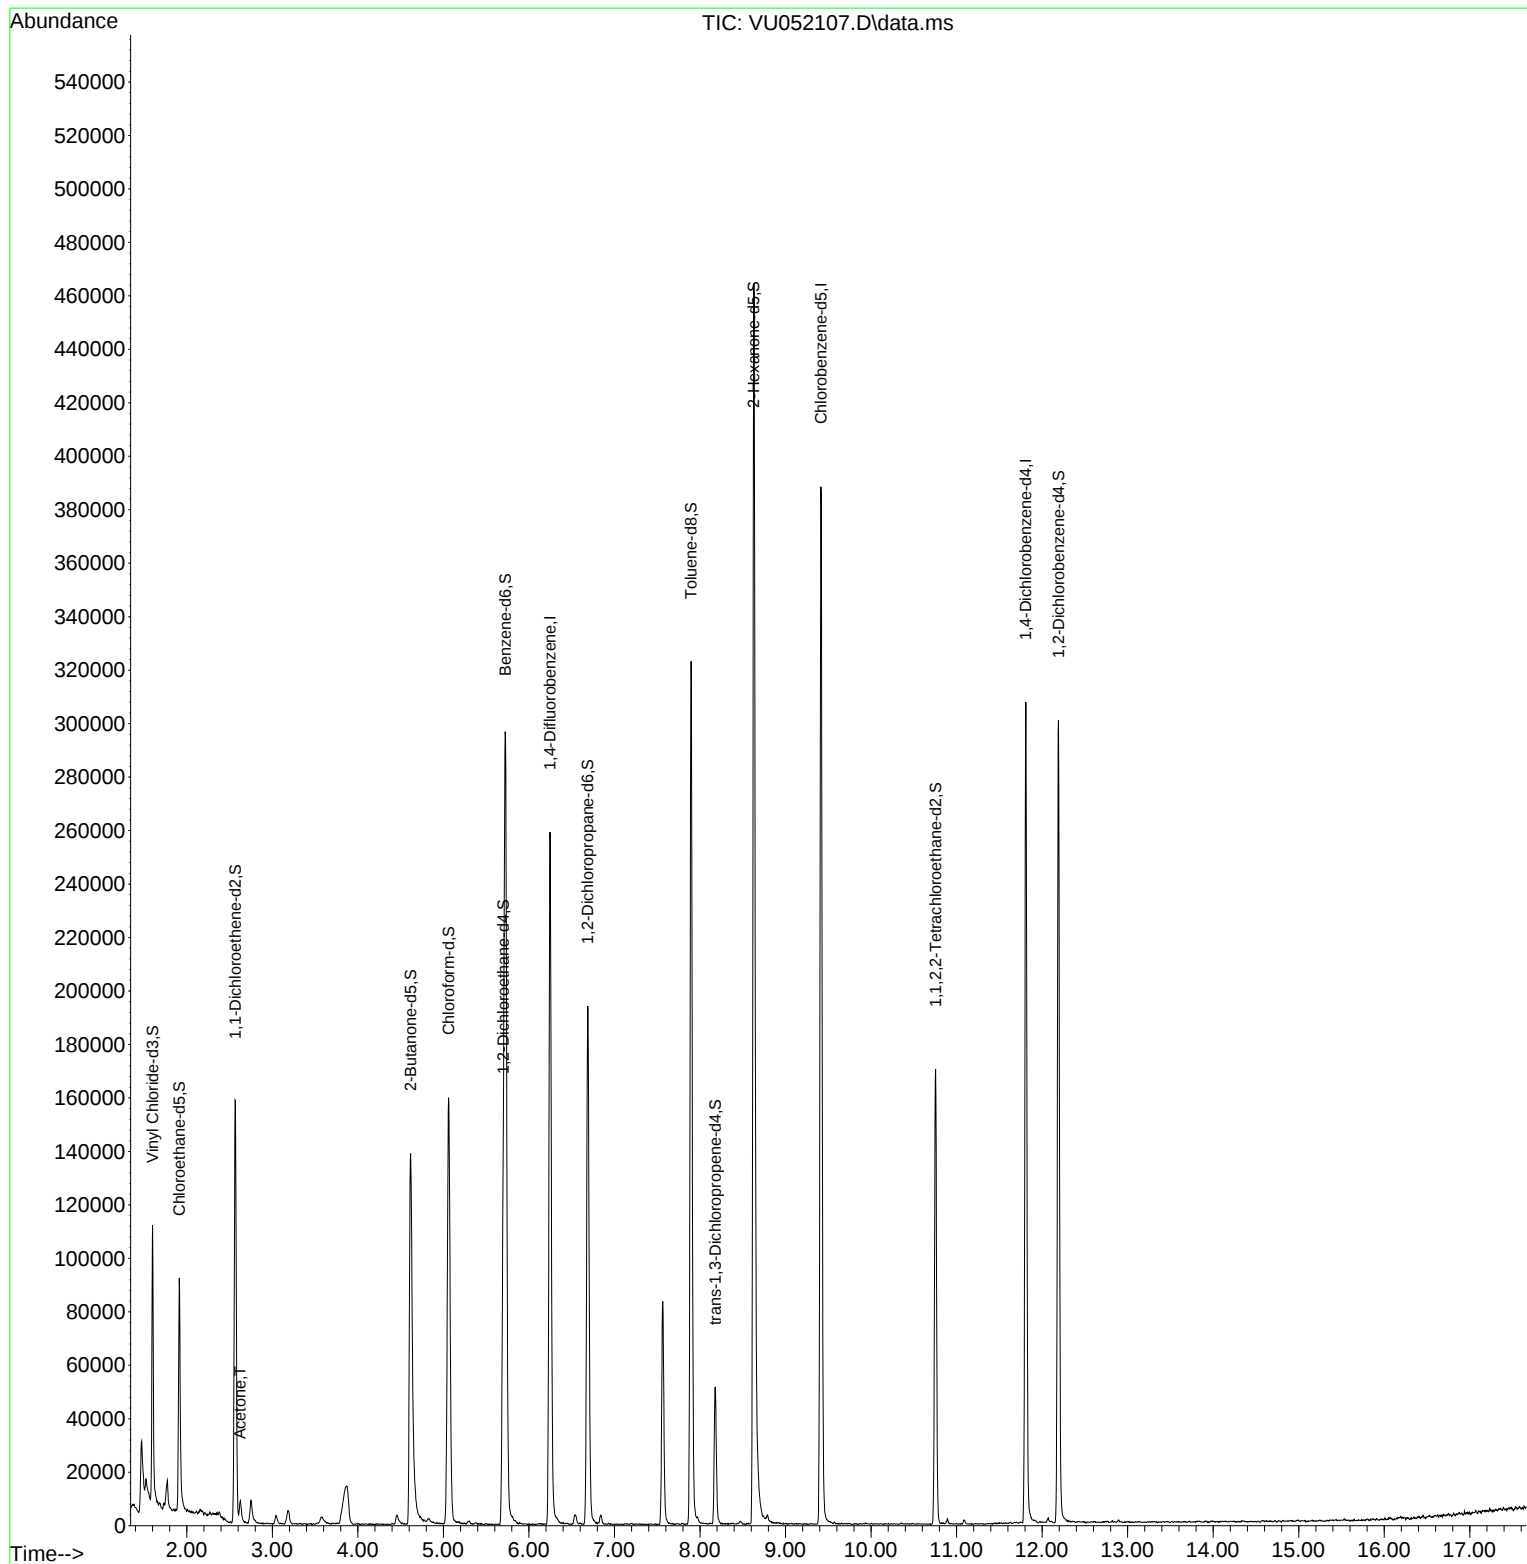

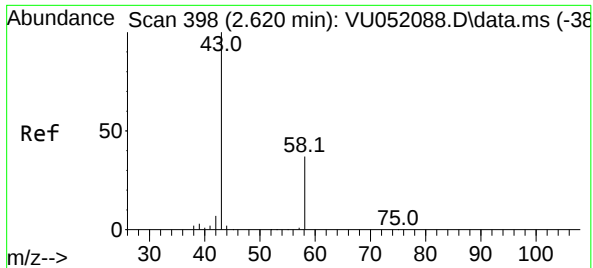

#13
 Acetone
 Concen: 3.306 ug/L
 RT: 2.623 min Scan# 398
 Delta R.T. 0.003 min
 Lab File: VU052107.D
 Acq: 23 Nov 2022 23:45

Instrument :
 MSVOA_U
 ClientSampleId :
 BHB77

Tgt Ion: 43 Resp: 8479
 Ion Ratio Lower Upper
 43 100
 58 38.2 0.0 76.0

