

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU112322\  
 Data File : VU052111.D  
 Acq On : 24 Nov 2022 02:02  
 Operator : JC/MD  
 Sample : N5739-04  
 Misc : 25.0mL/MSVOA\_U/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 VHBLK001

Quant Time: Nov 24 07:00:39 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR111822WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Thu Nov 24 05:20:45 2022  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon  | Response | Conc     | Units  | Dev(Min) |
|-------------------------------|--------|-------|----------|----------|--------|----------|
| -----                         |        |       |          |          |        |          |
| Internal Standards            |        |       |          |          |        |          |
| 1) 1,4-Difluorobenzene        | 6.247  | 114   | 205448   | 5.000    | ug/L   | 0.00     |
| 28) Chlorobenzene-d5          | 9.417  | 117   | 212056   | 5.000    | ug/L   | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.809 | 152   | 80104    | 5.000    | ug/L   | 0.00     |
|                               |        |       |          |          |        |          |
| System Monitoring Compounds   |        |       |          |          |        |          |
| 4) Vinyl Chloride-d3          | 1.597  | 65    | 72480    | 3.627    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 40 - 130 | Recovery | =      | 72.600%  |
| 7) Chloroethane-d5            | 1.912  | 69    | 68513    | 4.414    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 130 | Recovery | =      | 88.200%  |
| 11) 1,1-Dichloroethene-d2     | 2.568  | 65    | 28403    | 3.965    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 125 | Recovery | =      | 79.400%  |
| 20) 2-Butanone-d5             | 4.616  | 46    | 206021   | 56.875   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 40 - 130 | Recovery | =      | 113.740% |
| 24) Chloroform-d              | 5.063  | 84    | 150499   | 5.125    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =      | 102.600% |
| 26) 1,2-Dichloroethane-d4     | 5.700  | 65    | 77014    | 5.193    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =      | 103.800% |
| 32) Benzene-d6                | 5.726  | 84    | 292085   | 4.640    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =      | 92.800%  |
| 36) 1,2-Dichloropropane-d6    | 6.687  | 67    | 98779    | 5.070    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 140 | Recovery | =      | 101.400% |
| 41) Toluene-d8                | 7.896  | 98    | 220734   | 3.875    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =      | 77.600%  |
| 43) trans-1,3-Dichloroprop... | 8.179  | 79    | 29397    | 4.141    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 55 - 130 | Recovery | =      | 82.800%  |
| 46) 2-Hexanone-d5             | 8.629  | 63    | 160426   | 53.318   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 45 - 130 | Recovery | =      | 106.640% |
| 56) 1,1,2,2-Tetrachloroeth... | 10.754 | 84    | 88976    | 5.267    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 120 | Recovery | =      | 105.400% |
| 66) 1,2-Dichlorobenzene-d4    | 12.192 | 152   | 82429    | 5.375    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 80 - 120 | Recovery | =      | 107.400% |
|                               |        |       |          |          |        |          |
| Target Compounds              |        |       |          |          | Qvalue |          |
| 13) Acetone                   | 2.629  | 43    | 7987     | 3.247    | ug/L   | 96       |
| -----                         |        |       |          |          |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU112322\  
Data File : VU052111.D  
Acq On : 24 Nov 2022 02:02  
Operator : JC/MD  
Sample : N5739-04  
Misc : 25.0mL/MSVOA\_U/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
VHBLK001

Quant Time: Nov 24 07:00:39 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR111822WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Thu Nov 24 05:20:45 2022  
Response via : Initial Calibration

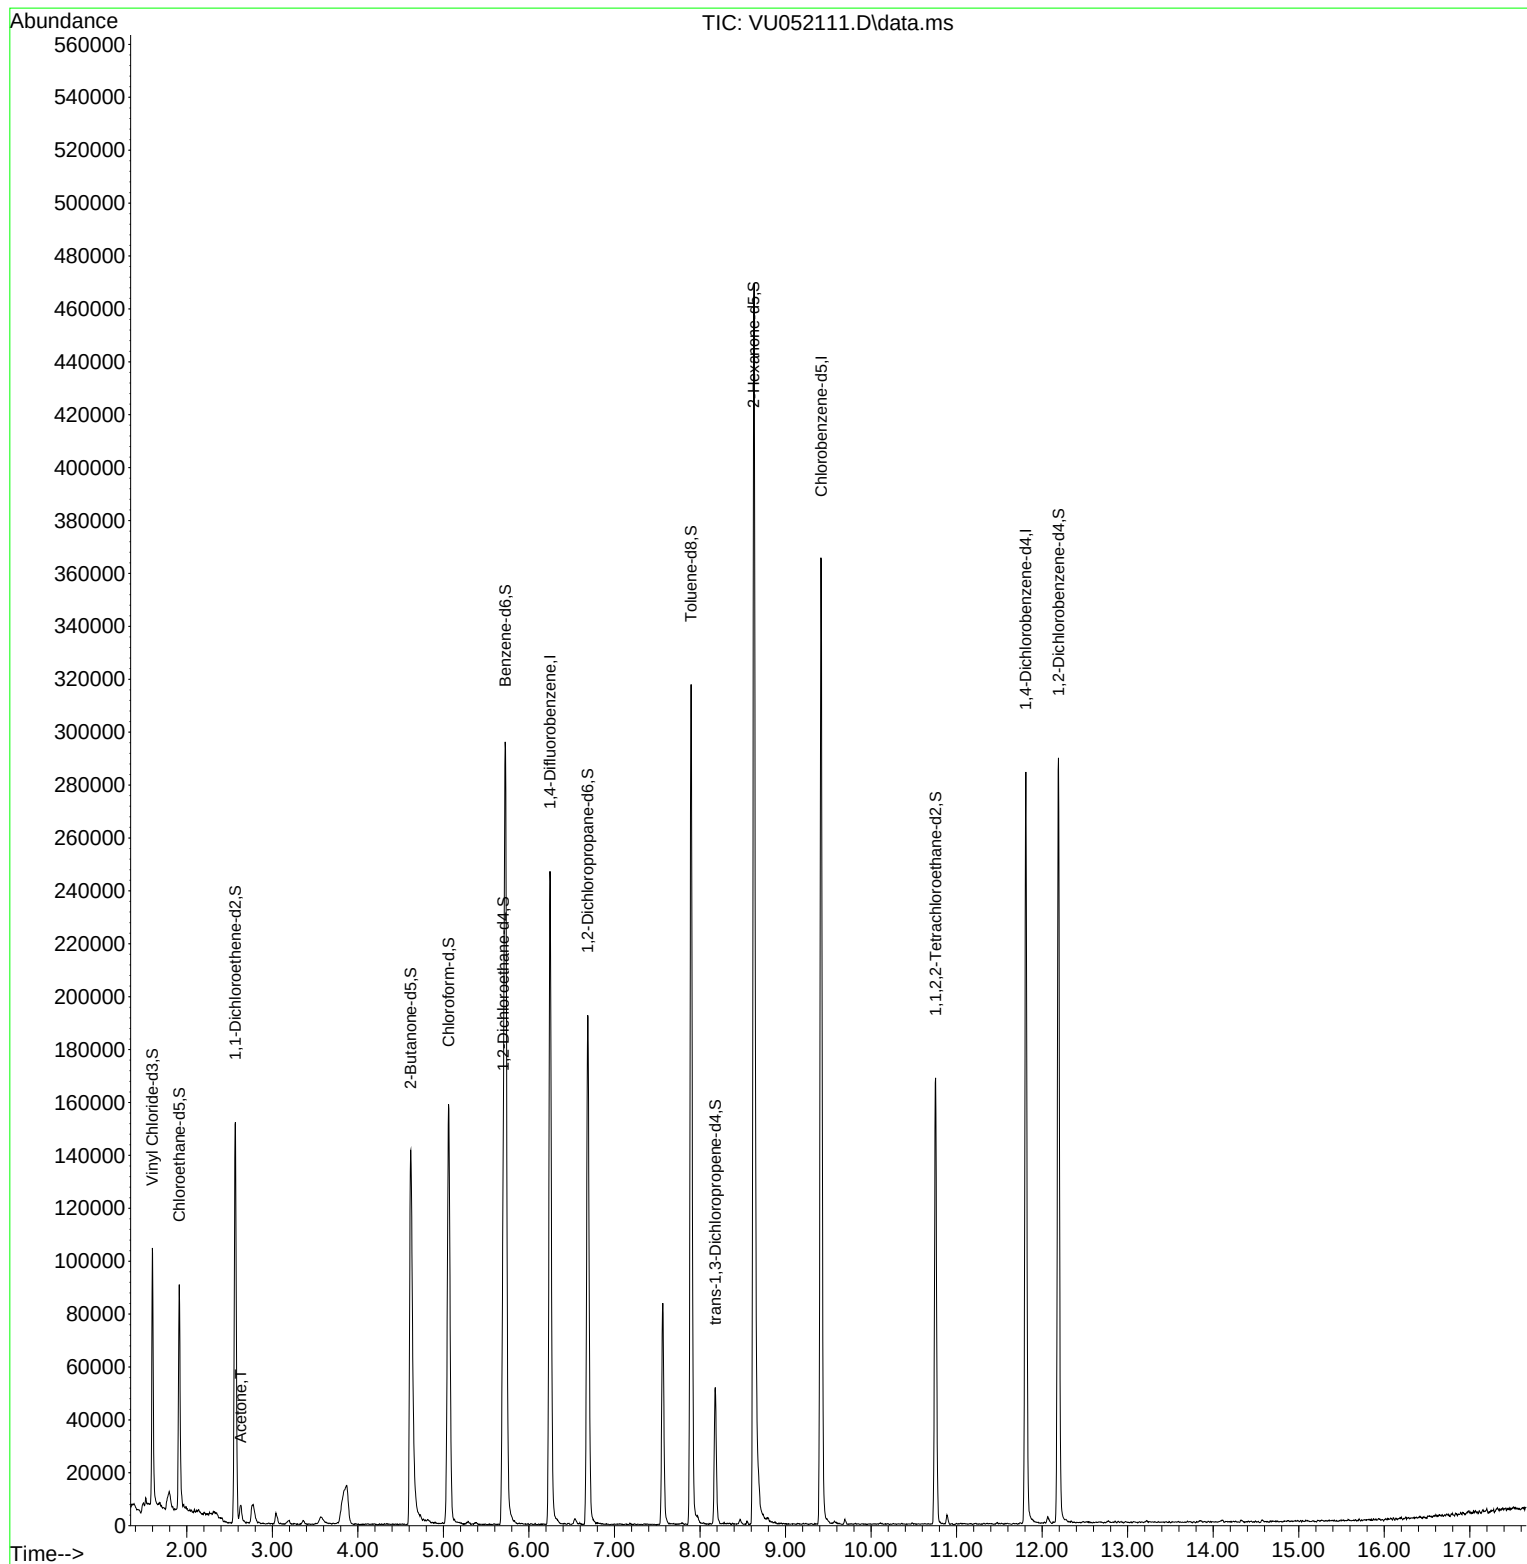

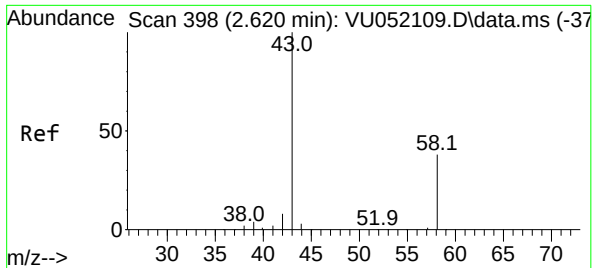

#13  
 Acetone  
 Concen: 3.247 ug/L  
 RT: 2.629 min Scan# 401  
 Delta R.T. 0.010 min  
 Lab File: VU052111.D  
 Acq: 24 Nov 2022 02:02

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 VHBLK001

Tgt Ion: 43 Resp: 7987  
 Ion Ratio Lower Upper  
 43 100  
 58 40.5 0.0 76.0

