

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112322\
 Data File : VU052118.D
 Acq On : 24 Nov 2022 05:14
 Operator : JC/MD
 Sample : N5770-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH1G1

Quant Time: Nov 24 07:02:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Nov 24 05:20:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	216156	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	224416	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	79755	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	77015	3.663	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	73.200%
7) Chloroethane-d5	1.913	69	72048	4.412	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.200%
11) 1,1-Dichloroethene-d2	2.565	65	30036	3.985	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	79.800%
20) 2-Butanone-d5	4.617	46	210309	55.183	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	110.360%
24) Chloroform-d	5.064	84	152637	4.941	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.800%
26) 1,2-Dichloroethane-d4	5.700	65	78980	5.061	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.200%
32) Benzene-d6	5.726	84	304824	4.575	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.600%
36) 1,2-Dichloropropane-d6	6.687	67	101580	4.927	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.600%
41) Toluene-d8	7.896	98	228775	3.795	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	76.000%
43) trans-1,3-Dichloroprop...	8.176	79	31746	4.225	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.600%
46) 2-Hexanone-d5	8.629	63	161654	50.767	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.540%
56) 1,1,2,2-Tetrachloroeth...	10.751	84	88793	4.967	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.400%
66) 1,2-Dichlorobenzene-d4	12.192	152	80678	5.284	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.600%
Target Compounds					Qvalue	
13) Acetone	2.623	43	18470	7.137	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112322\
Data File : VU052118.D
Acq On : 24 Nov 2022 05:14
Operator : JC/MD
Sample : N5770-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH1G1

Quant Time: Nov 24 07:02:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Nov 24 05:20:45 2022
Response via : Initial Calibration

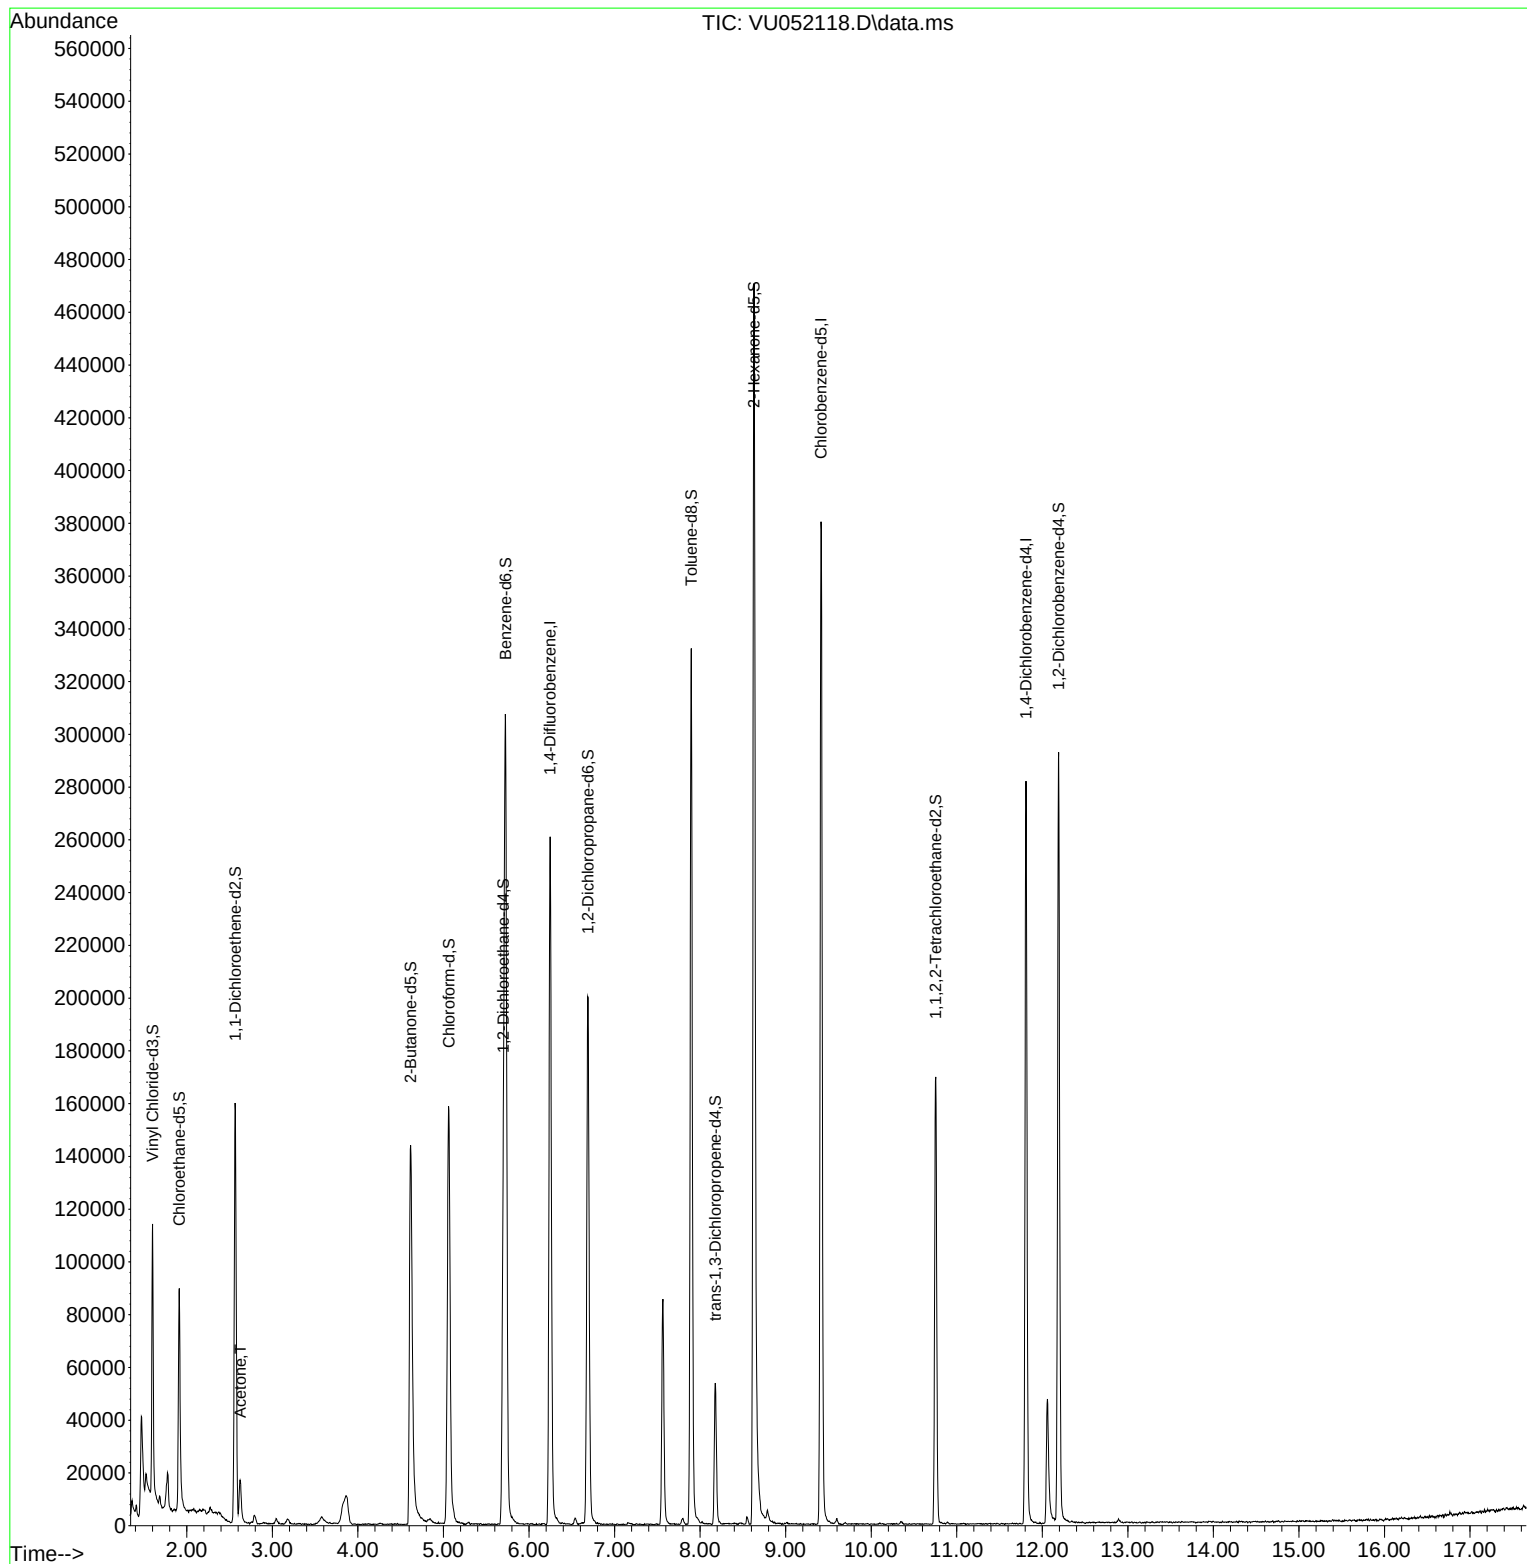

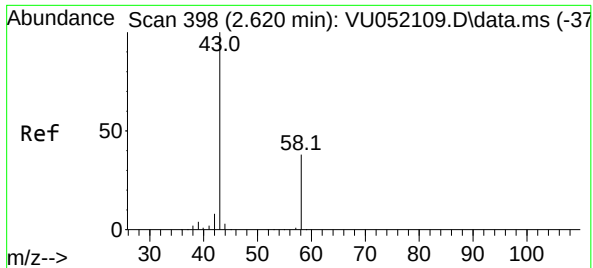

#13

Acetone

Concen: 7.137 ug/L

RT: 2.623 min Scan# 398

Delta R.T. 0.003 min

Lab File: VU052118.D


Acq: 24 Nov 2022 05:14

Instrument :

MSVOA_U

ClientSampleId :

BH1G1

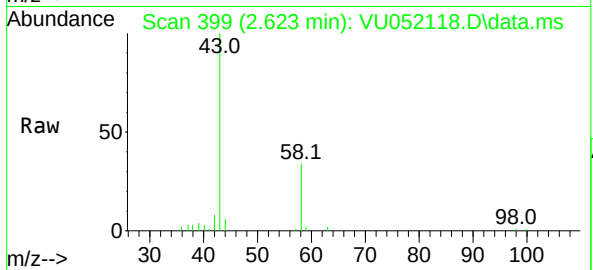

Tgt Ion: 43 Resp: 18470

Ion Ratio Lower Upper

43 100

58 35.5 0.0 76.0

