

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112322\
 Data File : VU052122.D
 Acq On : 24 Nov 2022 07:03
 Operator : JC/MD
 Sample : N5770-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH1N0

Quant Time: Nov 24 07:30:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Nov 24 05:20:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	209900	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	221904	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	85173	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	72402	3.546	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	71.000%
7) Chloroethane-d5	1.912	69	71422	4.504	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.000%
11) 1,1-Dichloroethene-d2	2.565	65	28718	3.924	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	78.400%
20) 2-Butanone-d5	4.616	46	204928	55.373	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	110.740%
24) Chloroform-d	5.060	84	149972	4.999	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.000%
26) 1,2-Dichloroethane-d4	5.700	65	77361	5.105	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.200%
32) Benzene-d6	5.726	84	296001	4.493	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.800%
36) 1,2-Dichloropropane-d6	6.690	67	99482	4.879	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.600%
41) Toluene-d8	7.896	98	223473	3.749	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	75.000%
43) trans-1,3-Dichloroprop...	8.179	79	30189	4.063	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.200%
46) 2-Hexanone-d5	8.629	63	160018	50.822	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.640%
56) 1,1,2,2-Tetrachloroeth...	10.754	84	89958	5.089	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.800%
66) 1,2-Dichlorobenzene-d4	12.192	152	88166	5.407	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.200%
Target Compounds					Qvalue	
13) Acetone	2.620	43	45778	18.216	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112322\
Data File : VU052122.D
Acq On : 24 Nov 2022 07:03
Operator : JC/MD
Sample : N5770-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH1N0

Quant Time: Nov 24 07:30:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Nov 24 05:20:45 2022
Response via : Initial Calibration

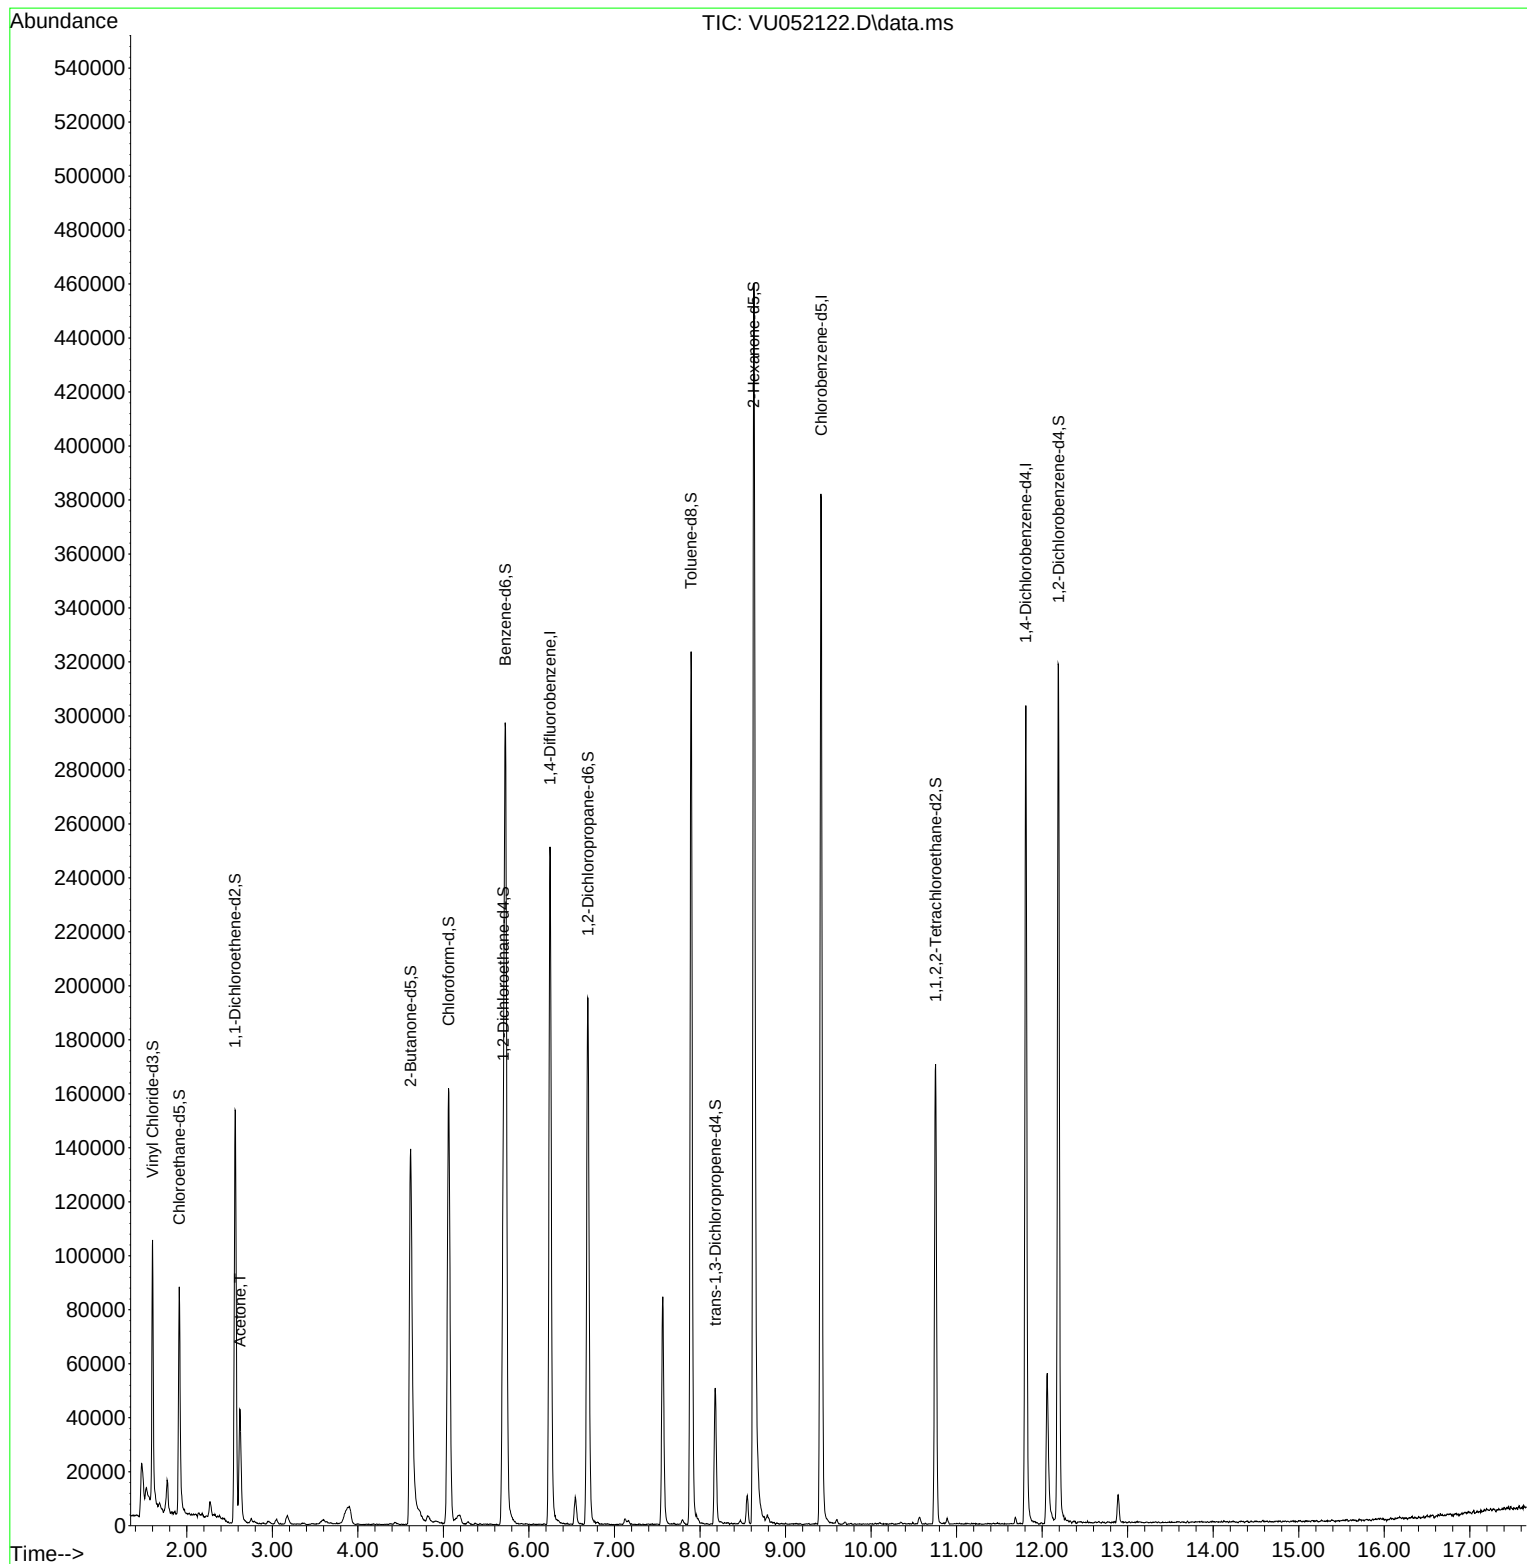

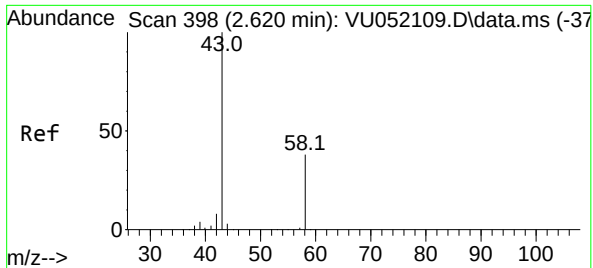

#13
 Acetone
 Concen: 18.216 ug/L
 RT: 2.620 min Scan# 398
 Delta R.T. -0.000 min
 Lab File: VU052122.D
 Acq: 24 Nov 2022 07:03

Instrument :
 MSVOA_U
 ClientSampleId :
 BH1N0

Tgt Ion: 43 Resp: 45778
 Ion Ratio Lower Upper
 43 100
 58 39.1 0.0 76.0

